

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037528.D
 Acq On : 25 Sep 2024 16:39
 Operator : SY/MD
 Sample : P4162-13
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 26 04:14:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 26 04:08:51 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	612013	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	600826	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	283878	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	193941	34.642	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	69.280%		
7) Chloroethane-d5	1.532	69	170935	39.506	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	79.020%		
11) 1,1-Dichloroethene-d2	2.060	65	89031	37.837	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	75.680%		
21) 2-Butanone-d5	3.793	46	179487	82.789	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	82.790%		
24) Chloroform-d	4.243	84	406034	46.340	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.680%		
26) 1,2-Dichloroethane-d4	4.937	65	248954	45.118	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.240%		
32) Benzene-d6	4.953	84	793670	43.735	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.460%		
36) 1,2-Dichloropropane-d6	5.982	67	258087	45.406	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	90.820%		
41) Toluene-d8	7.236	98	681732	41.625	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	83.240%		
43) trans-1,3-Dichloroprop...	7.551	79	107042	40.706	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	81.420%		
47) 2-Hexanone-d5	8.024	63	112978	72.830	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	72.830%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84	308186	44.706	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	89.420%		
66) 1,2-Dichlorobenzene-d4	11.554	152	274102	48.211	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.420%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.908	75	6516	0.888	ug/L #	50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037528.D
Acq On : 25 Sep 2024 16:39
Operator : SY/MD
Sample : P4162-13
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Sep 26 04:14:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 26 04:08:51 2024
Response via : Initial Calibration

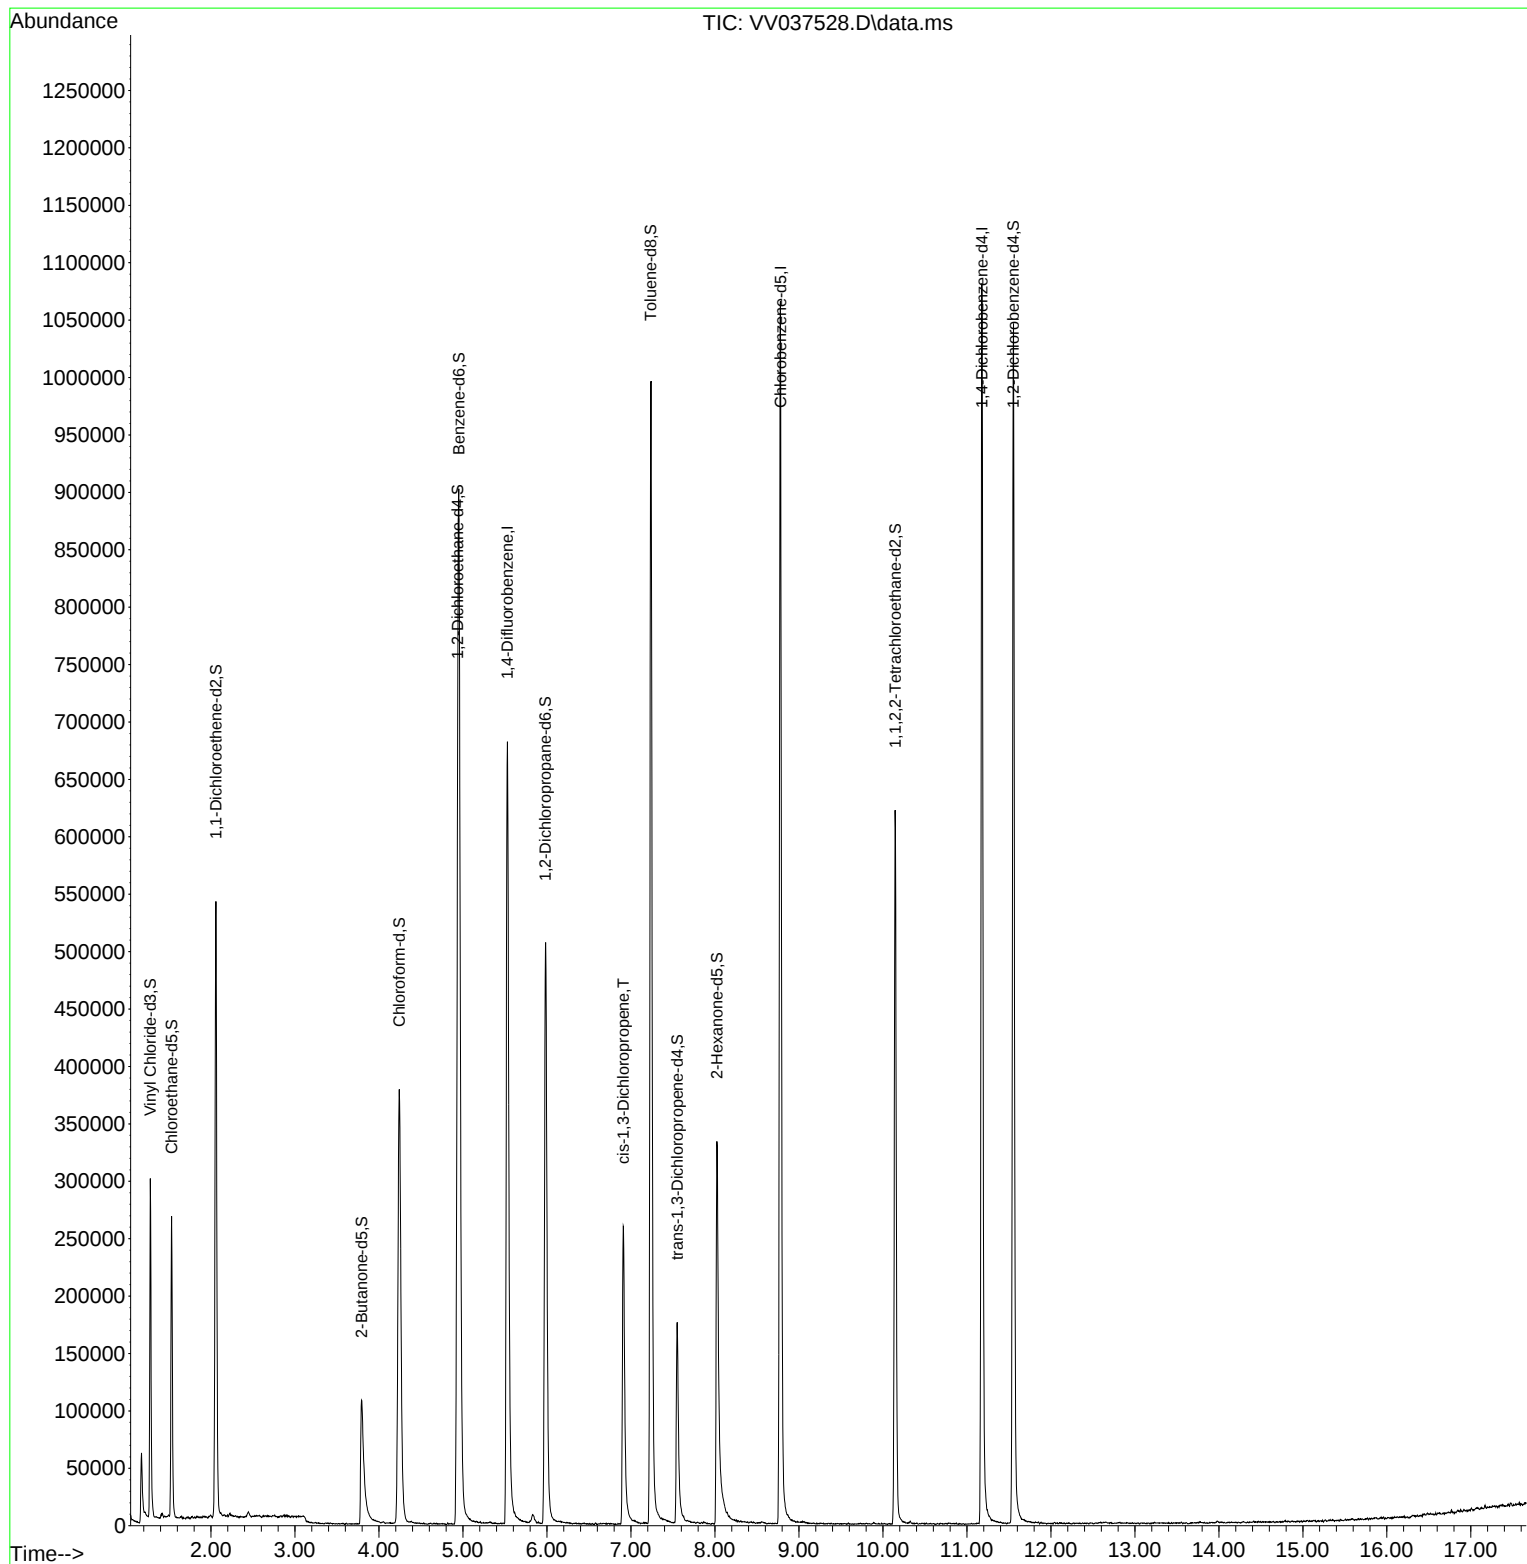

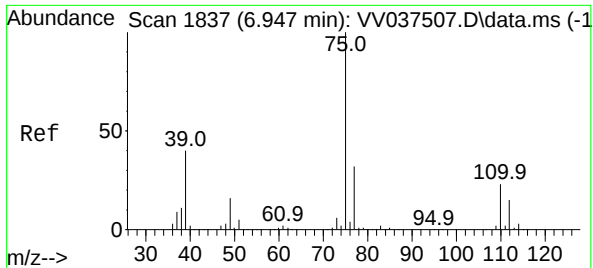

#39
 cis-1,3-Dichloropropene
 Concen: 0.888 ug/L
 RT: 6.908 min Scan# 11
 Delta R.T. -0.039 min
 Lab File: VV037528.D
 Acq: 25 Sep 2024 16:39

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 6516
 Ion Ratio Lower Upper
 75 100
 77 58.4 21.7 40.3#

