

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037512.D
 Acq On : 25 Sep 2024 10:45
 Operator : SY/MD
 Sample : P4109-14ME
 Misc : 5.05G/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4ET6ME

Quant Time: Sep 26 04:10:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 26 04:08:51 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.526	114	450330	50.000	ug/L	0.00
28) Chlorobenzene-d5		8.780	117	438088	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.178	152	217032	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.278	65	249506	60.568	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	121.140%	
7) Chloroethane-d5		1.503	69	93019	29.217	ug/L	-0.03
Spiked Amount	50.000	Range	70 - 130	Recovery	=	58.440%#	
11) 1,1-Dichloroethene-d2		2.047	65	116364	67.208	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	134.420%#	
21) 2-Butanone-d5		3.796	46	226007	141.675	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	141.670%#	
24) Chloroform-d		4.236	84	490330	76.052	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	152.100%#	
26) 1,2-Dichloroethane-d4		4.931	65	304483	74.993	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	149.980%#	
32) Benzene-d6		4.947	84	1001701	75.703	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	151.400%#	
36) 1,2-Dichloropropane-d6		5.982	67	318087	76.751	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	153.500%#	
41) Toluene-d8		7.236	98	879948	73.685	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	147.380%#	
43) trans-1,3-Dichloroprop...		7.548	79	142088	74.105	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	148.200%#	
47) 2-Hexanone-d5		8.024	63	154943	136.986	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	136.990%#	
56) 1,1,2,2-Tetrachloroeth...		10.146	84	363731	72.364	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	144.720%#	
66) 1,2-Dichlorobenzene-d4		11.551	152	353882	81.414	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	162.820%#	
Target Compounds							Qvalue
15) Methyl Acetate		2.371	43	43280	15.089	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037512.D
Acq On : 25 Sep 2024 10:45
Operator : SY/MD
Sample : P4109-14ME
Misc : 5.05G/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4ET6ME

Quant Time: Sep 26 04:10:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 26 04:08:51 2024
Response via : Initial Calibration

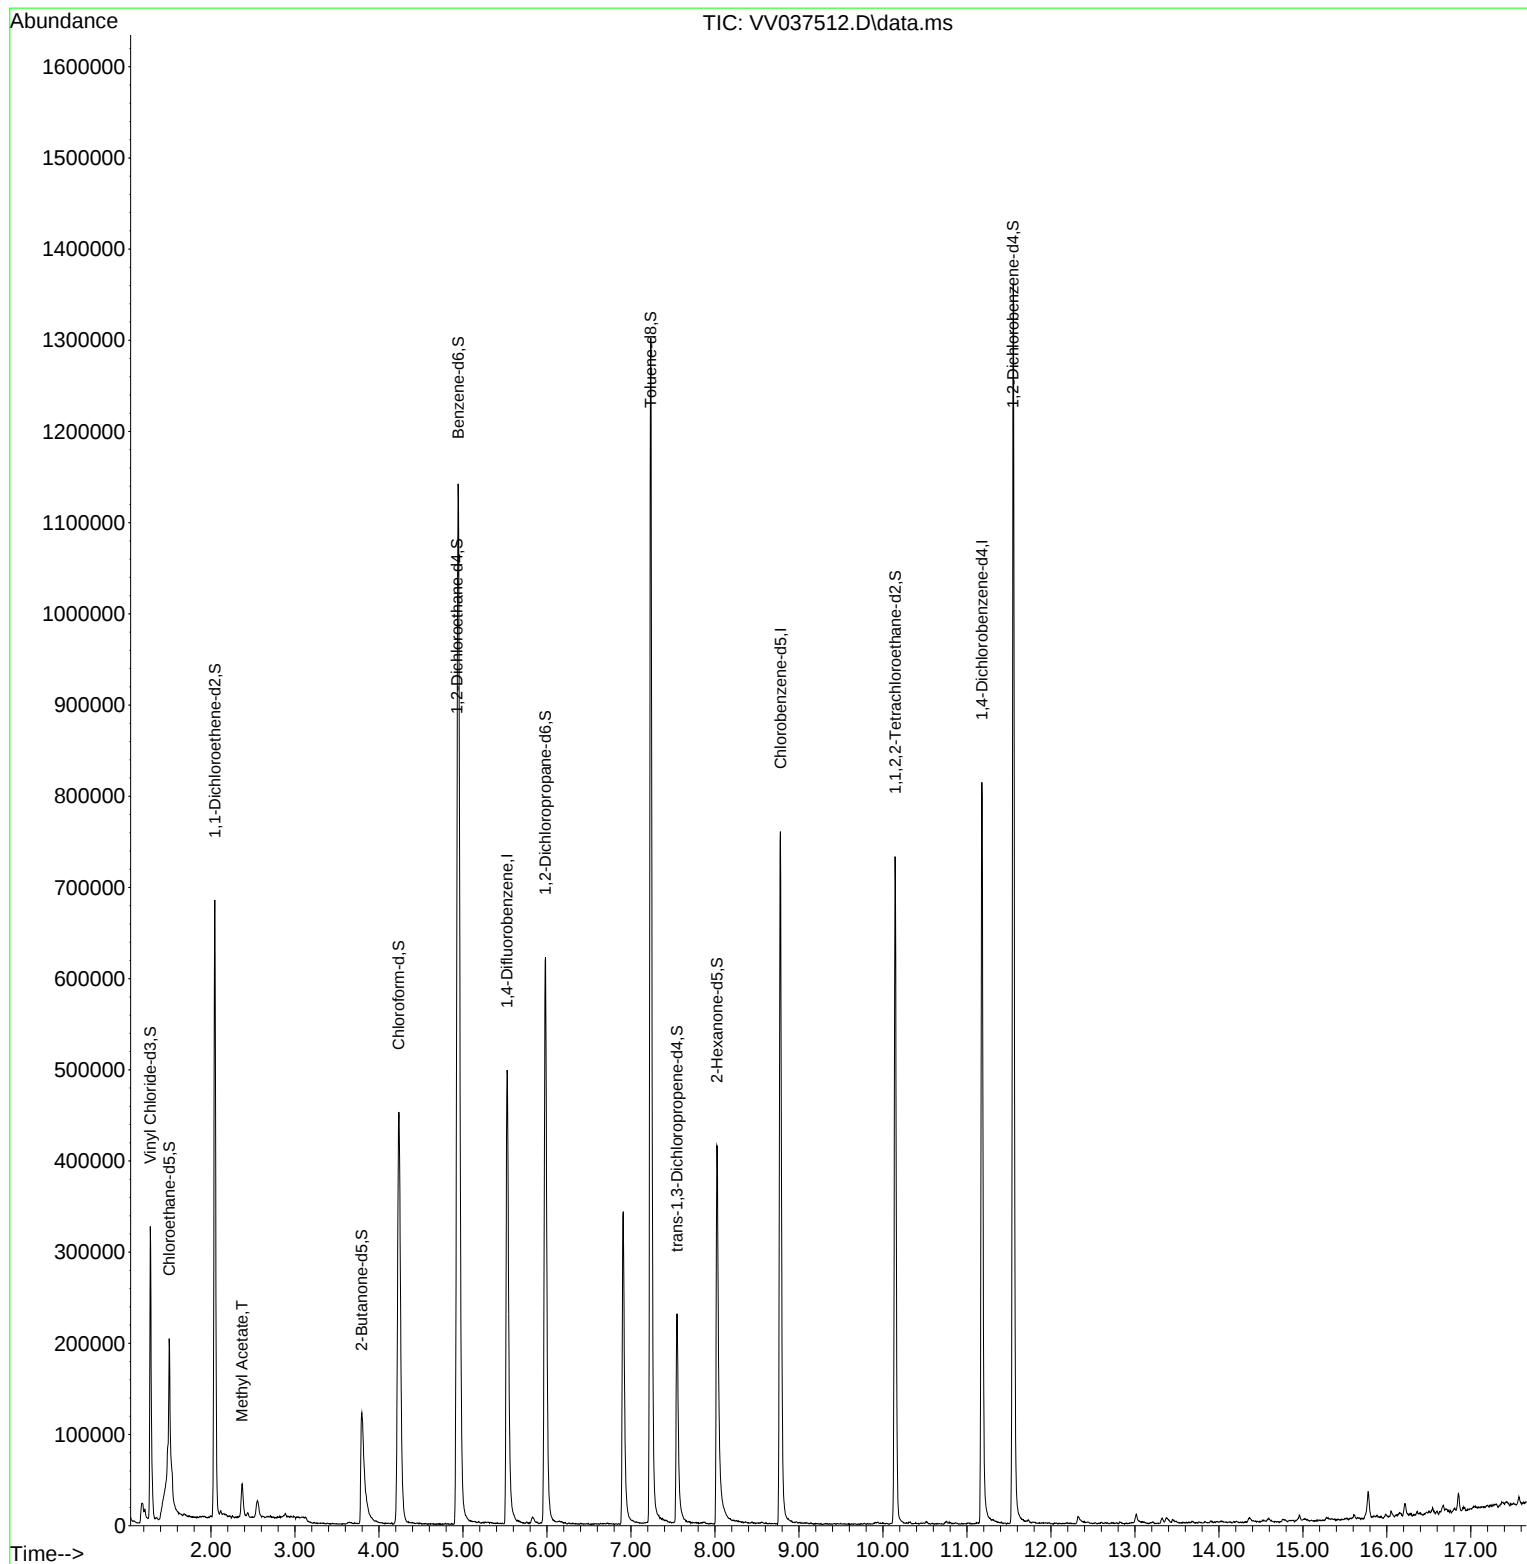

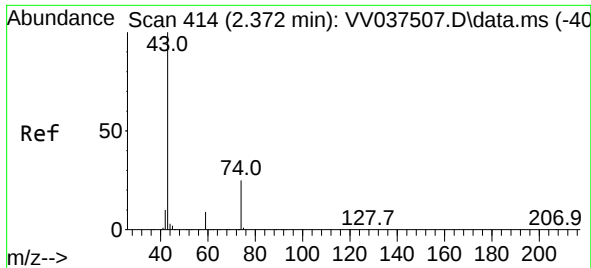

#15
Methyl Acetate
Concen: 15.089 ug/L
RT: 2.371 min Scan# 41
Delta R.T. -0.000 min
Lab File: VV037512.D
Acq: 25 Sep 2024 10:45

Instrument :
MSVOA_V
ClientSampleId :
A4ET6ME

Tgt Ion: 43 Resp: 43280
Ion Ratio Lower Upper
43 100
74 24.5 18.4 27.6

