

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037520.D
 Acq On : 25 Sep 2024 13:47
 Operator : SY/MD
 Sample : P4131-06
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4EB0

Quant Time: Sep 26 04:12:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 26 04:08:51 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	640727	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	615947	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	297668	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	212497	36.255	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	72.520%	
7) Chloroethane-d5	1.532	69	186202	41.106	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	82.220%	
11) 1,1-Dichloroethene-d2	2.060	65	96504	39.174	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	78.340%	
21) 2-Butanone-d5	3.796	46	190893	84.104	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	84.100%	
24) Chloroform-d	4.243	84	438359	47.787	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.580%	
26) 1,2-Dichloroethane-d4	4.937	65	270475	46.821	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	93.640%	
32) Benzene-d6	4.953	84	874596	47.011	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	94.020%	
36) 1,2-Dichloropropane-d6	5.982	67	279736	48.007	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	96.020%	
41) Toluene-d8	7.236	98	763267	45.459	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	90.920%	
43) trans-1,3-Dichloroprop...	7.548	79	122752	45.534	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	91.060%	
47) 2-Hexanone-d5	8.024	63	121490	76.394	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	76.390%	
56) 1,1,2,2-Tetrachloroeth...	10.146	84	315966	44.710	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	89.420%	
66) 1,2-Dichlorobenzene-d4	11.555	152	298625	50.091	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	100.180%	
Target Compounds						
13) Acetone	2.114	43	34685	14.249	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037520.D
Acq On : 25 Sep 2024 13:47
Operator : SY/MD
Sample : P4131-06
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4EB0

Quant Time: Sep 26 04:12:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 26 04:08:51 2024
Response via : Initial Calibration

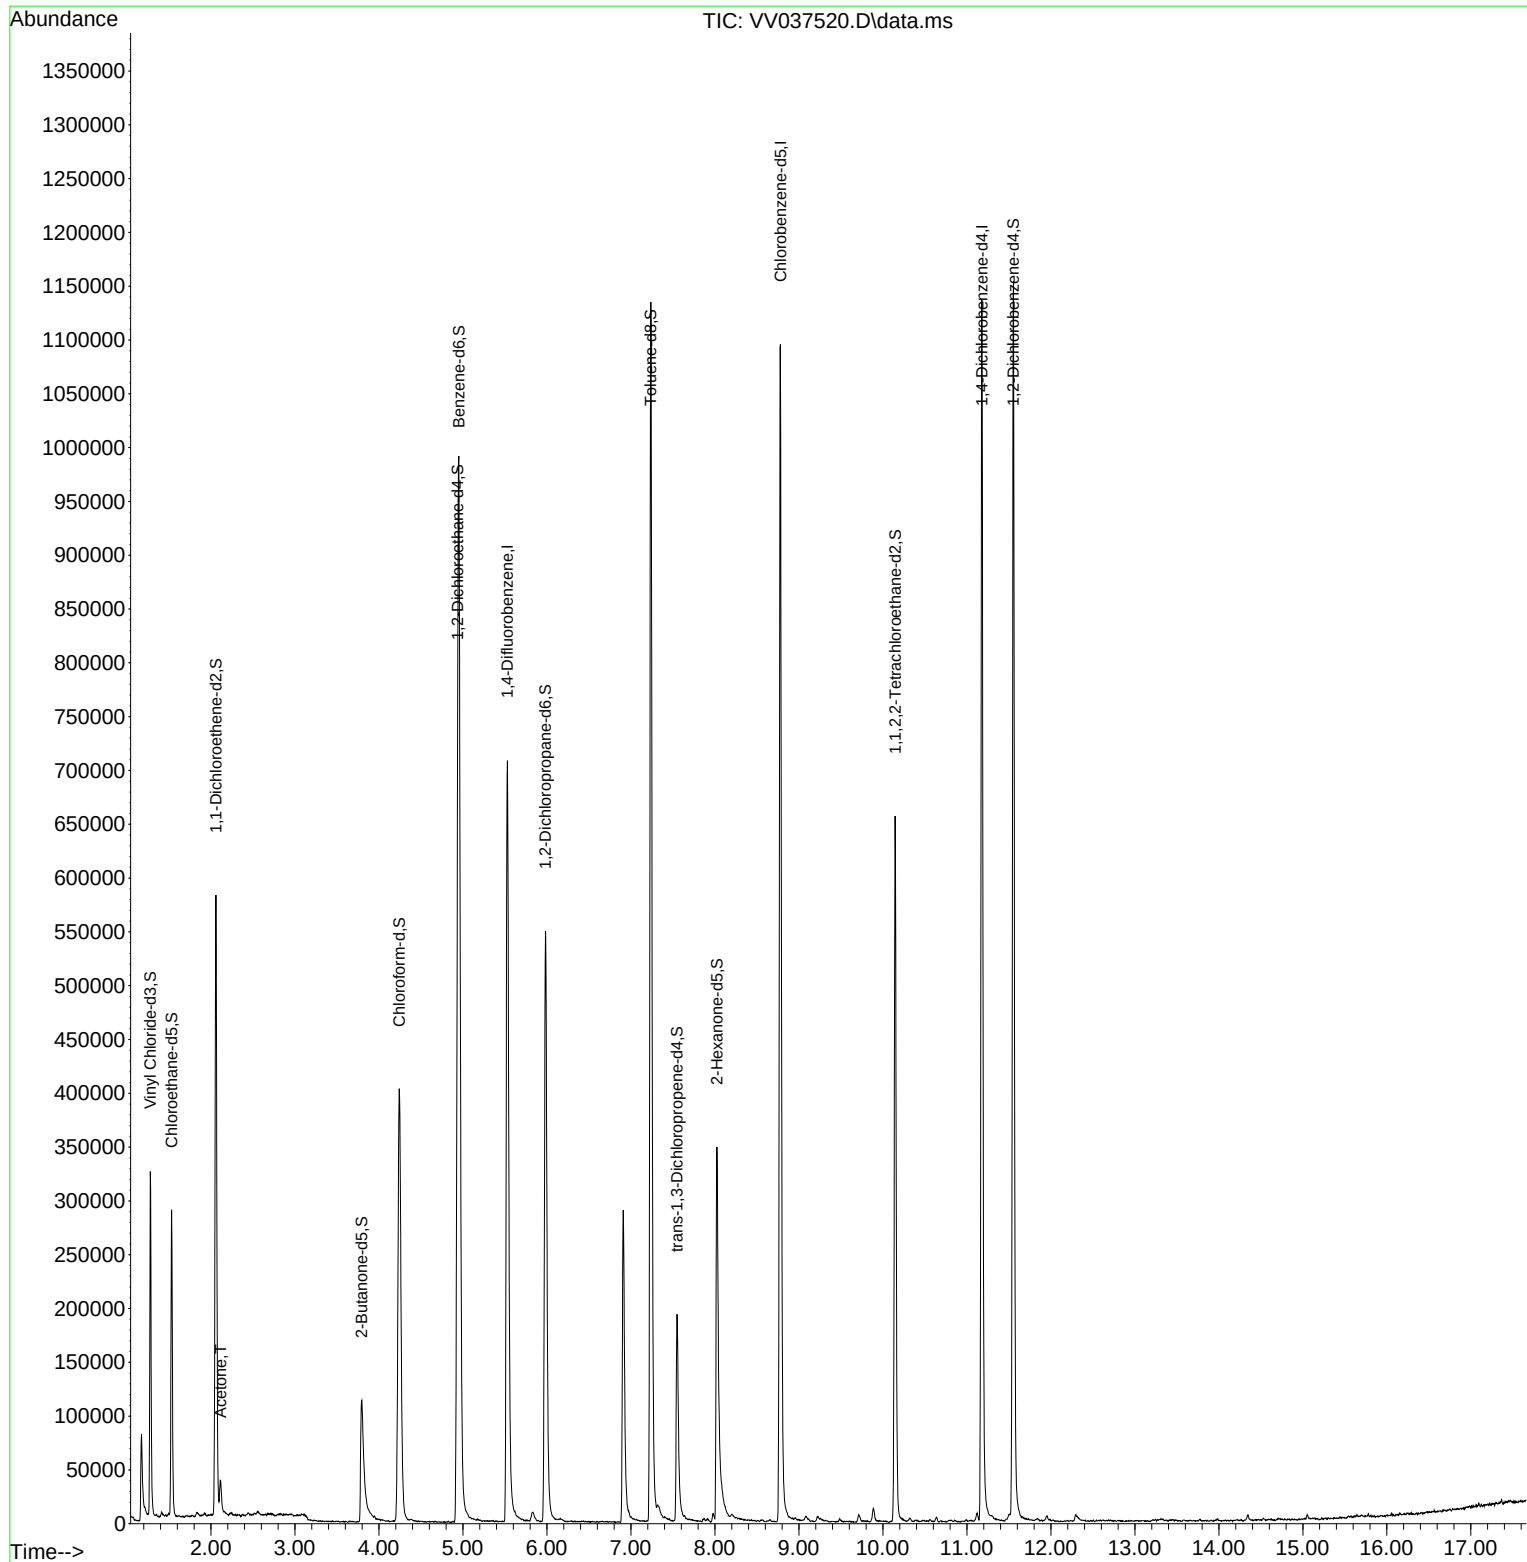

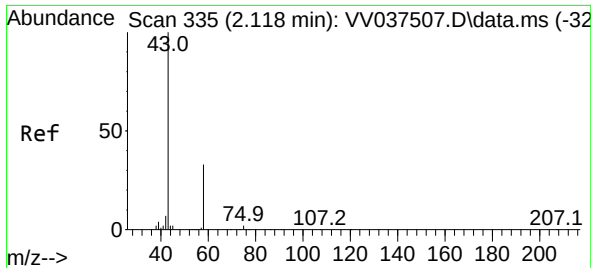

#13

Acetone

Concen: 14.249 ug/L

RT: 2.114 min Scan# 31

Delta R.T. -0.003 min

Lab File: VV037520.D


Acq: 25 Sep 2024 13:47

Instrument :

MSVOA_V

ClientSampleId :

A4EB0

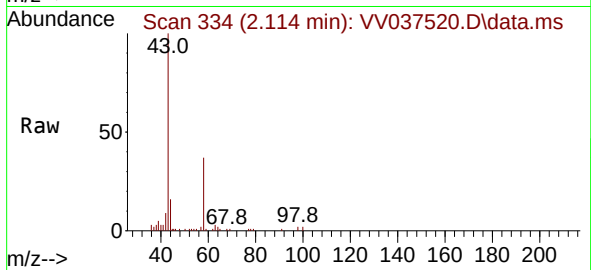

Tgt Ion: 43 Resp: 34685

Ion Ratio Lower Upper

43 100

58 35.6 0.0 64.8

