

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037521.D
 Acq On : 25 Sep 2024 14:08
 Operator : SY/MD
 Sample : P4131-19
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FC1

Quant Time: Sep 26 04:13:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 26 04:08:51 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	636347	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	615310	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	291227	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	207056	35.570	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	71.140%		
7) Chloroethane-d5	1.532	69	182481	40.562	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	81.120%		
11) 1,1-Dichloroethene-d2	2.060	65	92723	37.899	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	75.800%		
21) 2-Butanone-d5	3.793	46	192435	85.367	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	85.370%		
24) Chloroform-d	4.243	84	428340	47.016	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.040%		
26) 1,2-Dichloroethane-d4	4.937	65	264795	46.153	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.300%		
32) Benzene-d6	4.953	84	852040	45.846	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.700%		
36) 1,2-Dichloropropane-d6	5.982	67	275937	47.404	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	94.800%		
41) Toluene-d8	7.236	98	743070	44.302	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.600%		
43) trans-1,3-Dichloroprop...	7.548	79	119684	44.442	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	88.880%		
47) 2-Hexanone-d5	8.024	63	122433	77.067	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	77.070%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84	314648	44.569	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	89.140%		
66) 1,2-Dichlorobenzene-d4	11.554	152	291348	49.951	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	99.900%		
Target Compounds					Qvalue	
13) Acetone	2.114	43	27224	11.261	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037521.D
Acq On : 25 Sep 2024 14:08
Operator : SY/MD
Sample : P4131-19
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FC1

Quant Time: Sep 26 04:13:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 26 04:08:51 2024
Response via : Initial Calibration

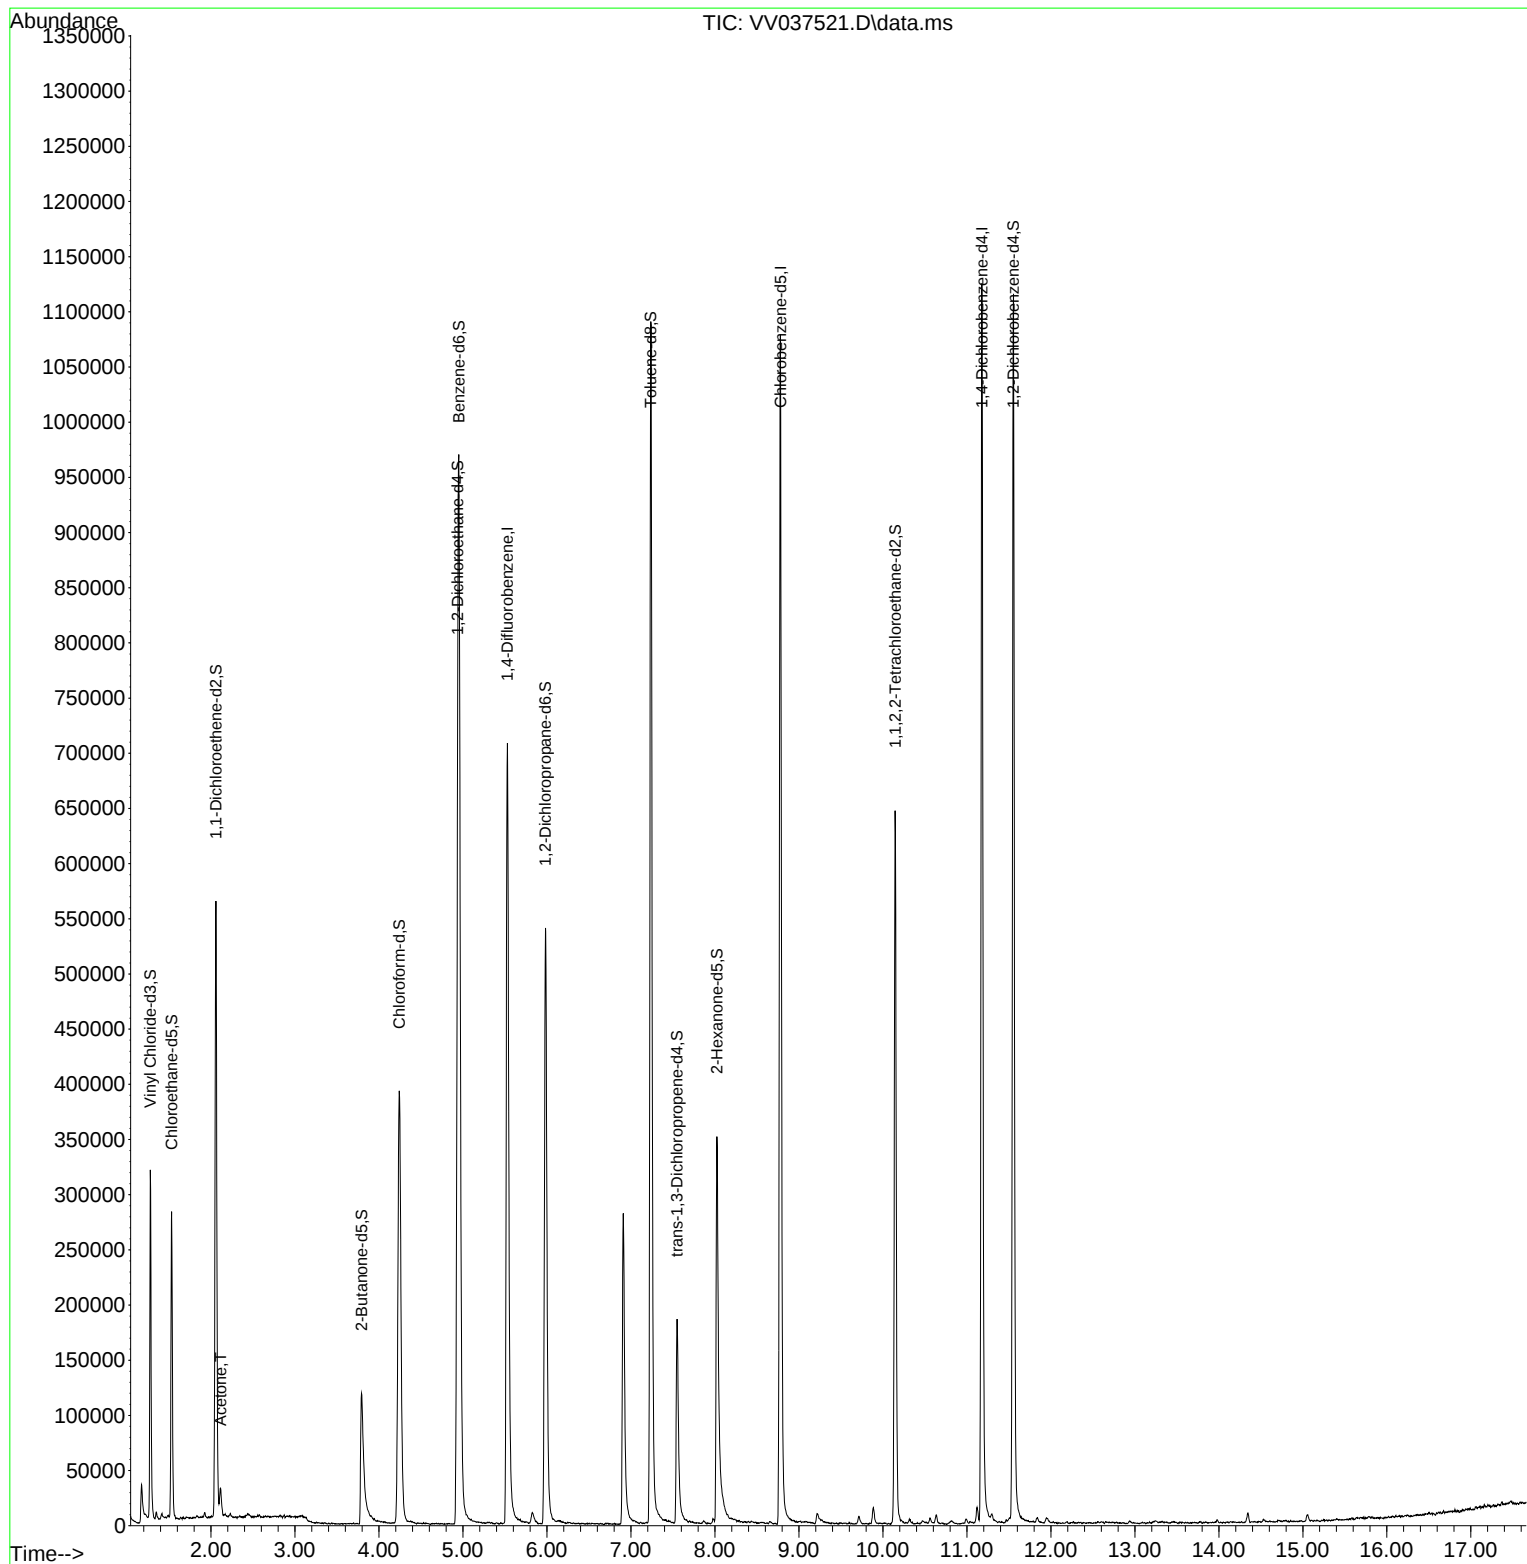

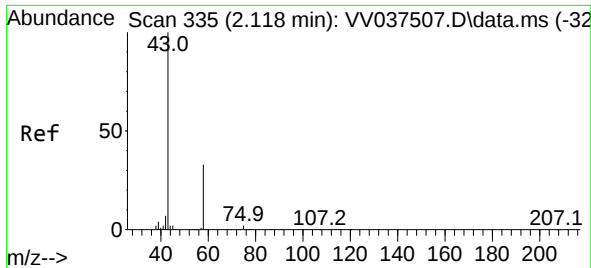

#13

Acetone

Concen: 11.261 ug/L

RT: 2.114 min Scan# 31

Delta R.T. -0.003 min

Lab File: VV037521.D


Acq: 25 Sep 2024 14:08

Instrument :

MSVOA_V

ClientSampleId :

A4FC1

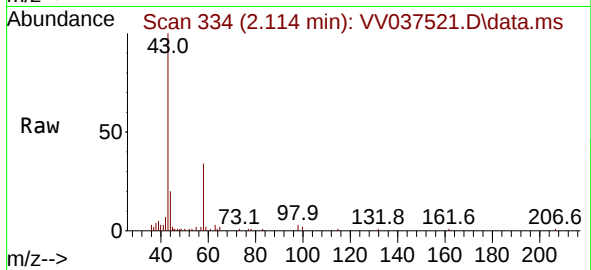

Tgt Ion: 43 Resp: 27224

Ion Ratio Lower Upper

43 100

58 36.4 0.0 64.8

