

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037522.D
 Acq On : 25 Sep 2024 14:30
 Operator : SY/MD
 Sample : P4162-11
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FC2

Quant Time: Sep 26 04:13:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 26 04:08:51 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	633297	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	604289	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	293758	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	211660	36.536	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	73.080%
7) Chloroethane-d5	1.532	69	183607	41.008	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	82.020%
11) 1,1-Dichloroethene-d2	2.060	65	97515	40.049	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.100%
21) 2-Butanone-d5	3.793	46	190691	85.001	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	85.000%
24) Chloroform-d	4.243	84	436731	48.168	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.340%
26) 1,2-Dichloroethane-d4	4.937	65	266932	46.750	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.500%
32) Benzene-d6	4.953	84	874762	47.927	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.860%
36) 1,2-Dichloropropane-d6	5.985	67	278907	48.788	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.580%
41) Toluene-d8	7.236	98	758597	46.052	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.100%
43) trans-1,3-Dichloroprop...	7.551	79	118000	44.616	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.240%
47) 2-Hexanone-d5	8.024	63	129831	83.214	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	83.210%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	321068	46.308	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.620%
66) 1,2-Dichlorobenzene-d4	11.554	152	299230	50.860	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.720%
Target Compounds						
13) Acetone	2.114	43	25021	10.399	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037522.D
Acq On : 25 Sep 2024 14:30
Operator : SY/MD
Sample : P4162-11
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FC2

Quant Time: Sep 26 04:13:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 26 04:08:51 2024
Response via : Initial Calibration

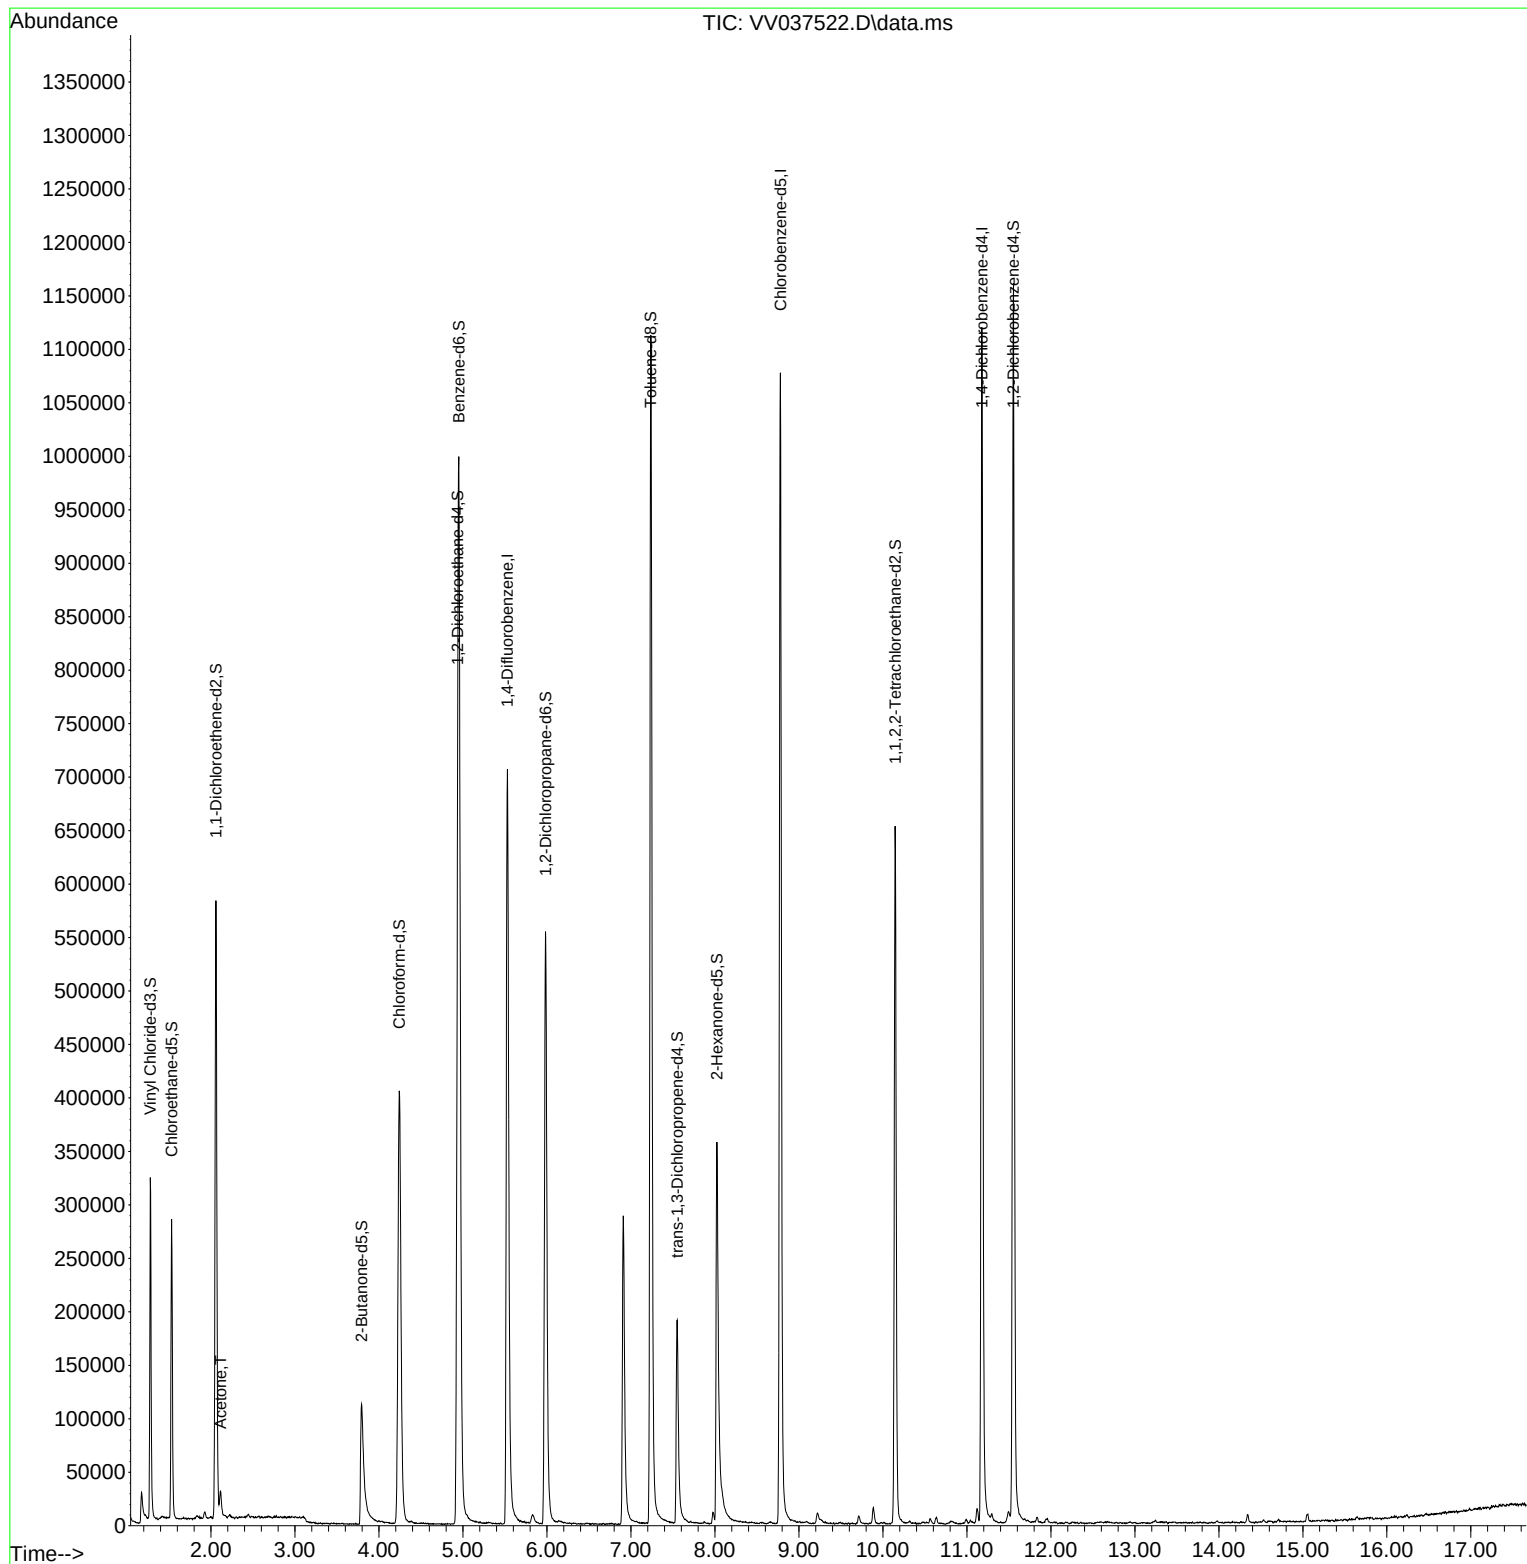

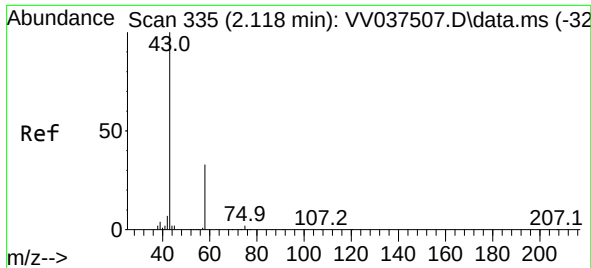

#13

Acetone

Concen: 10.399 ug/L

RT: 2.114 min Scan# 31

Delta R.T. -0.003 min

Lab File: VV037522.D


Acq: 25 Sep 2024 14:30

Instrument :

MSVOA_V

ClientSampleId :

A4FC2

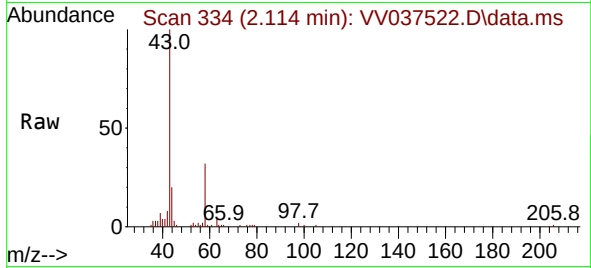

Tgt Ion: 43 Resp: 25021

Ion Ratio Lower Upper

43 100

58 34.7 0.0 64.8

