

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037517.D
 Acq On : 25 Sep 2024 12:42
 Operator : SY/MD
 Sample : VIBLK388
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK388

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037517.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	35	41	51	rBV	33842	51796	2.01%	0.269%
2	1.278	67	74	90	rVB	339163	359690	13.94%	1.868%
3	1.532	145	153	170	rVB	288532	348479	13.51%	1.810%
4	2.056	306	316	333	rBV	594772	865326	33.54%	4.495%
5	3.355	717	720	724	rVB3	842	575	0.02%	0.003%
6	3.468	752	755	758	rVB2	1327	871	0.03%	0.005%
7	3.494	758	763	764	rBV2	869	707	0.03%	0.004%
8	3.516	767	770	773	rBV2	899	706	0.03%	0.004%
9	3.587	789	792	796	rBV6	1002	802	0.03%	0.004%
10	3.719	831	833	837	rVB2	824	443	0.02%	0.002%
11	3.789	846	855	901	rBV	115737	357184	13.84%	1.855%
12	4.056	936	938	942	rBV4	643	592	0.02%	0.003%
13	4.240	978	995	1020	rVV	411035	1040791	40.34%	5.406%
14	4.458	1061	1063	1067	rVB4	1204	733	0.03%	0.004%
15	4.478	1067	1069	1073	rBV3	724	609	0.02%	0.003%
16	4.728	1144	1147	1152	rVB4	827	656	0.03%	0.003%
17	4.867	1188	1190	1193	rBV2	881	554	0.02%	0.003%
18	4.947	1194	1215	1249	rBV2	1012482	2580351	100.00%	13.403%
19	5.526	1383	1395	1427	rBV	809706	1677275	65.00%	8.712%
20	5.828	1477	1489	1492	rBV9	8213	13697	0.53%	0.071%
21	5.931	1517	1521	1523	rVB3	1189	812	0.03%	0.004%
22	5.982	1523	1537	1571	rBV	564855	1172537	45.44%	6.090%
23	6.217	1606	1610	1613	rBV3	1629	1291	0.05%	0.007%
24	6.307	1635	1638	1642	rVB5	1024	677	0.03%	0.004%
25	6.355	1649	1653	1655	rBV5	846	650	0.03%	0.003%
26	6.394	1662	1665	1668	rVV3	722	446	0.02%	0.002%
27	6.619	1731	1735	1738	rVB4	958	811	0.03%	0.004%
28	6.635	1738	1740	1742	rBV4	749	458	0.02%	0.002%
29	6.648	1742	1744	1746	rBV2	915	511	0.02%	0.003%
30	6.677	1751	1753	1761	rVV8	1315	1074	0.04%	0.006%
31	6.725	1765	1768	1771	rBV2	909	499	0.02%	0.003%
32	6.748	1771	1775	1779	rBV4	604	494	0.02%	0.003%
33	6.793	1787	1789	1791	rBV3	852	431	0.02%	0.002%
34	6.908	1813	1825	1865	rBV	297537	587092	22.75%	3.049%
35	7.130	1891	1894	1898	rVB5	1346	817	0.03%	0.004%
36	7.236	1915	1927	1959	rBV	1134999	2035768	78.90%	10.574%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037517.D
 Acq On : 25 Sep 2024 12:42
 Operator : SY/MD
 Sample : VIBLK388
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK388

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	7.548	2014	2024	2051	rBV	191081	362924	14.06%	1.885%
38	7.802	2099	2103	2106	rBV6	1041	890	0.03%	0.005%
39	7.850	2116	2118	2121	rVV3	774	532	0.02%	0.003%
40	7.973	2151	2156	2158	rVB4	939	624	0.02%	0.003%
41	8.024	2163	2172	2210	rBV2	347729	738352	28.61%	3.835%
42	8.423	2293	2296	2300	rBV5	712	578	0.02%	0.003%
43	8.458	2305	2307	2312	rVB4	915	613	0.02%	0.003%
44	8.609	2352	2354	2356	rBV3	763	529	0.02%	0.003%
45	8.709	2382	2385	2386	rBV2	956	484	0.02%	0.003%
46	8.776	2395	2406	2438	rBV	1245181	2054110	79.61%	10.669%
47	9.304	2566	2570	2572	rBV4	630	482	0.02%	0.003%
48	9.342	2579	2582	2587	rBV5	875	706	0.03%	0.004%
49	9.464	2617	2620	2622	rBV3	766	473	0.02%	0.002%
50	9.529	2637	2640	2642	rVV4	1522	949	0.04%	0.005%
51	9.587	2655	2658	2663	rVB4	989	805	0.03%	0.004%
52	9.731	2700	2703	2705	rVV2	762	508	0.02%	0.003%
53	9.757	2709	2711	2713	rBV3	803	449	0.02%	0.002%
54	9.841	2734	2737	2739	rBV	713	428	0.02%	0.002%
55	9.944	2766	2769	2773	rBV4	508	434	0.02%	0.002%
56	10.146	2820	2832	2857	rBV	646911	1029268	39.89%	5.346%
57	10.265	2867	2869	2872	rVB4	1100	685	0.03%	0.004%
58	10.397	2908	2910	2914	rVB5	843	541	0.02%	0.003%
59	10.487	2936	2938	2941	rBV4	682	458	0.02%	0.002%
60	10.564	2958	2962	2967	rVB4	636	622	0.02%	0.003%
61	10.587	2967	2969	2973	rVB4	856	598	0.02%	0.003%
62	10.696	2998	3003	3007	rBV4	720	675	0.03%	0.004%
63	10.780	3024	3029	3032	rBV5	1358	1211	0.05%	0.006%
64	10.837	3044	3047	3049	rBV	694	510	0.02%	0.003%
65	10.921	3068	3073	3076	rBV4	513	550	0.02%	0.003%
66	11.024	3103	3105	3110	rVB4	850	654	0.03%	0.003%
67	11.056	3110	3115	3117	rBV4	888	880	0.03%	0.005%
68	11.130	3136	3138	3141	rVB2	956	442	0.02%	0.002%
69	11.178	3142	3153	3188	rBV	1287422	2039819	79.05%	10.595%
70	11.432	3229	3232	3236	rVB3	1766	1439	0.06%	0.007%
71	11.458	3236	3240	3242	rBV4	1079	790	0.03%	0.004%
72	11.554	3253	3270	3300	rBV	1183612	1882937	72.97%	9.780%
73	11.767	3334	3336	3339	rBV3	1025	605	0.02%	0.003%
74	11.866	3365	3367	3373	rVB5	1031	765	0.03%	0.004%
75	11.960	3394	3396	3399	rVB3	1477	816	0.03%	0.004%
76	12.043	3420	3422	3426	rVB4	741	533	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037517.D
 Acq On : 25 Sep 2024 12:42
 Operator : SY/MD
 Sample : VIBLK388
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK388

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	12.069	3426	3430	3432	rBV4	1028	678	0.03%	0.004%
78	12.143	3448	3453	3456	rBV2	600	649	0.03%	0.003%
79	12.188	3462	3467	3470	rBV6	953	851	0.03%	0.004%
80	12.262	3487	3490	3494	rBV3	619	498	0.02%	0.003%
81	12.464	3549	3553	3557	rVB5	982	866	0.03%	0.004%
82	12.683	3618	3621	3623	rBV3	1398	771	0.03%	0.004%
83	12.998	3715	3719	3723	rBV2	815	730	0.03%	0.004%
84	13.021	3723	3726	3727	rBV2	587	428	0.02%	0.002%
85	13.178	3771	3775	3777	rBV3	1081	655	0.03%	0.003%
86	13.201	3778	3782	3784	rBV4	1416	1054	0.04%	0.005%
87	13.214	3784	3786	3788	rVB3	1286	500	0.02%	0.003%
88	13.226	3788	3790	3792	rBV3	841	536	0.02%	0.003%
89	13.397	3840	3843	3845	rBV3	1334	1001	0.04%	0.005%
90	13.455	3858	3861	3863	rBV3	1047	650	0.03%	0.003%
91	13.513	3873	3879	3880	rBV3	884	757	0.03%	0.004%
92	13.606	3905	3908	3912	rVB4	833	624	0.02%	0.003%
93	13.625	3912	3914	3918	rVB2	854	471	0.02%	0.002%
94	13.660	3923	3925	3928	rBV4	791	449	0.02%	0.002%
95	13.686	3930	3933	3935	rBV3	1103	642	0.02%	0.003%
96	13.963	4017	4019	4020	rBV	1314	559	0.02%	0.003%
97	14.197	4089	4092	4095	rVB3	1175	766	0.03%	0.004%
98	14.294	4120	4122	4125	rVB4	1161	662	0.03%	0.003%
99	14.310	4125	4127	4132	rVB5	1374	971	0.04%	0.005%
100	14.339	4132	4136	4137	rBV3	1019	810	0.03%	0.004%




Sum of corrected areas: 19252451

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037517.D
Acq On : 25 Sep 2024 12:42
Operator : SY/MD
Sample : VIBLK388
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK388

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

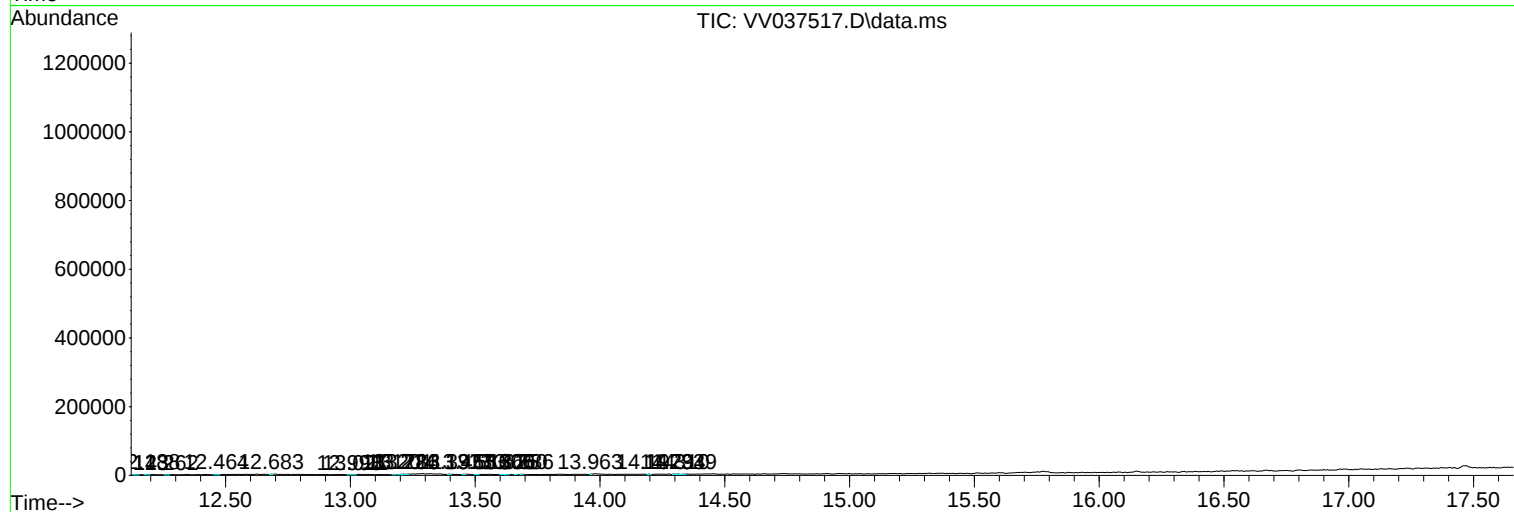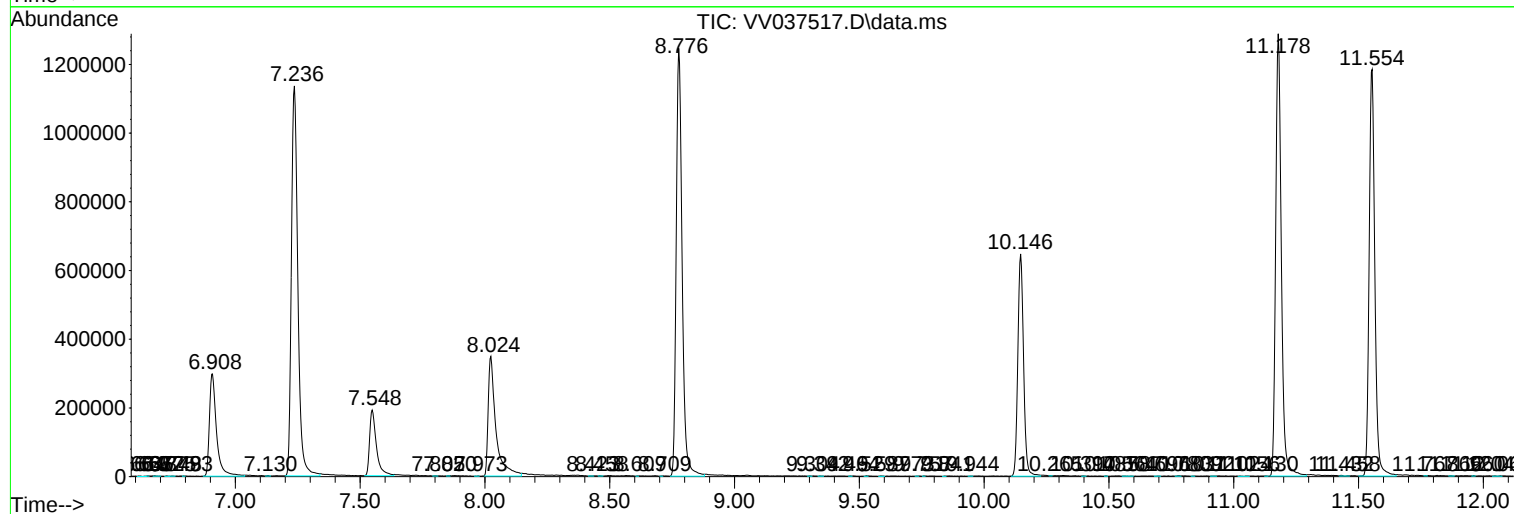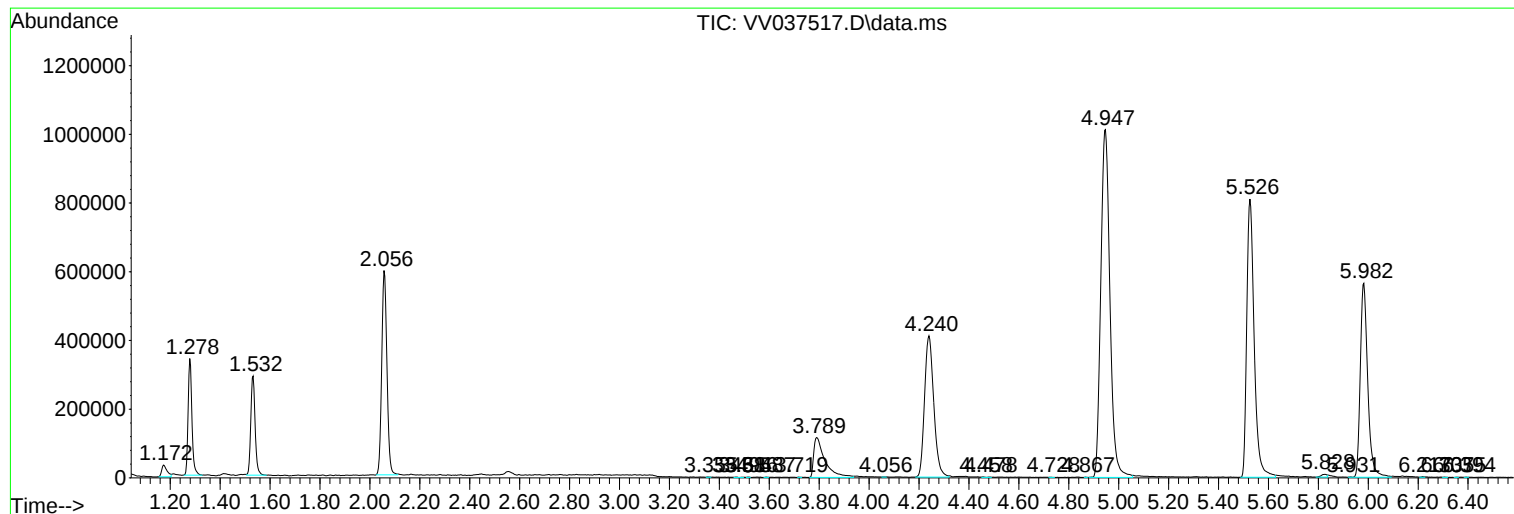

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037517.D
Acq On : 25 Sep 2024 12:42
Operator : SY/MD
Sample : VIBLK388
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK388

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037517.D
Acq On : 25 Sep 2024 12:42
Operator : SY/MD
Sample : VIBLK388
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK388

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------