

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037518.D
 Acq On : 25 Sep 2024 13:04
 Operator : SY/MD
 Sample : P4106-05
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0SY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037518.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	34	41	51	rBV	73392	104037	4.00%	0.553%
2	1.278	68	74	92	rVB	337983	358854	13.81%	1.909%
3	1.532	146	153	167	rVB	289743	339451	13.07%	1.806%
4	2.060	307	317	332	rBV	598781	866770	33.36%	4.611%
5	3.455	749	751	755	rBV4	670	492	0.02%	0.003%
6	3.474	755	757	760	rVV2	863	578	0.02%	0.003%
7	3.503	764	766	767	rBV	491	257	0.01%	0.001%
8	3.606	794	798	801	rBV2	531	410	0.02%	0.002%
9	3.629	801	805	807	rVV3	1026	635	0.02%	0.003%
10	3.645	807	810	813	rVB4	601	460	0.02%	0.002%
11	3.661	813	815	818	rBV3	604	380	0.01%	0.002%
12	3.741	836	840	844	rBV4	902	898	0.03%	0.005%
13	3.793	847	856	901	rBV2	121480	361744	13.92%	1.924%
14	4.243	979	996	1027	rBV	414807	1053794	40.56%	5.606%
15	4.587	1100	1103	1107	rVB5	1035	708	0.03%	0.004%
16	4.699	1135	1138	1141	rVB3	695	426	0.02%	0.002%
17	4.722	1142	1145	1148	rBV3	713	448	0.02%	0.002%
18	4.764	1156	1158	1161	rBV3	572	388	0.01%	0.002%
19	4.822	1172	1176	1178	rBV3	920	701	0.03%	0.004%
20	4.857	1183	1187	1189	rVV4	757	560	0.02%	0.003%
21	4.950	1199	1216	1258	rBV2	1010887	2598060	100.00%	13.821%
22	5.352	1338	1341	1347	rVB4	1214	1032	0.04%	0.005%
23	5.529	1384	1396	1431	rBV	731514	1517156	58.40%	8.071%
24	5.982	1522	1537	1565	rBV	566404	1176291	45.28%	6.257%
25	6.281	1627	1630	1633	rBV4	723	683	0.03%	0.004%
26	6.323	1640	1643	1644	rBV2	945	554	0.02%	0.003%
27	6.561	1715	1717	1721	rVB4	813	451	0.02%	0.002%
28	6.580	1721	1723	1728	rVB2	460	346	0.01%	0.002%
29	6.606	1728	1731	1733	rBV3	359	261	0.01%	0.001%
30	6.632	1737	1739	1741	rBV2	262	120	0.00%	0.001%
31	6.654	1743	1746	1749	rBV4	405	209	0.01%	0.001%
32	6.667	1749	1750	1753	rBV	672	339	0.01%	0.002%
33	6.719	1764	1766	1768	rBV	430	176	0.01%	0.001%
34	6.732	1768	1770	1771	rBV	873	362	0.01%	0.002%
35	6.822	1796	1798	1799	rBV	427	203	0.01%	0.001%
36	6.844	1802	1805	1806	rBV2	390	175	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037518.D
 Acq On : 25 Sep 2024 13:04
 Operator : SY/MD
 Sample : P4106-05
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0SY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	6.854	1806	1808	1811	rVB	494	225	0.01%	0.001%
38	6.870	1811	1813	1815	rBV2	607	415	0.02%	0.002%
39	6.908	1815	1825	1856	rBV	299624	575007	22.13%	3.059%
40	7.236	1916	1927	1966	rBV	1165426	2049709	78.89%	10.904%
41	7.548	2016	2024	2050	rBV	192079	362009	13.93%	1.926%
42	8.024	2159	2172	2218	rBV2	354890	780341	30.04%	4.151%
43	8.638	2361	2363	2367	rBV4	539	268	0.01%	0.001%
44	8.683	2375	2377	2378	rBV2	578	220	0.01%	0.001%
45	8.780	2395	2407	2433	rBV	1127276	1862246	71.68%	9.907%
46	9.172	2527	2529	2533	rVB5	1107	672	0.03%	0.004%
47	9.256	2553	2555	2556	rBV	382	97	0.00%	0.001%
48	9.326	2573	2577	2581	rBV4	801	820	0.03%	0.004%
49	9.416	2603	2605	2606	rBV	427	195	0.01%	0.001%
50	9.468	2619	2621	2622	rBV2	526	194	0.01%	0.001%
51	9.519	2635	2637	2638	rBV	453	162	0.01%	0.001%
52	9.584	2653	2657	2658	rBV2	615	362	0.01%	0.002%
53	9.661	2679	2681	2683	rVB3	920	312	0.01%	0.002%
54	9.696	2690	2692	2694	rVB3	404	190	0.01%	0.001%
55	9.725	2697	2701	2705	rVV4	608	483	0.02%	0.003%
56	9.825	2730	2732	2734	rBV2	355	114	0.00%	0.001%
57	9.976	2777	2779	2781	rVB	378	135	0.01%	0.001%
58	10.002	2781	2787	2790	rBV5	733	954	0.04%	0.005%
59	10.040	2797	2799	2801	rBV3	771	342	0.01%	0.002%
60	10.146	2820	2832	2854	rBV	666101	1056656	40.67%	5.621%
61	10.436	2919	2922	2925	rVB3	957	488	0.02%	0.003%
62	10.452	2925	2927	2929	rVB3	534	204	0.01%	0.001%
63	10.471	2929	2933	2937	rBV6	1205	1193	0.05%	0.006%
64	10.619	2976	2979	2980	rBV2	662	366	0.01%	0.002%
65	10.654	2988	2990	2991	rBV	421	224	0.01%	0.001%
66	10.693	2999	3002	3006	rBV3	717	506	0.02%	0.003%
67	10.818	3036	3041	3042	rBV3	742	610	0.02%	0.003%
68	10.860	3051	3054	3056	rBV3	744	510	0.02%	0.003%
69	10.905	3066	3068	3070	rBV2	535	291	0.01%	0.002%
70	11.027	3104	3106	3109	rVB3	451	242	0.01%	0.001%
71	11.063	3113	3117	3118	rBV5	700	409	0.02%	0.002%
72	11.075	3120	3121	3125	rBV2	402	286	0.01%	0.002%
73	11.127	3133	3137	3139	rBV3	734	488	0.02%	0.003%
74	11.178	3141	3153	3189	rBV	1154741	1840531	70.84%	9.791%
75	11.481	3245	3247	3248	rBV	891	411	0.02%	0.002%
76	11.555	3259	3270	3300	rBV	1155962	1847869	71.12%	9.830%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037518.D
Acq On : 25 Sep 2024 13:04
Operator : SY/MD
Sample : P4106-05
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

77	12.172	3460	3462	3463	rBV2	534	249	0.01%	0.001%
78	12.281	3494	3496	3499	rBV2	406	252	0.01%	0.001%
79	12.458	3549	3551	3554	rBV2	881	562	0.02%	0.003%
80	12.490	3559	3561	3562	rBV	1239	526	0.02%	0.003%
81	12.985	3713	3715	3719	rBV2	1243	743	0.03%	0.004%
82	13.265	3799	3802	3803	rBV3	1083	754	0.03%	0.004%
83	13.554	3887	3892	3902	rVB	20719	17894	0.69%	0.095%
84	14.911	4312	4314	4320	rBV5	2421	1984	0.08%	0.011%




Sum of corrected areas: 18798129

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037518.D
Acq On : 25 Sep 2024 13:04
Operator : SY/MD
Sample : P4106-05
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

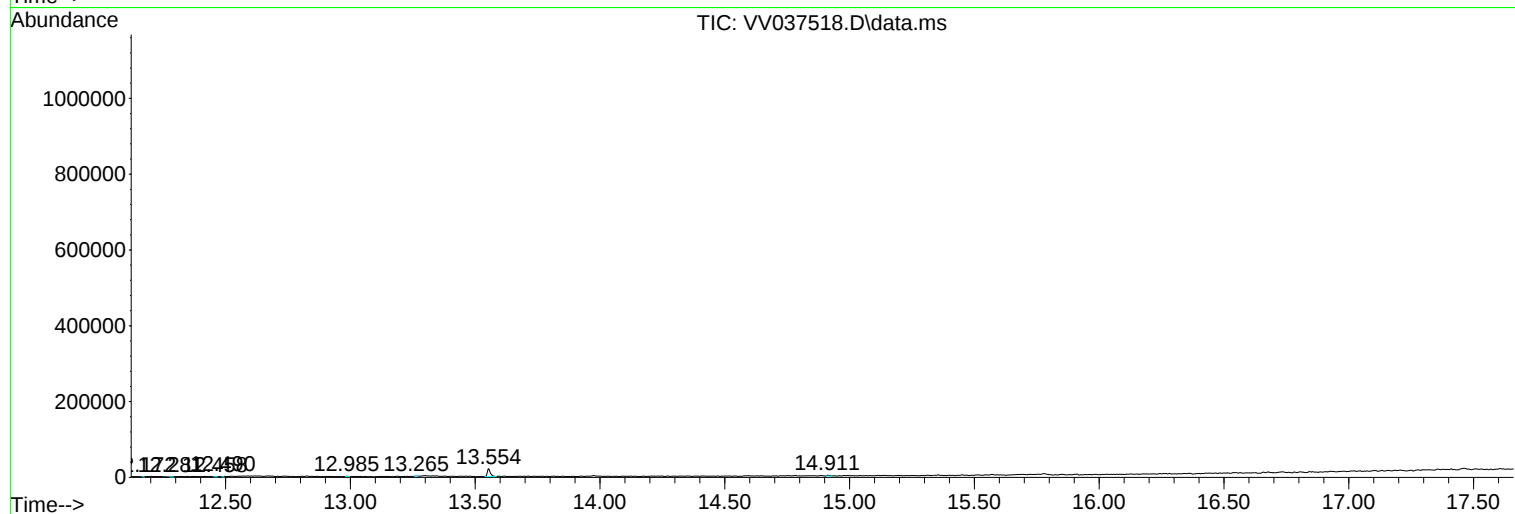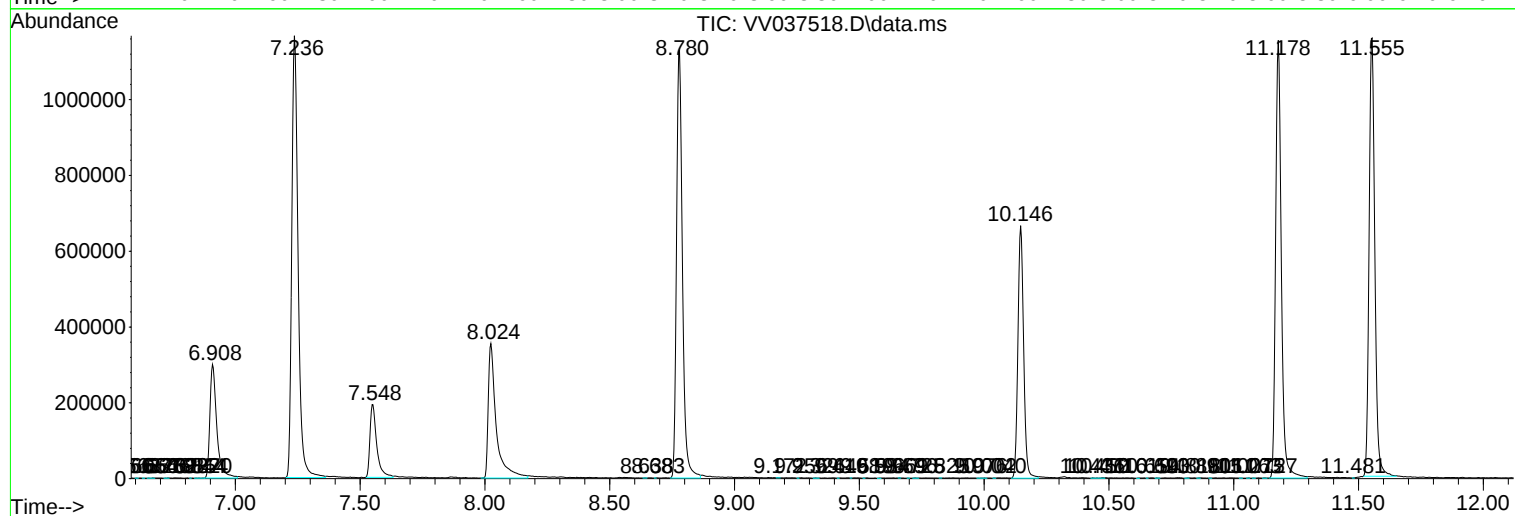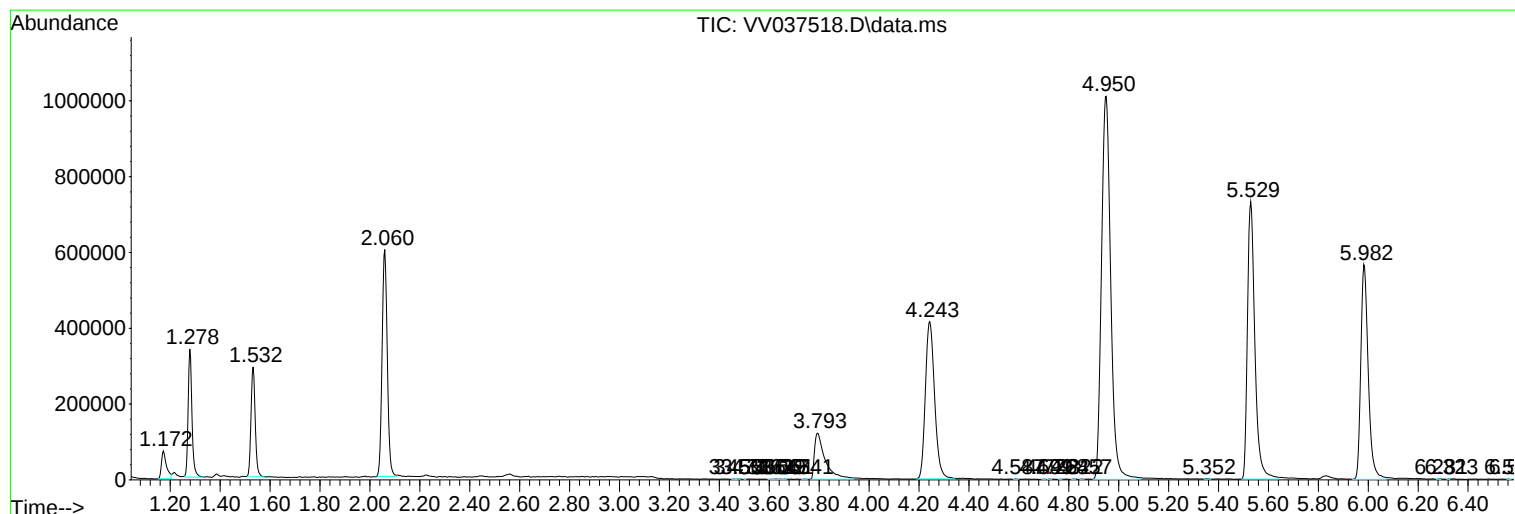

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037518.D
Acq On : 25 Sep 2024 13:04
Operator : SY/MD
Sample : P4106-05
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037518.D
Acq On : 25 Sep 2024 13:04
Operator : SY/MD
Sample : P4106-05
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------