

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037524.D
 Acq On : 25 Sep 2024 15:13
 Operator : SY/MD
 Sample : P4109-10
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037524.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	35	41	51	rBV	42238	61967	2.54%	0.353%
2	1.278	68	74	90	rVB	306472	331842	13.60%	1.890%
3	1.532	145	153	170	rVB	270873	323959	13.27%	1.846%
4	2.060	308	317	335	rVB	560220	805234	32.99%	4.587%
5	3.372	723	725	726	rBV	741	311	0.01%	0.002%
6	3.632	803	806	811	rVB3	723	463	0.02%	0.003%
7	3.683	819	822	823	rBV	540	262	0.01%	0.001%
8	3.699	823	827	830	rBV2	539	460	0.02%	0.003%
9	3.719	830	833	836	rBV2	537	471	0.02%	0.003%
10	3.754	842	844	847	rVB2	392	187	0.01%	0.001%
11	3.793	847	856	898	rBV2	111518	328321	13.45%	1.870%
12	4.124	957	959	960	rBV2	1143	462	0.02%	0.003%
13	4.243	981	996	1025	rBV	391278	987904	40.47%	5.628%
14	4.503	1073	1077	1080	rBV4	1094	915	0.04%	0.005%
15	4.561	1090	1095	1098	rBV5	1032	899	0.04%	0.005%
16	4.580	1099	1101	1103	rBV2	498	210	0.01%	0.001%
17	4.770	1158	1160	1163	rBV2	922	523	0.02%	0.003%
18	4.950	1200	1216	1256	rBV2	958427	2440809	100.00%	13.905%
19	5.240	1304	1306	1309	rBV2	912	485	0.02%	0.003%
20	5.407	1356	1358	1359	rBV	607	219	0.01%	0.001%
21	5.529	1385	1396	1428	rBV	689830	1405785	57.60%	8.008%
22	5.982	1525	1537	1568	rBV	531187	1108257	45.41%	6.313%
23	6.371	1655	1658	1663	rBV5	1479	1177	0.05%	0.007%
24	6.445	1678	1681	1684	rBV4	698	582	0.02%	0.003%
25	6.481	1689	1692	1696	rBV4	847	802	0.03%	0.005%
26	6.526	1704	1706	1707	rBV	507	178	0.01%	0.001%
27	6.551	1712	1714	1716	rVV3	900	528	0.02%	0.003%
28	6.577	1720	1722	1725	rBV3	452	242	0.01%	0.001%
29	6.596	1725	1728	1729	rBV2	411	231	0.01%	0.001%
30	6.641	1740	1742	1744	rBV2	516	210	0.01%	0.001%
31	6.822	1797	1798	1799	rBV	305	112	0.00%	0.001%
32	6.873	1811	1814	1815	rBV2	480	309	0.01%	0.002%
33	6.908	1815	1825	1847	rBV	272132	524556	21.49%	2.988%
34	7.236	1917	1927	1964	rBV	1078236	1915975	78.50%	10.915%
35	7.551	2016	2025	2046	rBV	182521	338411	13.86%	1.928%
36	8.024	2163	2172	2215	rBV2	336460	739904	30.31%	4.215%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037524.D
 Acq On : 25 Sep 2024 15:13
 Operator : SY/MD
 Sample : P4109-10
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	8.542	2331	2333	2334	rBV	782	296	0.01%	0.002%
38	8.690	2377	2379	2381	rBV	883	462	0.02%	0.003%
39	8.780	2396	2407	2439	rBV	1060447	1757106	71.99%	10.010%
40	9.188	2531	2534	2537	rVB3	1092	649	0.03%	0.004%
41	9.214	2537	2542	2544	rBV5	1218	1063	0.04%	0.006%
42	9.310	2571	2572	2573	rBV	379	86	0.00%	0.000%
43	9.394	2595	2598	2601	rVB2	607	436	0.02%	0.002%
44	9.416	2601	2605	2607	rBV4	1153	948	0.04%	0.005%
45	9.461	2617	2619	2620	rBV	423	164	0.01%	0.001%
46	9.516	2634	2636	2639	rBV	594	197	0.01%	0.001%
47	9.567	2650	2652	2654	rBV2	432	189	0.01%	0.001%
48	9.612	2660	2666	2670	rBV5	878	930	0.04%	0.005%
49	9.632	2670	2672	2675	rVV3	607	292	0.01%	0.002%
50	9.648	2675	2677	2681	rVB2	394	216	0.01%	0.001%
51	9.674	2683	2685	2687	rBV	452	181	0.01%	0.001%
52	9.683	2687	2688	2690	rBV	521	185	0.01%	0.001%
53	9.805	2724	2726	2728	rBV3	398	209	0.01%	0.001%
54	9.870	2745	2746	2749	rBV2	502	314	0.01%	0.002%
55	9.892	2751	2753	2759	rVB4	855	706	0.03%	0.004%
56	9.924	2759	2763	2764	rBV2	469	301	0.01%	0.002%
57	9.960	2769	2774	2779	rBV4	1077	1152	0.05%	0.007%
58	9.985	2779	2782	2785	rVB2	959	594	0.02%	0.003%
59	10.005	2785	2788	2789	rBV2	854	470	0.02%	0.003%
60	10.018	2789	2792	2799	rVB4	690	664	0.03%	0.004%
61	10.085	2811	2813	2817	rVB2	986	503	0.02%	0.003%
62	10.146	2820	2832	2852	rBV	637840	1008850	41.33%	5.747%
63	10.464	2928	2931	2934	rBV3	952	796	0.03%	0.005%
64	10.603	2972	2974	2977	rBV2	358	227	0.01%	0.001%
65	10.622	2979	2980	2982	rBV	468	213	0.01%	0.001%
66	10.680	2996	2998	3001	rBV2	416	215	0.01%	0.001%
67	10.693	3001	3002	3003	rVB2	334	67	0.00%	0.000%
68	10.783	3027	3030	3033	rBV3	1649	1260	0.05%	0.007%
69	10.831	3043	3045	3046	rBV2	325	113	0.00%	0.001%
70	10.937	3073	3078	3081	rBV4	676	591	0.02%	0.003%
71	10.982	3090	3092	3096	rBV2	761	467	0.02%	0.003%
72	11.005	3096	3099	3100	rBV	760	422	0.02%	0.002%
73	11.053	3112	3114	3116	rVB2	541	195	0.01%	0.001%
74	11.072	3116	3120	3123	rBV4	1057	846	0.03%	0.005%
75	11.108	3129	3131	3132	rBV	315	97	0.00%	0.001%
76	11.124	3132	3136	3138	rBV4	781	505	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037524.D
 Acq On : 25 Sep 2024 15:13
 Operator : SY/MD
 Sample : P4109-10
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

77	11.140	3138	3141	3142	rBV	523	307	0.01%	0.002%
78	11.178	3142	3153	3182	rBV	1071273	1680938	68.87%	9.576%
79	11.554	3258	3270	3297	rBV	1106862	1761641	72.17%	10.036%
80	12.075	3429	3432	3434	rBV2	965	560	0.02%	0.003%
81	12.146	3452	3454	3460	rBV4	822	745	0.03%	0.004%
82	12.175	3460	3463	3464	rBV2	671	343	0.01%	0.002%
83	12.220	3472	3477	3481	rBV5	859	927	0.04%	0.005%
84	12.924	3694	3696	3699	rBV3	649	283	0.01%	0.002%
85	12.979	3710	3713	3714	rBV3	978	627	0.03%	0.004%
86	13.368	3831	3834	3838	rBV4	1443	1179	0.05%	0.007%




Sum of corrected areas: 17553889

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037524.D
Acq On : 25 Sep 2024 15:13
Operator : SY/MD
Sample : P4109-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

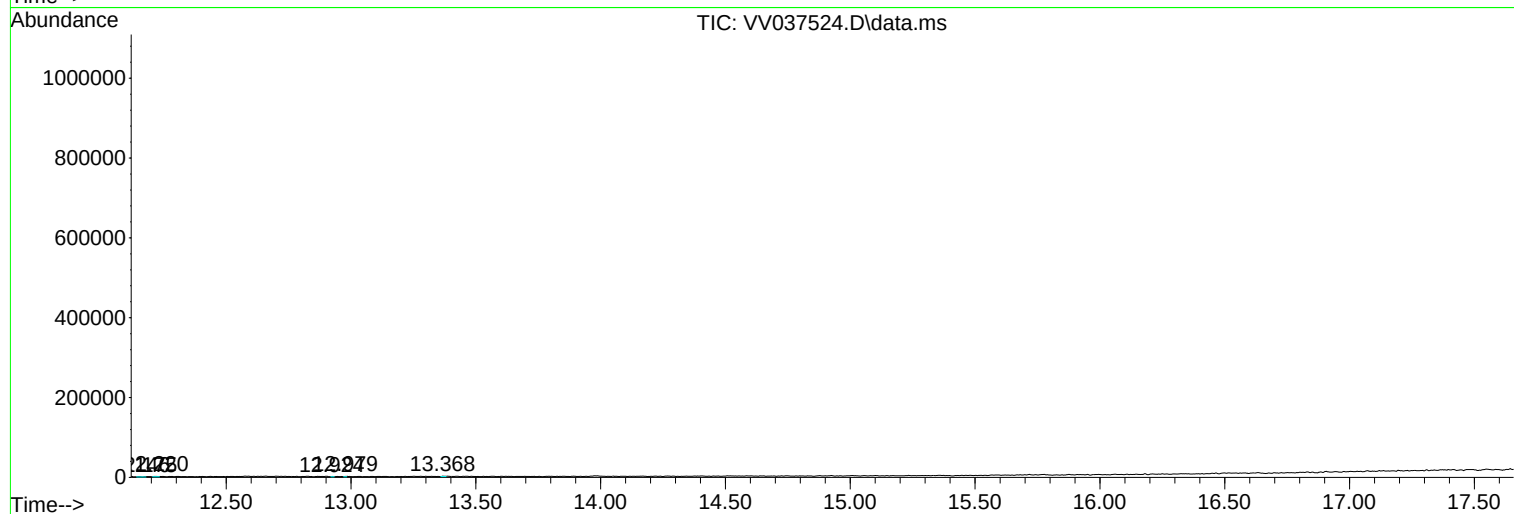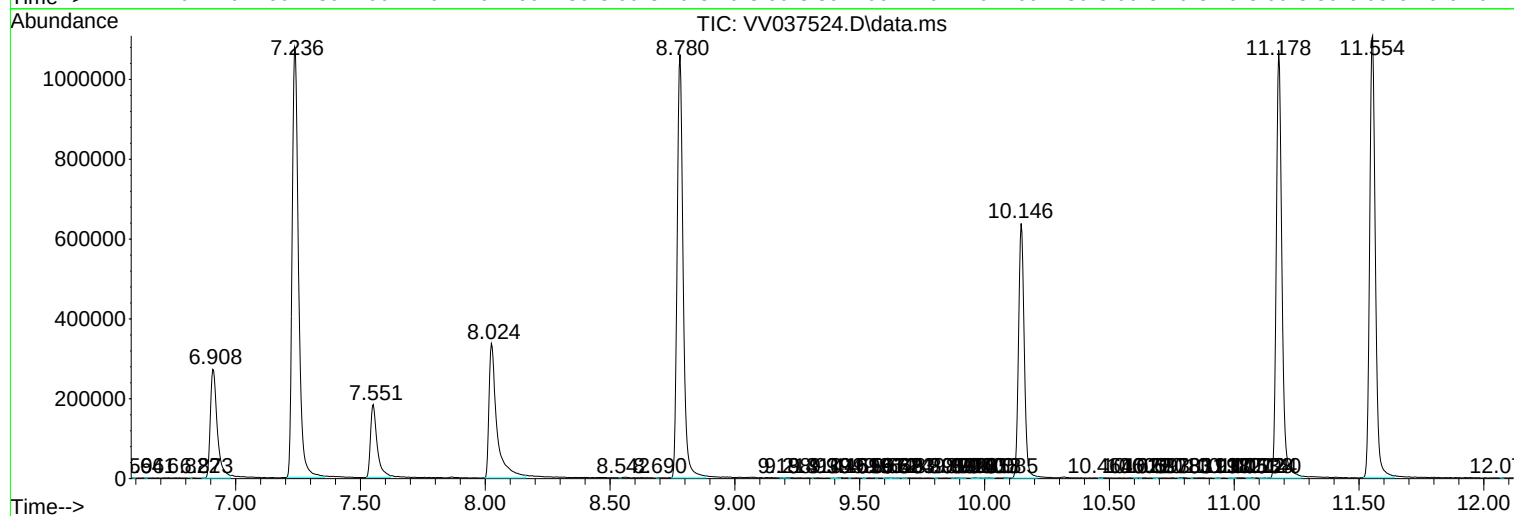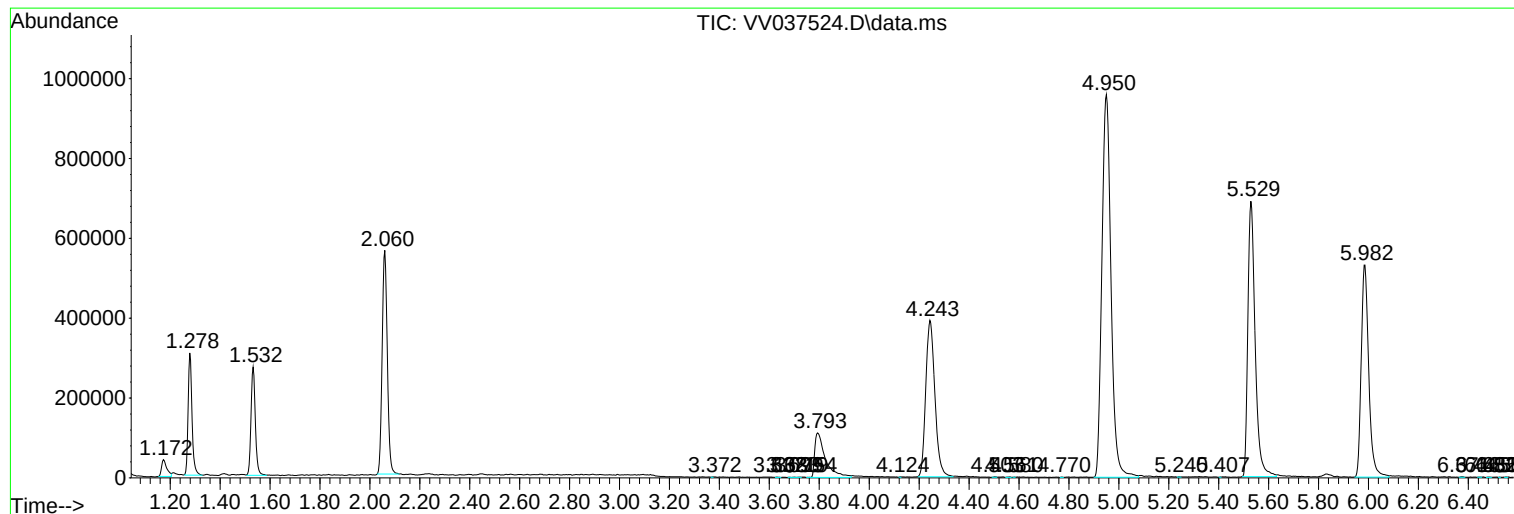

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037524.D
Acq On : 25 Sep 2024 15:13
Operator : SY/MD
Sample : P4109-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037524.D
Acq On : 25 Sep 2024 15:13
Operator : SY/MD
Sample : P4109-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------