

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037526.D
 Acq On : 25 Sep 2024 15:56
 Operator : SY/MD
 Sample : P4131-05
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	35	41	52	rBV	36846	57016	2.36%	0.330%
2	1.278	67	74	90	rVB	302000	325728	13.50%	1.883%
3	1.532	145	153	169	rVB	269994	317830	13.17%	1.837%
4	2.060	306	317	336	rBV	559474	811222	33.61%	4.689%
5	3.185	664	667	670	rVB4	1554	950	0.04%	0.005%
6	3.683	819	822	826	rVB2	594	553	0.02%	0.003%
7	3.722	831	834	837	rBV3	833	642	0.03%	0.004%
8	3.796	848	857	890	rBV2	110054	305386	12.65%	1.765%
9	4.082	943	946	951	rVB4	1208	918	0.04%	0.005%
10	4.243	979	996	1029	rVV	389988	992350	41.12%	5.736%
11	4.436	1053	1056	1058	rBV4	883	532	0.02%	0.003%
12	4.632	1112	1117	1118	rBV4	779	570	0.02%	0.003%
13	4.654	1122	1124	1130	rVB3	865	611	0.03%	0.004%
14	4.686	1130	1134	1136	rBV3	661	557	0.02%	0.003%
15	4.815	1167	1174	1177	rBV5	777	922	0.04%	0.005%
16	4.886	1192	1196	1200	rBV5	880	832	0.03%	0.005%
17	4.950	1200	1216	1257	rBV2	956466	2413568	100.00%	13.951%
18	5.198	1291	1293	1296	rVB3	925	505	0.02%	0.003%
19	5.256	1309	1311	1313	rBV3	871	495	0.02%	0.003%
20	5.368	1344	1346	1351	rVB4	980	633	0.03%	0.004%
21	5.420	1357	1362	1363	rBV2	1056	1063	0.04%	0.006%
22	5.442	1367	1369	1372	rVB3	998	569	0.02%	0.003%
23	5.468	1372	1377	1381	rBV6	1178	1189	0.05%	0.007%
24	5.529	1384	1396	1421	rBV	665215	1356511	56.20%	7.841%
25	5.722	1454	1456	1459	rBV4	1351	668	0.03%	0.004%
26	5.776	1471	1473	1476	rBV5	889	507	0.02%	0.003%
27	5.831	1478	1490	1504	rBV9	6450	15819	0.66%	0.091%
28	5.985	1523	1538	1575	rBV	528704	1102416	45.68%	6.372%
29	6.252	1619	1621	1625	rVB3	1124	574	0.02%	0.003%
30	6.278	1626	1629	1633	rVB6	948	659	0.03%	0.004%
31	6.365	1653	1656	1659	rBV3	906	595	0.02%	0.003%
32	6.535	1704	1709	1712	rBV4	739	795	0.03%	0.005%
33	6.555	1712	1715	1719	rVB2	1024	656	0.03%	0.004%
34	6.674	1749	1752	1757	rBV3	1149	954	0.04%	0.006%
35	6.735	1769	1771	1777	rVB5	1118	1059	0.04%	0.006%
36	6.764	1777	1780	1782	rBV2	898	598	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037526.D
 Acq On : 25 Sep 2024 15:56
 Operator : SY/MD
 Sample : P4131-05
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	6.908	1815	1825	1859	rBV	268491	528163	21.88%	3.053%
38	7.236	1916	1927	1957	rBV	1065572	1895153	78.52%	10.955%
39	7.487	2001	2005	2006	rBV3	987	552	0.02%	0.003%
40	7.551	2014	2025	2049	rBV	182468	337696	13.99%	1.952%
41	7.786	2096	2098	2102	rVB5	1107	711	0.03%	0.004%
42	7.866	2120	2123	2126	rBV4	771	604	0.03%	0.003%
43	7.924	2137	2141	2142	rBV3	802	531	0.02%	0.003%
44	8.024	2163	2172	2208	rBV2	329010	716961	29.71%	4.144%
45	8.358	2274	2276	2278	rBV3	885	484	0.02%	0.003%
46	8.490	2312	2317	2319	rBV5	884	893	0.04%	0.005%
47	8.780	2396	2407	2432	rBV	1015128	1690434	70.04%	9.771%
48	9.085	2499	2502	2504	rBV3	1154	672	0.03%	0.004%
49	9.378	2587	2593	2596	rBV4	1295	1228	0.05%	0.007%
50	9.423	2605	2607	2610	rVB3	978	562	0.02%	0.003%
51	9.458	2615	2618	2621	rVV3	621	496	0.02%	0.003%
52	9.519	2633	2637	2639	rBV3	891	681	0.03%	0.004%
53	9.538	2639	2643	2646	rVV3	811	717	0.03%	0.004%
54	9.609	2662	2665	2668	rBV3	969	699	0.03%	0.004%
55	9.677	2682	2686	2687	rBV2	844	521	0.02%	0.003%
56	9.718	2695	2699	2701	rBV3	613	482	0.02%	0.003%
57	9.734	2703	2704	2708	rVV3	856	535	0.02%	0.003%
58	9.757	2708	2711	2714	rVB2	729	492	0.02%	0.003%
59	9.866	2741	2745	2749	rVB4	1066	770	0.03%	0.004%
60	9.892	2749	2753	2758	rBV3	875	839	0.03%	0.005%
61	9.921	2758	2762	2763	rBV2	887	580	0.02%	0.003%
62	10.014	2788	2791	2793	rVV3	950	520	0.02%	0.003%
63	10.146	2817	2832	2855	rBV	628056	1002424	41.53%	5.794%
64	10.288	2873	2876	2878	rBV3	925	560	0.02%	0.003%
65	10.400	2909	2911	2916	rVB5	774	675	0.03%	0.004%
66	10.423	2916	2918	2921	rBV2	996	612	0.03%	0.004%
67	10.442	2921	2924	2928	rVB4	1096	1076	0.04%	0.006%
68	10.468	2928	2932	2935	rBV4	998	759	0.03%	0.004%
69	10.535	2951	2953	2958	rVB3	1101	792	0.03%	0.005%
70	10.715	3007	3009	3016	rBV6	754	741	0.03%	0.004%
71	10.796	3031	3034	3038	rVB4	896	634	0.03%	0.004%
72	10.876	3055	3059	3064	rVV4	718	687	0.03%	0.004%
73	10.931	3073	3076	3079	rBV3	646	480	0.02%	0.003%
74	10.947	3079	3081	3086	rVB5	647	488	0.02%	0.003%
75	10.976	3086	3090	3093	rBV5	988	828	0.03%	0.005%
76	11.178	3142	3153	3183	rBV	1009254	1630039	67.54%	9.422%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037526.D
 Acq On : 25 Sep 2024 15:56
 Operator : SY/MD
 Sample : P4131-05
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	11.500	3251	3253	3256	rVB3	1207	575	0.02%	0.003%
78	11.554	3257	3270	3299	rBV	1092102	1742360	72.19%	10.071%
79	11.750	3328	3331	3334	rBV5	1490	1014	0.04%	0.006%
80	11.934	3385	3388	3390	rBV3	916	599	0.02%	0.003%
81	11.947	3390	3392	3395	rVV2	831	536	0.02%	0.003%
82	12.046	3420	3423	3427	rBV4	684	609	0.03%	0.004%
83	12.307	3502	3504	3510	rVB5	899	561	0.02%	0.003%
84	12.355	3516	3519	3521	rBV3	838	482	0.02%	0.003%
85	12.525	3568	3572	3574	rBV3	920	778	0.03%	0.004%
86	12.567	3579	3585	3586	rBV3	1426	1245	0.05%	0.007%
87	12.741	3633	3639	3641	rBV5	945	887	0.04%	0.005%
88	12.950	3703	3704	3707	rVB3	1003	486	0.02%	0.003%
89	12.992	3714	3717	3720	rVB5	1007	604	0.03%	0.003%
90	13.111	3751	3754	3757	rBV3	1091	772	0.03%	0.004%
91	13.439	3850	3856	3859	rVB5	1061	899	0.04%	0.005%
92	13.641	3916	3919	3923	rVB4	931	719	0.03%	0.004%
93	14.149	4072	4077	4079	rBV7	1111	891	0.04%	0.005%
94	14.303	4121	4125	4129	rBV5	1266	1058	0.04%	0.006%
95	14.545	4197	4200	4202	rBV3	1044	736	0.03%	0.004%
96	14.721	4253	4255	4258	rBV4	802	496	0.02%	0.003%
97	15.085	4366	4368	4372	rBV4	1282	735	0.03%	0.004%
98	15.223	4406	4411	4415	rBV6	1425	1774	0.07%	0.010%
99	15.406	4464	4468	4470	rBV4	1376	1152	0.05%	0.007%
100	15.442	4476	4479	4480	rBV2	1539	888	0.04%	0.005%




Sum of corrected areas: 17300079

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037526.D
Acq On : 25 Sep 2024 15:56
Operator : SY/MD
Sample : P4131-05
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

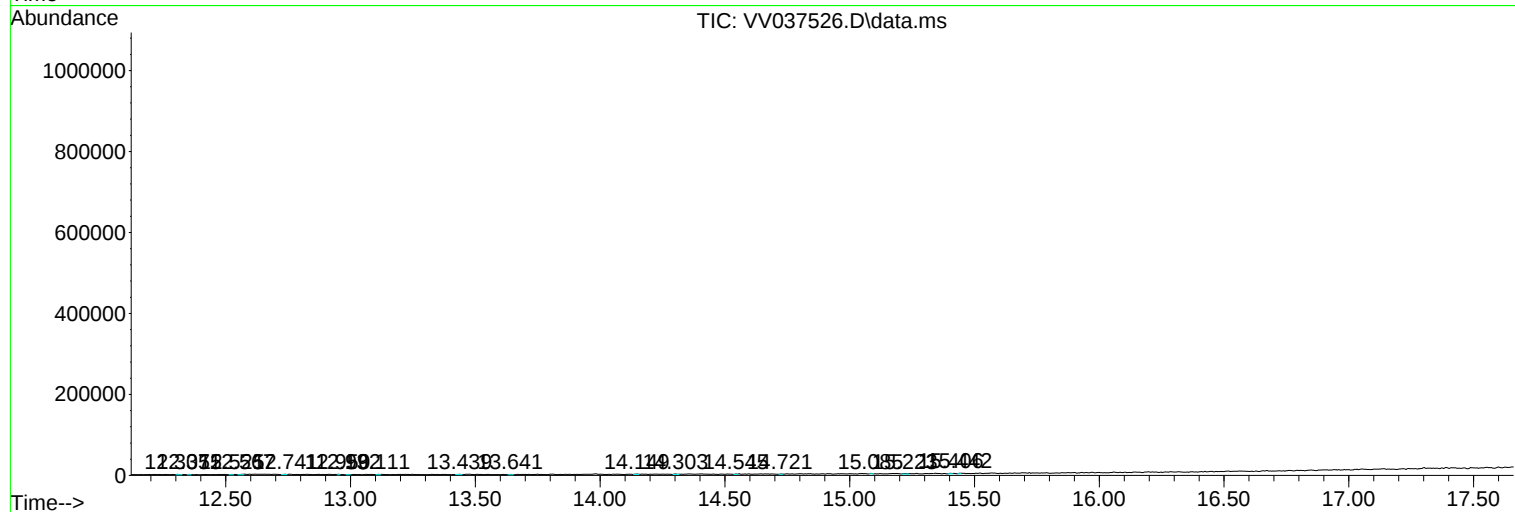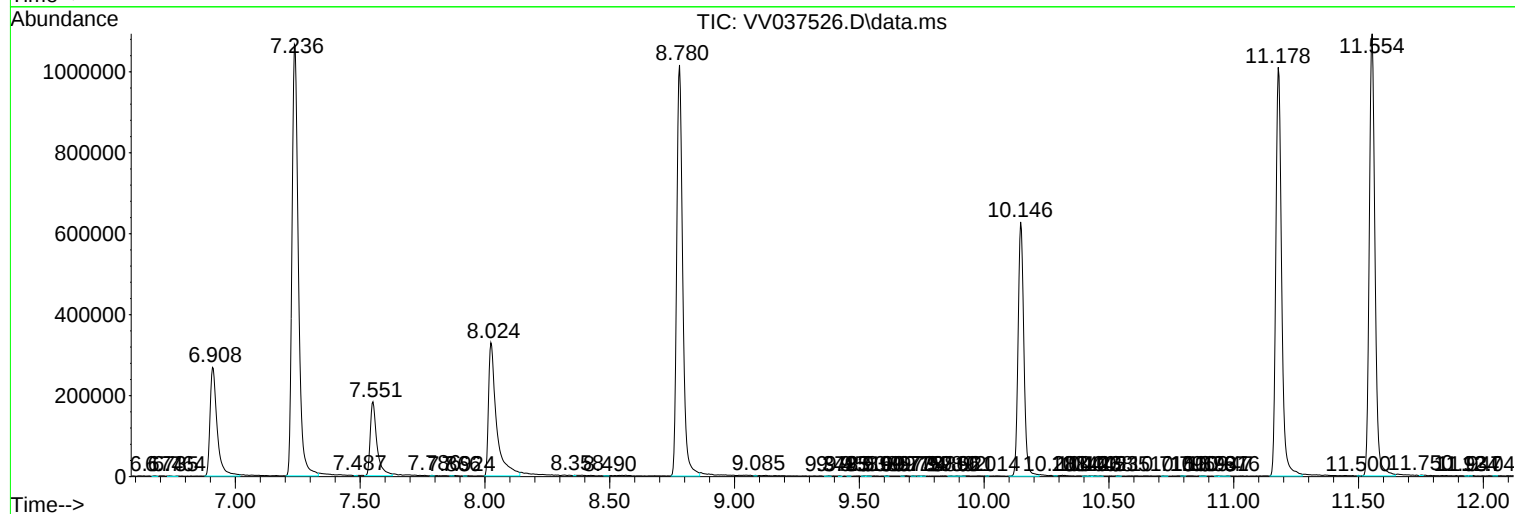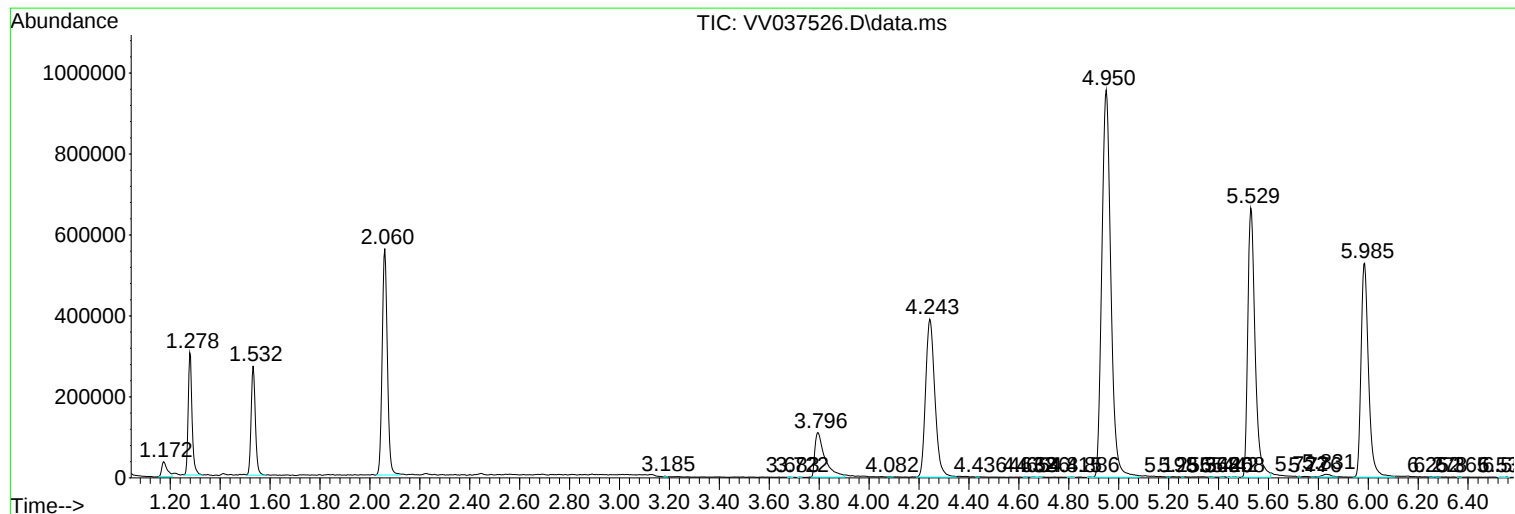

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037526.D
Acq On : 25 Sep 2024 15:56
Operator : SY/MD
Sample : P4131-05
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037526.D
Acq On : 25 Sep 2024 15:56
Operator : SY/MD
Sample : P4131-05
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------