

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037527.D
 Acq On : 25 Sep 2024 16:17
 Operator : SY/MD
 Sample : P4183-07
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037527.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	35	42	52	rBV	24015	40444	1.75%	0.234%
2	1.278	68	74	92	rVB	299484	320918	13.91%	1.860%
3	1.532	146	153	170	rVB	267660	316460	13.72%	1.834%
4	2.060	308	317	328	rBV	536576	767264	33.27%	4.446%
5	3.433	742	744	749	rVB3	738	639	0.03%	0.004%
6	3.455	749	751	753	rBV2	803	434	0.02%	0.003%
7	3.696	824	826	831	rBV4	560	503	0.02%	0.003%
8	3.722	831	834	837	rBV3	571	333	0.01%	0.002%
9	3.738	837	839	840	rBV2	360	141	0.01%	0.001%
10	3.796	847	857	892	rBV	111118	320191	13.88%	1.855%
11	4.243	981	996	1025	rBV	372019	950650	41.22%	5.509%
12	4.513	1078	1080	1082	rBV2	608	385	0.02%	0.002%
13	4.580	1097	1101	1104	rBV4	872	734	0.03%	0.004%
14	4.596	1104	1106	1109	rVV2	732	295	0.01%	0.002%
15	4.616	1110	1112	1115	rVB	579	279	0.01%	0.002%
16	4.658	1122	1125	1127	rBV3	630	455	0.02%	0.003%
17	4.709	1139	1141	1147	rBB4	622	370	0.02%	0.002%
18	4.751	1151	1154	1155	rBV2	379	174	0.01%	0.001%
19	4.764	1155	1158	1160	rBV2	713	310	0.01%	0.002%
20	4.838	1177	1181	1184	rBV3	1044	881	0.04%	0.005%
21	4.950	1198	1216	1246	rBV2	903710	2306349	100.00%	13.365%
22	5.420	1359	1362	1363	rBV2	794	473	0.02%	0.003%
23	5.439	1366	1368	1372	rVV4	1253	834	0.04%	0.005%
24	5.529	1385	1396	1427	rBV	703738	1442941	62.56%	8.361%
25	5.986	1525	1538	1563	rBV	512171	1058270	45.89%	6.132%
26	6.349	1650	1651	1652	rBV	490	154	0.01%	0.001%
27	6.413	1668	1671	1673	rVB3	967	524	0.02%	0.003%
28	6.436	1673	1678	1682	rBV5	998	1024	0.04%	0.006%
29	6.519	1700	1704	1706	rBV3	749	581	0.03%	0.003%
30	6.600	1727	1729	1731	rVB3	590	242	0.01%	0.001%
31	6.619	1732	1735	1737	rBV2	337	224	0.01%	0.001%
32	6.635	1738	1740	1744	rVB4	874	508	0.02%	0.003%
33	6.667	1749	1750	1754	rBV2	716	388	0.02%	0.002%
34	6.683	1754	1755	1761	rBV4	395	307	0.01%	0.002%
35	6.712	1761	1764	1765	rBV3	660	331	0.01%	0.002%
36	6.764	1778	1780	1784	rVB3	798	467	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037527.D
 Acq On : 25 Sep 2024 16:17
 Operator : SY/MD
 Sample : P4183-07
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	6.828	1797	1800	1805	rVB5	928	599	0.03%	0.003%
38	6.850	1805	1807	1809	rBV2	381	169	0.01%	0.001%
39	6.860	1809	1810	1812	rBV	370	108	0.00%	0.001%
40	6.873	1812	1814	1815	rBV	667	351	0.02%	0.002%
41	6.908	1815	1825	1859	rBV	261714	508699	22.06%	2.948%
42	7.236	1916	1927	1964	rBV	992467	1792639	77.73%	10.388%
43	7.551	2016	2025	2045	rBV	172964	321702	13.95%	1.864%
44	7.915	2137	2138	2140	rBV2	552	231	0.01%	0.001%
45	7.953	2147	2150	2151	rBV3	1030	546	0.02%	0.003%
46	7.976	2152	2157	2164	rVV5	7882	11505	0.50%	0.067%
47	8.024	2164	2172	2218	rVV2	342929	737855	31.99%	4.276%
48	8.638	2358	2363	2365	rBV5	1593	1299	0.06%	0.008%
49	8.780	2391	2407	2440	rBV	1103816	1815441	78.71%	10.520%
50	9.143	2518	2520	2523	rBV2	725	277	0.01%	0.002%
51	9.419	2604	2606	2608	rBV2	660	347	0.02%	0.002%
52	9.468	2619	2621	2622	rVB2	355	87	0.00%	0.001%
53	9.484	2622	2626	2627	rBV3	980	596	0.03%	0.003%
54	9.577	2652	2655	2659	rVB4	759	490	0.02%	0.003%
55	9.664	2679	2682	2683	rBV3	458	192	0.01%	0.001%
56	9.715	2692	2698	2710	rVB7	7378	11680	0.51%	0.068%
57	9.889	2743	2752	2761	rVB6	12874	20462	0.89%	0.119%
58	10.037	2797	2798	2800	rVB2	633	226	0.01%	0.001%
59	10.146	2821	2832	2854	rBV	630626	992776	43.05%	5.753%
60	10.355	2895	2897	2900	rVB3	891	413	0.02%	0.002%
61	10.419	2914	2917	2918	rBV2	913	443	0.02%	0.003%
62	10.567	2956	2963	2968	rBV7	3380	5763	0.25%	0.033%
63	10.677	2995	2997	3001	rBV4	839	692	0.03%	0.004%
64	10.738	3015	3016	3019	rVB	546	147	0.01%	0.001%
65	10.760	3019	3023	3025	rBV2	402	301	0.01%	0.002%
66	10.776	3025	3028	3029	rBV2	840	484	0.02%	0.003%
67	10.786	3029	3031	3033	rVB2	1288	563	0.02%	0.003%
68	10.808	3034	3038	3041	rBV6	1331	1355	0.06%	0.008%
69	11.124	3129	3136	3143	rBV7	11713	17459	0.76%	0.101%
70	11.178	3143	3153	3182	rBV	1118098	1769953	76.74%	10.256%
71	11.554	3260	3270	3302	rVB	1061829	1699230	73.68%	9.846%
72	12.011	3409	3412	3414	rBV2	1427	1093	0.05%	0.006%
73	12.461	3549	3552	3554	rBV3	1083	701	0.03%	0.004%
74	12.522	3569	3571	3574	rBV3	1004	574	0.02%	0.003%
75	12.927	3694	3697	3698	rBV2	886	469	0.02%	0.003%
76	13.040	3731	3732	3733	rBV	610	216	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037527.D
Acq On : 25 Sep 2024 16:17
Operator : SY/MD
Sample : P4183-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FC3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Title : VOC Analysis

77	13.168	3768	3772	3778	rBV5	1271	1282	0.06%	0.007%
78	13.558	3891	3893	3896	rBV2	913	669	0.03%	0.004%
79	13.689	3932	3934	3938	rBV4	1025	648	0.03%	0.004%
80	14.127	4067	4070	4073	rBV4	1462	1014	0.04%	0.006%




Sum of corrected areas: 17257223

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037527.D
Acq On : 25 Sep 2024 16:17
Operator : SY/MD
Sample : P4183-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FC3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

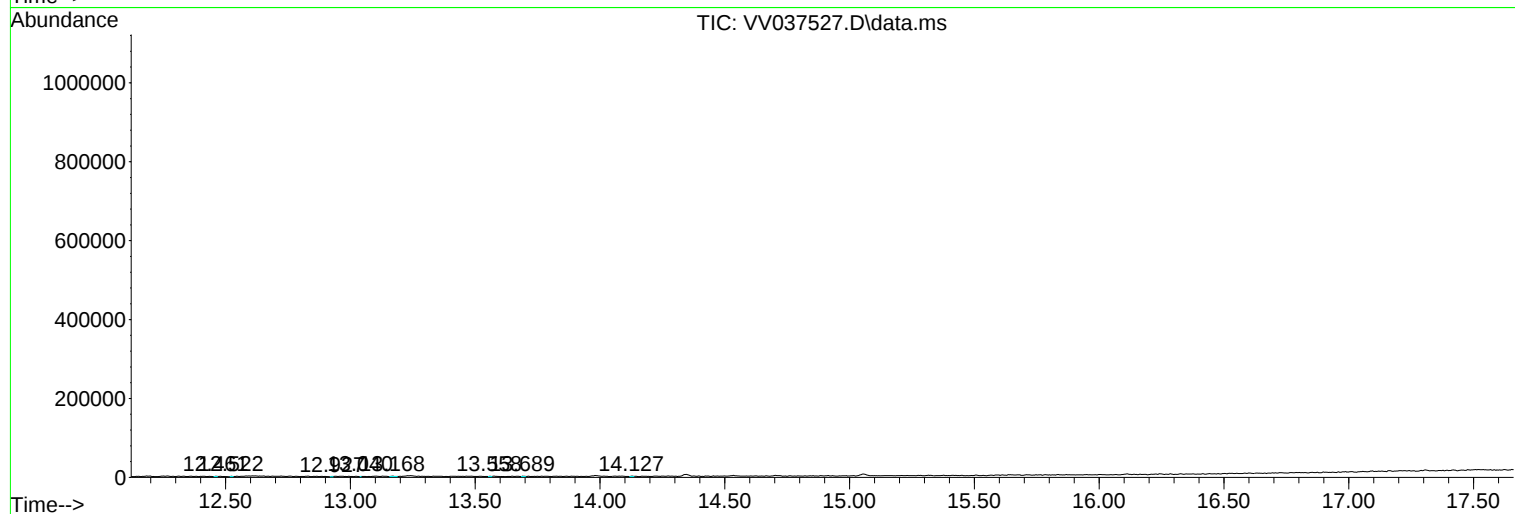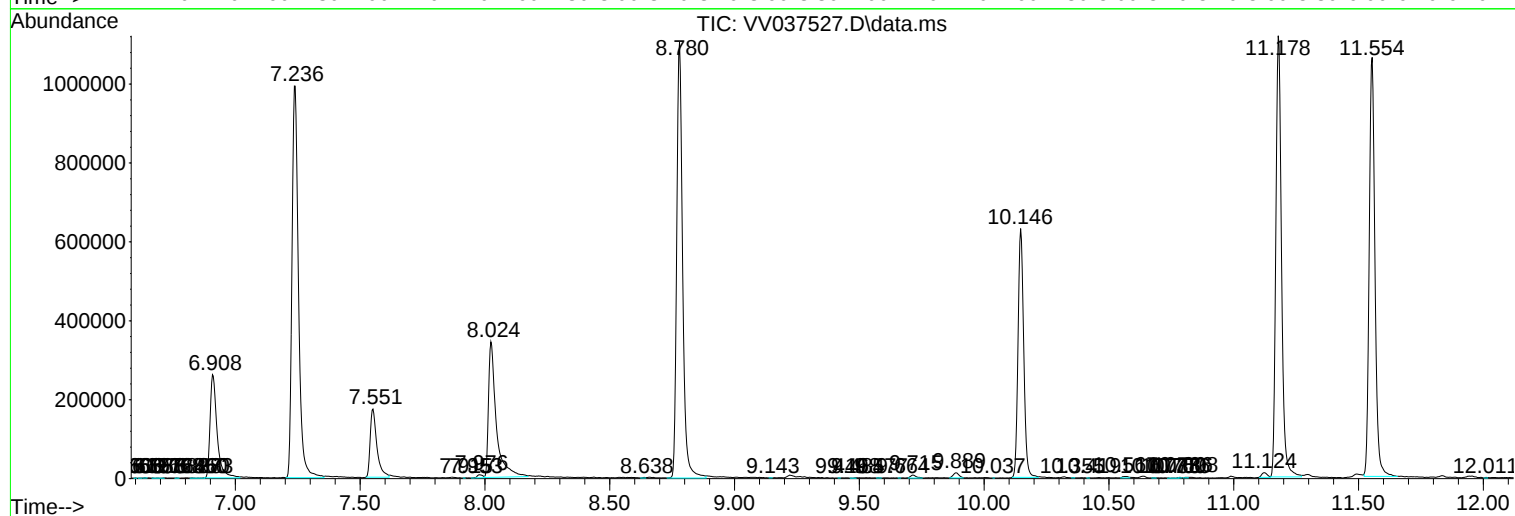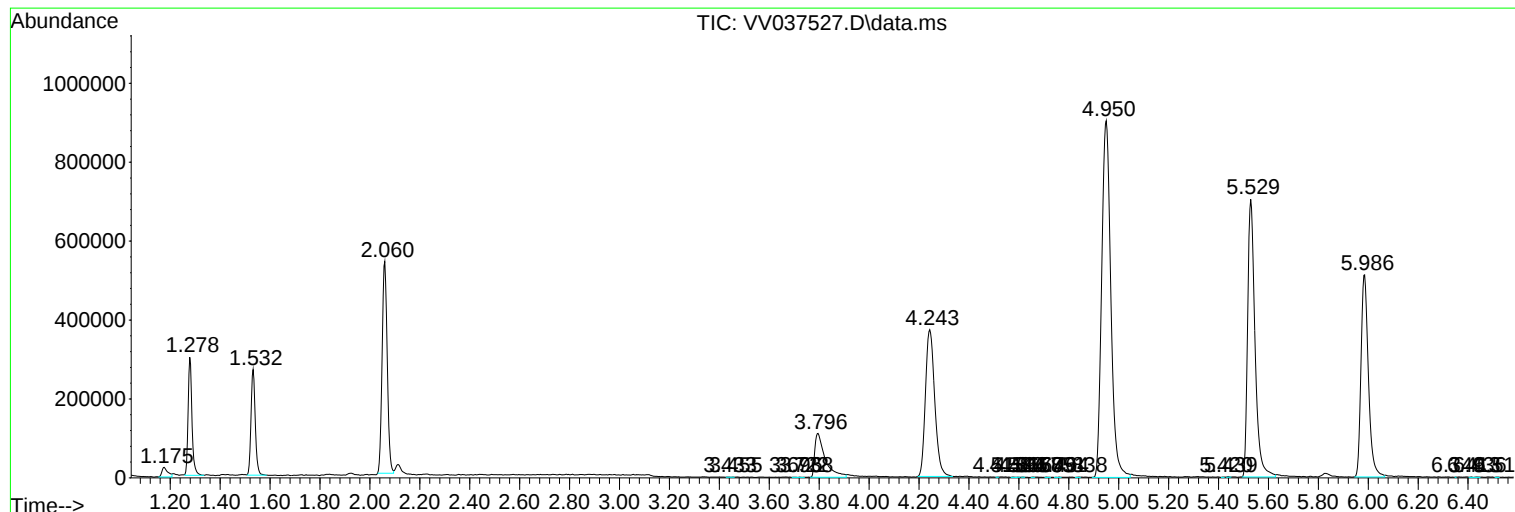

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037527.D
Acq On : 25 Sep 2024 16:17
Operator : SY/MD
Sample : P4183-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FC3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037527.D
Acq On : 25 Sep 2024 16:17
Operator : SY/MD
Sample : P4183-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FC3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------