

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037529.D
 Acq On : 25 Sep 2024 17:01
 Operator : SY/MD
 Sample : P4183-09
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037529.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	35	41	51	rBV	36550	54711	2.41%	0.324%
2	1.278	68	74	93	rVB	290472	312815	13.77%	1.855%
3	1.532	146	153	165	rVB	257064	300248	13.21%	1.780%
4	2.059	308	317	334	rVB	523572	751217	33.06%	4.454%
5	3.436	741	745	746	rBV3	764	438	0.02%	0.003%
6	3.596	792	795	797	rBV2	520	352	0.02%	0.002%
7	3.641	806	809	810	rBV2	356	243	0.01%	0.001%
8	3.670	815	818	819	rVV2	487	318	0.01%	0.002%
9	3.693	823	825	827	rVB3	618	263	0.01%	0.002%
10	3.712	827	831	835	rBV4	712	746	0.03%	0.004%
11	3.796	848	857	889	rBV	109589	306106	13.47%	1.815%
12	4.095	948	950	953	rBV2	777	458	0.02%	0.003%
13	4.243	982	996	1025	rVB	369444	925693	40.74%	5.489%
14	4.513	1078	1080	1083	rVB3	1076	455	0.02%	0.003%
15	4.628	1113	1116	1117	rBV2	427	209	0.01%	0.001%
16	4.699	1136	1138	1140	rBV2	344	166	0.01%	0.001%
17	4.828	1176	1178	1181	rBV3	683	350	0.02%	0.002%
18	4.892	1196	1198	1200	rBV2	473	202	0.01%	0.001%
19	4.950	1200	1216	1248	rBV2	894804	2272269	100.00%	13.473%
20	5.387	1350	1352	1353	rBV2	497	144	0.01%	0.001%
21	5.468	1373	1377	1381	rBV4	1259	997	0.04%	0.006%
22	5.529	1384	1396	1434	rBV	680028	1428987	62.89%	8.473%
23	5.937	1521	1523	1524	rBV3	701	165	0.01%	0.001%
24	5.985	1524	1538	1566	rBV	494754	1041455	45.83%	6.175%
25	6.329	1643	1645	1647	rBV3	552	274	0.01%	0.002%
26	6.355	1651	1653	1655	rBV2	572	271	0.01%	0.002%
27	6.397	1663	1666	1667	rBV3	644	335	0.01%	0.002%
28	6.500	1694	1698	1700	rVB3	704	453	0.02%	0.003%
29	6.513	1700	1702	1703	rBV	369	178	0.01%	0.001%
30	6.535	1707	1709	1715	rVB4	921	756	0.03%	0.004%
31	6.558	1715	1716	1718	rBV	488	264	0.01%	0.002%
32	6.596	1726	1728	1730	rBV	701	273	0.01%	0.002%
33	6.612	1730	1733	1735	rBV2	436	284	0.01%	0.002%
34	6.673	1750	1752	1755	rVB2	722	390	0.02%	0.002%
35	6.690	1755	1757	1758	rBV	508	213	0.01%	0.001%
36	6.718	1762	1766	1771	rBV5	1105	1047	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037529.D
 Acq On : 25 Sep 2024 17:01
 Operator : SY/MD
 Sample : P4183-09
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	6.754	1772	1777	1779	rBV4	878	777	0.03%	0.005%
38	6.767	1779	1781	1784	rBV3	932	445	0.02%	0.003%
39	6.815	1793	1796	1799	rBV4	876	531	0.02%	0.003%
40	6.908	1815	1825	1864	rBV	256362	505769	22.26%	2.999%
41	7.236	1917	1927	1955	rBV	989877	1751751	77.09%	10.386%
42	7.551	2016	2025	2050	rBV	174032	319789	14.07%	1.896%
43	7.966	2152	2154	2158	rBV3	730	523	0.02%	0.003%
44	7.988	2159	2161	2163	rBV2	461	137	0.01%	0.001%
45	8.024	2163	2172	2209	rBV2	332230	730750	32.16%	4.333%
46	8.709	2381	2385	2386	rBV2	489	264	0.01%	0.002%
47	8.718	2386	2388	2391	rBV2	890	522	0.02%	0.003%
48	8.779	2395	2407	2437	rBV	1060099	1764232	77.64%	10.460%
49	9.120	2511	2513	2514	rBV2	793	316	0.01%	0.002%
50	9.345	2581	2583	2585	rBV2	458	220	0.01%	0.001%
51	9.361	2585	2588	2589	rBV	776	349	0.02%	0.002%
52	9.384	2594	2595	2596	rBV	636	226	0.01%	0.001%
53	9.410	2601	2603	2605	rBV3	677	372	0.02%	0.002%
54	9.468	2617	2621	2625	rVB4	860	705	0.03%	0.004%
55	9.493	2627	2629	2631	rBV2	674	371	0.02%	0.002%
56	9.529	2638	2640	2644	rVB4	771	482	0.02%	0.003%
57	9.577	2650	2655	2656	rBV2	611	442	0.02%	0.003%
58	9.722	2698	2700	2701	rBV	780	414	0.02%	0.002%
59	9.767	2712	2714	2715	rBV	604	250	0.01%	0.001%
60	9.805	2723	2726	2727	rBV2	471	202	0.01%	0.001%
61	9.818	2727	2730	2731	rBV	373	186	0.01%	0.001%
62	9.857	2740	2742	2747	rBV5	379	262	0.01%	0.002%
63	9.934	2765	2766	2769	rVB2	339	180	0.01%	0.001%
64	9.953	2769	2772	2774	rBV3	401	282	0.01%	0.002%
65	9.985	2780	2782	2783	rBV	369	143	0.01%	0.001%
66	10.030	2794	2796	2799	rVB3	773	362	0.02%	0.002%
67	10.050	2799	2802	2804	rBV2	460	292	0.01%	0.002%
68	10.062	2804	2806	2809	rVB2	525	256	0.01%	0.002%
69	10.082	2809	2812	2813	rBV2	353	177	0.01%	0.001%
70	10.146	2820	2832	2858	rBV	625980	997220	43.89%	5.913%
71	10.435	2920	2922	2926	rVB2	781	332	0.01%	0.002%
72	10.458	2926	2929	2932	rVB3	526	344	0.02%	0.002%
73	10.474	2932	2934	2939	rBV3	866	734	0.03%	0.004%
74	10.496	2939	2941	2942	rBV2	770	335	0.01%	0.002%
75	10.580	2961	2967	2969	rBV5	902	880	0.04%	0.005%
76	10.606	2973	2975	2977	rBV2	380	168	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037529.D
 Acq On : 25 Sep 2024 17:01
 Operator : SY/MD
 Sample : P4183-09
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	10.725	3010	3012	3018	rBV5	776	676	0.03%	0.004%
78	10.760	3021	3023	3026	rBV3	541	284	0.01%	0.002%
79	10.779	3028	3029	3030	rBV3	531	158	0.01%	0.001%
80	10.853	3050	3052	3054	rBV2	711	363	0.02%	0.002%
81	10.921	3070	3073	3075	rBV2	586	355	0.02%	0.002%
82	10.953	3079	3083	3085	rBV3	491	408	0.02%	0.002%
83	11.069	3114	3119	3120	rBV5	605	458	0.02%	0.003%
84	11.178	3141	3153	3184	rBV	1054928	1706925	75.12%	10.121%
85	11.554	3257	3270	3295	rBV	1038700	1661715	73.13%	9.853%
86	12.387	3527	3529	3532	rBV2	692	458	0.02%	0.003%
87	12.419	3536	3539	3541	rBV2	582	433	0.02%	0.003%
88	12.564	3581	3584	3585	rBV	846	505	0.02%	0.003%
89	12.889	3680	3685	3690	rBV5	922	957	0.04%	0.006%
90	12.911	3690	3692	3696	rVB4	1018	597	0.03%	0.004%
91	12.940	3696	3701	3703	rBV5	1207	983	0.04%	0.006%
92	12.988	3714	3716	3719	rVB2	651	273	0.01%	0.002%
93	13.024	3725	3727	3729	rBV	611	291	0.01%	0.002%
94	13.056	3735	3737	3739	rBV	589	363	0.02%	0.002%
95	13.114	3752	3755	3762	rBV6	1291	1246	0.05%	0.007%
96	13.201	3779	3782	3787	rBV3	564	520	0.02%	0.003%
97	13.512	3877	3879	3881	rBV2	949	515	0.02%	0.003%
98	13.747	3950	3952	3954	rBV2	929	459	0.02%	0.003%
99	13.869	3989	3990	3994	rVB3	895	395	0.02%	0.002%
100	14.120	4065	4068	4070	rBV3	1181	728	0.03%	0.004%




Sum of corrected areas: 16865802

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037529.D
Acq On : 25 Sep 2024 17:01
Operator : SY/MD
Sample : P4183-09
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

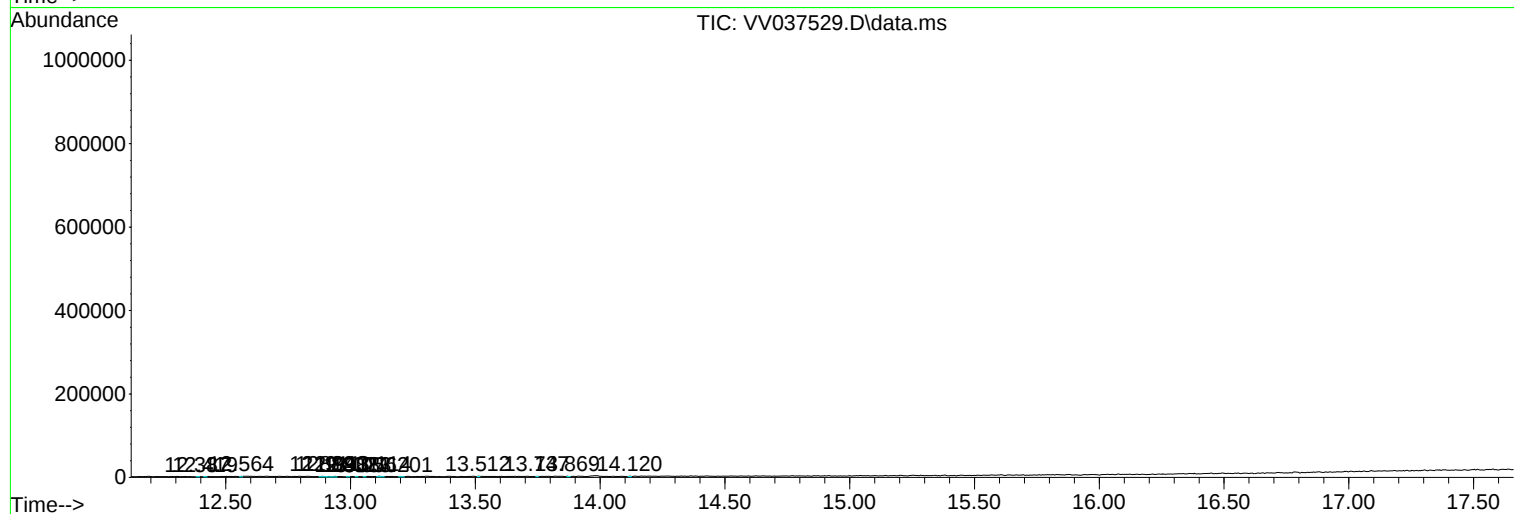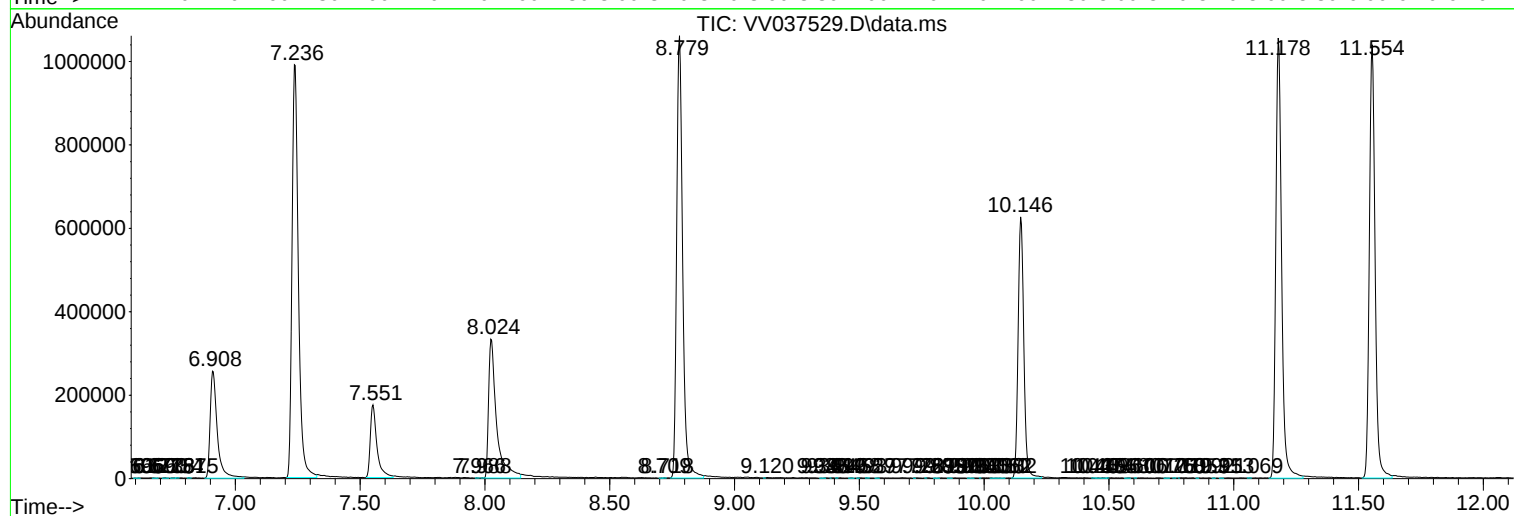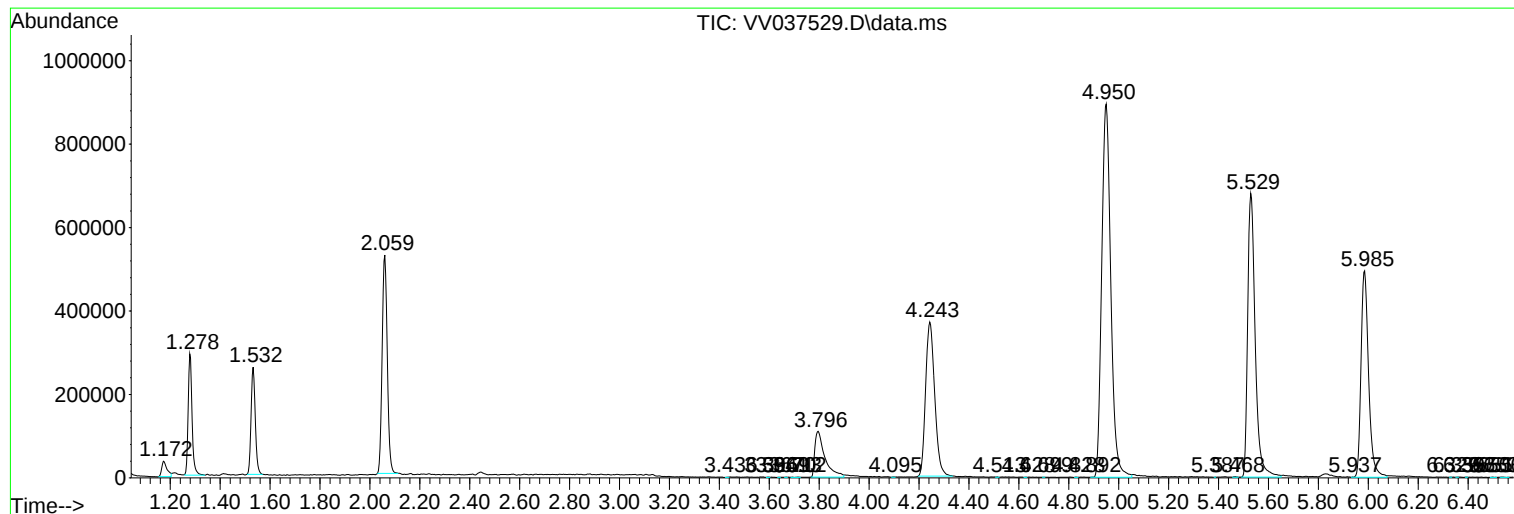

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037529.D
Acq On : 25 Sep 2024 17:01
Operator : SY/MD
Sample : P4183-09
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037529.D
Acq On : 25 Sep 2024 17:01
Operator : SY/MD
Sample : P4183-09
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------