

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037530.D
 Acq On : 25 Sep 2024 17:22
 Operator : SY/MD
 Sample : VIBLK389
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK389

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037530.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	52	rBV	19748	32678	1.42%	0.190%
2	1.278	68	74	88	rBV	291446	308164	13.42%	1.793%
3	1.532	146	153	168	rVB	261806	305974	13.33%	1.781%
4	2.060	307	317	340	rBV	526858	768056	33.45%	4.469%
5	3.442	745	747	748	rBV2	651	295	0.01%	0.002%
6	3.474	755	757	760	rBV	576	247	0.01%	0.001%
7	3.513	766	769	777	rVB5	1332	941	0.04%	0.005%
8	3.593	792	794	797	rBV3	829	445	0.02%	0.003%
9	3.645	805	810	811	rBV2	591	480	0.02%	0.003%
10	3.677	816	820	822	rVV3	570	441	0.02%	0.003%
11	3.757	843	845	847	rBV2	370	183	0.01%	0.001%
12	3.796	847	857	884	rBV2	109623	315141	13.73%	1.834%
13	4.243	980	996	1025	rBV	372923	957190	41.69%	5.570%
14	4.535	1086	1087	1091	rVB3	846	440	0.02%	0.003%
15	4.654	1122	1124	1126	rBV3	854	439	0.02%	0.003%
16	4.728	1143	1147	1150	rBV4	1073	830	0.04%	0.005%
17	4.764	1157	1158	1159	rVB	245	47	0.00%	0.000%
18	4.806	1168	1171	1173	rVB3	688	325	0.01%	0.002%
19	4.831	1178	1179	1182	rBV2	405	159	0.01%	0.001%
20	4.844	1182	1183	1185	rVB	731	196	0.01%	0.001%
21	4.863	1185	1189	1191	rBV2	1002	712	0.03%	0.004%
22	4.950	1199	1216	1249	rBV2	899463	2295789	100.00%	13.360%
23	5.416	1358	1361	1368	rVB6	1276	1494	0.07%	0.009%
24	5.449	1368	1371	1374	rBV5	804	765	0.03%	0.004%
25	5.529	1384	1396	1434	rBV	716411	1476823	64.33%	8.594%
26	5.986	1524	1538	1573	rBV	503841	1065020	46.39%	6.198%
27	6.355	1651	1653	1654	rBV	822	332	0.01%	0.002%
28	6.478	1689	1691	1697	rVB4	1000	886	0.04%	0.005%
29	6.510	1697	1701	1703	rVB3	829	475	0.02%	0.003%
30	6.526	1703	1706	1709	rBV3	710	467	0.02%	0.003%
31	6.542	1709	1711	1713	rBV4	533	221	0.01%	0.001%
32	6.571	1718	1720	1726	rVB4	857	681	0.03%	0.004%
33	6.596	1726	1728	1729	rBV	69	31	0.00%	0.000%
34	6.606	1729	1731	1734	rBV	581	420	0.02%	0.002%
35	6.680	1751	1754	1757	rBV3	666	371	0.02%	0.002%
36	6.699	1757	1760	1764	rBV4	1051	977	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037530.D
 Acq On : 25 Sep 2024 17:22
 Operator : SY/MD
 Sample : VIBLK389
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK389

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	6.773	1781	1783	1785	rBV3	523	239	0.01%	0.001%
38	6.805	1791	1793	1795	rBV	437	220	0.01%	0.001%
39	6.818	1795	1797	1799	rBV2	433	257	0.01%	0.001%
40	6.828	1799	1800	1802	rVB2	805	301	0.01%	0.002%
41	6.841	1802	1804	1806	rVB2	364	131	0.01%	0.001%
42	6.854	1806	1808	1811	rVB2	352	142	0.01%	0.001%
43	6.908	1811	1825	1852	rBV	263622	505210	22.01%	2.940%
44	7.236	1916	1927	1957	rBV	985887	1770832	77.13%	10.305%
45	7.551	2016	2025	2051	rBV	174057	326017	14.20%	1.897%
46	7.953	2147	2150	2152	rBV2	743	405	0.02%	0.002%
47	7.979	2156	2158	2160	rBV	661	295	0.01%	0.002%
48	8.024	2163	2172	2213	rBV2	334842	745507	32.47%	4.338%
49	8.738	2391	2394	2396	rBV3	705	447	0.02%	0.003%
50	8.780	2396	2407	2444	rBV	1090699	1831100	79.76%	10.655%
51	9.117	2510	2512	2515	rBV4	1110	607	0.03%	0.004%
52	9.329	2575	2578	2579	rBV2	885	356	0.02%	0.002%
53	9.368	2584	2590	2593	rBV5	978	1061	0.05%	0.006%
54	9.455	2614	2617	2621	rVB4	802	467	0.02%	0.003%
55	9.522	2636	2638	2639	rBV	381	159	0.01%	0.001%
56	9.567	2650	2652	2655	rVB3	482	283	0.01%	0.002%
57	9.641	2672	2675	2677	rBV3	1110	759	0.03%	0.004%
58	9.683	2685	2688	2690	rBV2	780	492	0.02%	0.003%
59	9.876	2746	2748	2751	rBV3	474	333	0.01%	0.002%
60	9.931	2763	2765	2768	rBV2	397	316	0.01%	0.002%
61	10.046	2797	2801	2807	rVB3	1027	964	0.04%	0.006%
62	10.072	2807	2809	2811	rBV2	593	273	0.01%	0.002%
63	10.146	2819	2832	2856	rBV	641383	1009409	43.97%	5.874%
64	10.397	2908	2910	2911	rBV	439	166	0.01%	0.001%
65	10.468	2930	2932	2934	rBV3	488	260	0.01%	0.002%
66	10.519	2946	2948	2952	rVB4	908	457	0.02%	0.003%
67	10.555	2955	2959	2967	rVB6	634	940	0.04%	0.005%
68	10.680	2996	2998	3001	rVB2	658	251	0.01%	0.001%
69	10.712	3006	3008	3012	rVB3	746	427	0.02%	0.002%
70	10.747	3012	3019	3022	rBV3	746	889	0.04%	0.005%
71	10.770	3022	3026	3028	rBV4	638	517	0.02%	0.003%
72	10.805	3034	3037	3039	rBV2	379	225	0.01%	0.001%
73	10.821	3039	3042	3043	rBV2	867	483	0.02%	0.003%
74	10.915	3068	3071	3076	rBV3	903	820	0.04%	0.005%
75	11.008	3095	3100	3102	rBV4	640	499	0.02%	0.003%
76	11.069	3115	3119	3121	rBV	683	518	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037530.D
 Acq On : 25 Sep 2024 17:22
 Operator : SY/MD
 Sample : VIBLK389
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK389

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

77	11.104	3126	3130	3135	rVB3	665	722	0.03%	0.004%
78	11.127	3135	3137	3138	rBV	761	315	0.01%	0.002%
79	11.178	3142	3153	3183	rBV	1109308	1755015	76.44%	10.213%
80	11.554	3258	3270	3301	rBV	1052998	1682707	73.30%	9.792%
81	11.972	3398	3400	3402	rVB3	886	344	0.01%	0.002%
82	12.178	3460	3464	3468	rBV5	1052	1021	0.04%	0.006%
83	13.149	3763	3766	3768	rBV3	662	502	0.02%	0.003%
84	13.197	3778	3781	3782	rBV2	448	231	0.01%	0.001%
85	13.297	3810	3812	3814	rBV2	785	444	0.02%	0.003%
86	13.400	3841	3844	3846	rBV4	949	704	0.03%	0.004%
87	13.464	3861	3864	3867	rBV4	1186	728	0.03%	0.004%
88	13.937	4008	4011	4014	rBV4	1147	711	0.03%	0.004%




Sum of corrected areas: 17184613

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037530.D
Acq On : 25 Sep 2024 17:22
Operator : SY/MD
Sample : VIBLK389
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK389

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

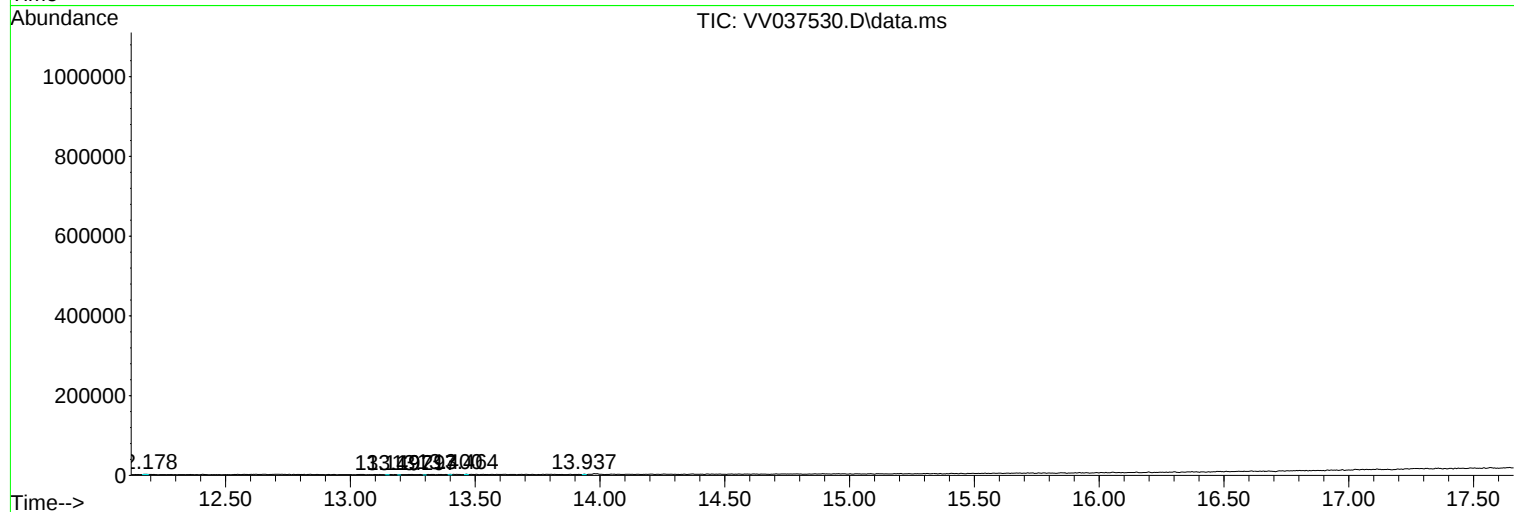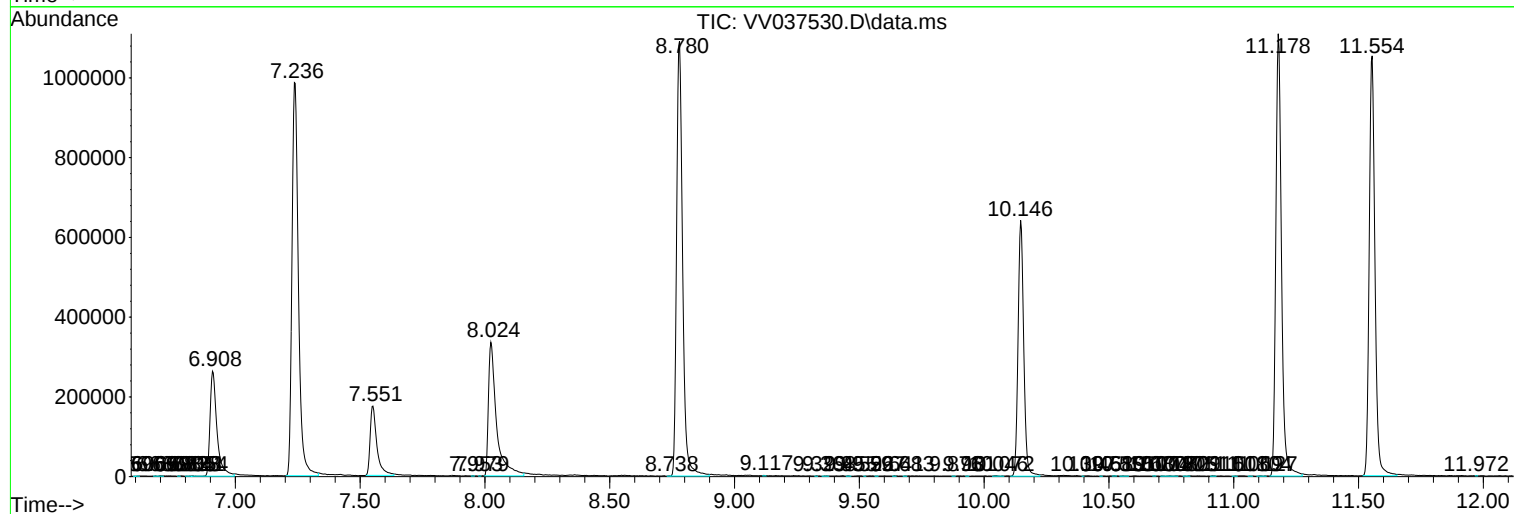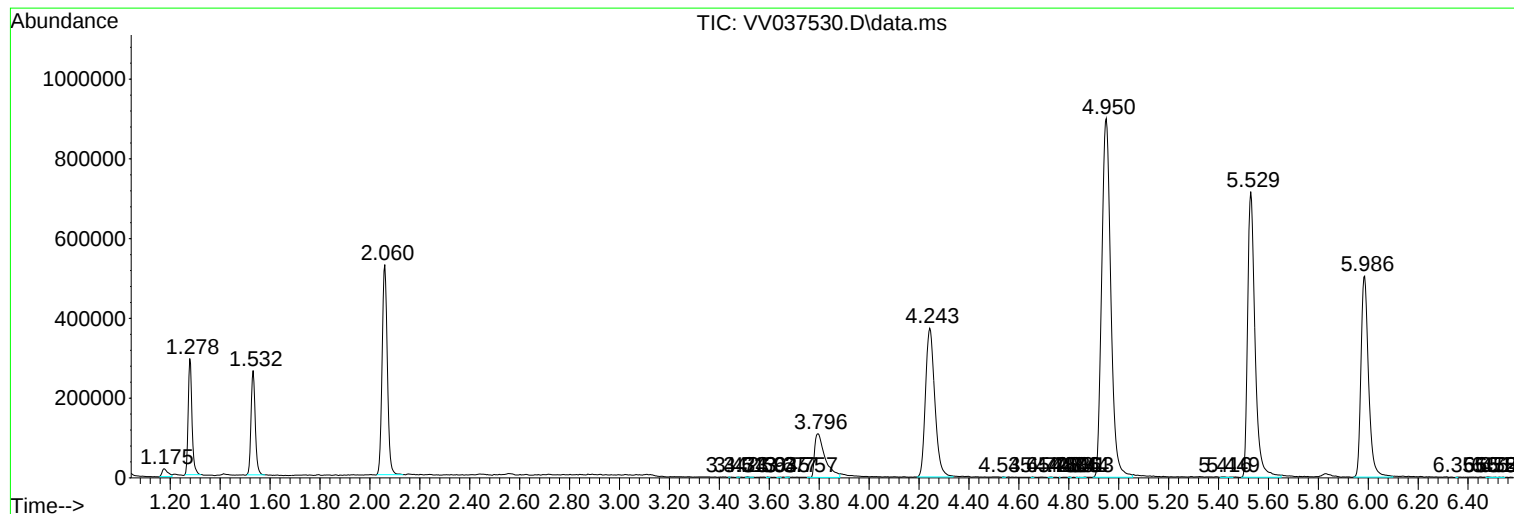

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037530.D
Acq On : 25 Sep 2024 17:22
Operator : SY/MD
Sample : VIBLK389
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK389

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037530.D
Acq On : 25 Sep 2024 17:22
Operator : SY/MD
Sample : VIBLK389
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK389

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------