
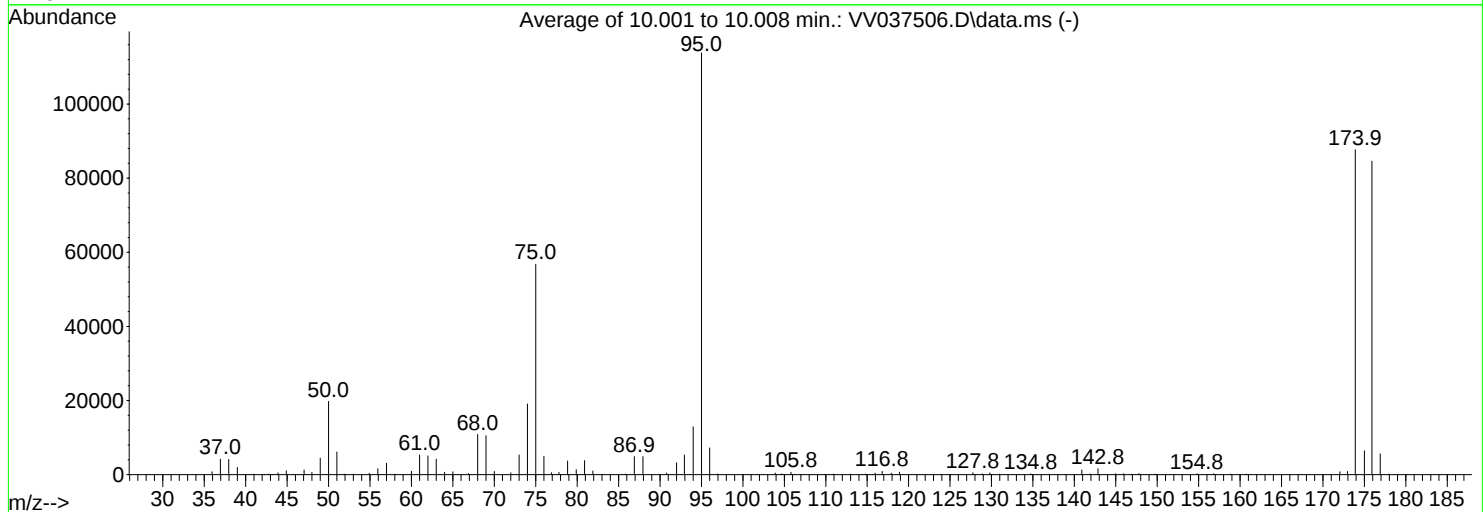


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037506.D
Acq On : 25 Sep 2024 07:53
Operator : SY/MD
Sample : BFB380
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB380

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Title : VOC Analysis
Last Update : Thu Sep 26 04:08:51 2024

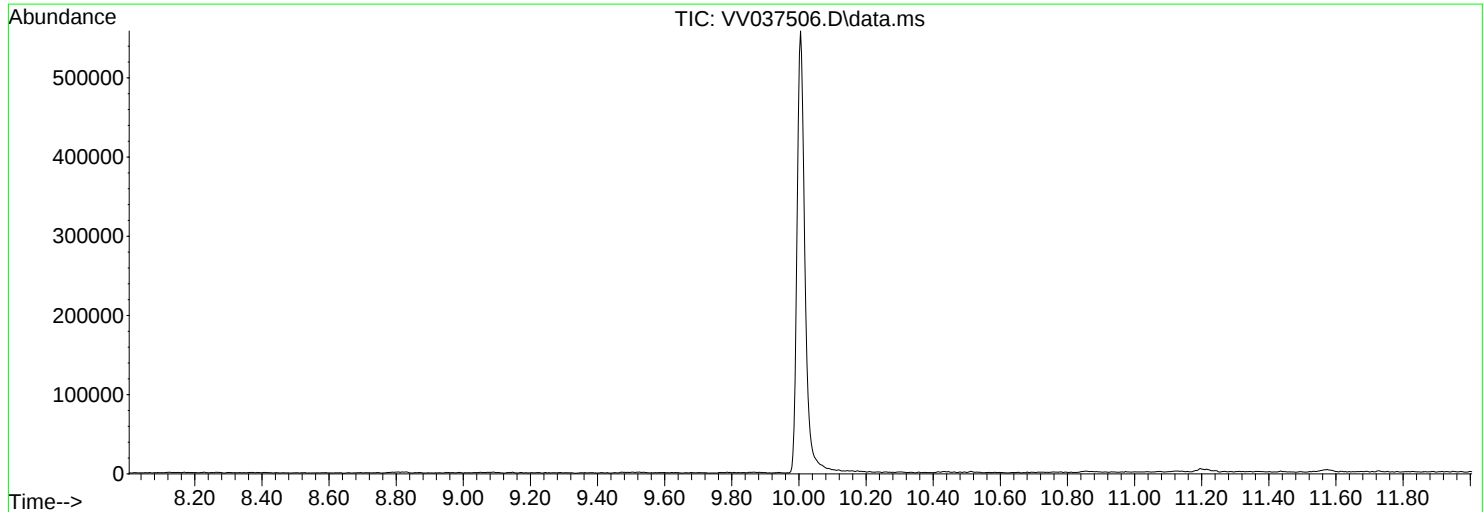

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	19763	PASS
75	95	30	80	49.9	56784	PASS
95	95	100	100	100.0	113811	PASS
96	95	5	9	6.3	7218	PASS
173	174	0.00	2	1.0	871	PASS
174	95	50	120	77.1	87693	PASS
175	174	5	9	7.3	6443	PASS
176	174	95	105	96.4	84560	PASS
177	176	5	10	6.6	5598	PASS

m/z	Abundance
36.90	128.0
37.90	112.0
39.90	279.0
41.90	140.0
44.00	609.0
76.90	150.0

Instrument :
MSVOA_V
ClientSampleId :
BFB380

m/z	Abundance
35.90	781.0
37.00	4613.0
38.00	4510.0
39.00	1945.0
39.90	281.0
41.00	146.0
42.30	113.0
42.80	168.0
43.20	183.0
43.90	1151.0
44.90	1037.0
47.00	1116.0
48.00	636.0
49.00	4466.0
50.00	20160.0
51.00	6141.0
51.90	296.0
53.00	184.0
54.80	321.0
56.00	1683.0
57.00	3249.0
58.00	129.0
60.00	939.0
61.00	5514.0
62.00	5019.0
63.00	4058.0
64.00	797.0
65.00	690.0
66.90	272.0
68.00	10880.0
69.00	10463.0
70.00	877.0
72.00	492.0
73.00	5247.0
74.00	19512.0
75.00	56272.0
76.00	4988.0
77.00	646.0
77.80	583.0
78.80	3535.0
79.90	1438.0
80.90	3741.0
81.90	1046.0
85.90	173.0
86.90	4891.0
87.90	4996.0
90.80	455.0
92.00	3266.0
92.90	5369.0
94.00	13042.0
95.00	111304.0
96.00	7375.0
97.00	247.0
103.80	505.0
104.70	226.0
105.80	581.0
110.90	126.0
112.90	154.0
114.80	182.0
116.00	453.0
116.80	836.0
117.90	457.0
118.90	674.0
127.80	555.0
128.90	172.0
129.80	404.0
131.10	188.0
134.70	202.0
136.90	152.0
138.80	104.0
140.90	1182.0
141.90	220.0
142.80	1512.0
144.90	276.0
145.90	248.0
147.00	123.0
147.80	311.0
149.70	151.0
154.90	294.0
156.80	273.0
158.90	136.0
160.80	108.0
172.00	785.0
173.00	878.0
173.90	83280.0
175.00	6442.0
175.90	80624.0
176.90	5556.0
177.90	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB380

m/z	Abundance
36.00	813.0
37.00	4431.0
38.00	4389.0
39.00	2060.0
40.00	280.0
41.00	162.0
42.30	119.0
42.80	170.0
43.90	1085.0
44.90	1122.0
47.10	1231.0
48.00	610.0
49.00	4639.0
50.00	20520.0
51.00	6291.0
51.90	257.0
53.00	209.0
54.90	350.0
55.90	1645.0
57.00	3200.0
57.90	131.0
60.00	911.0
61.00	5502.0
62.00	5247.0
63.00	4358.0
64.00	684.0
65.00	811.0
66.90	302.0
68.00	11379.0
69.00	10777.0
70.00	865.0
72.00	487.0
73.00	5485.0
74.00	19848.0
75.00	58760.0
76.00	5133.0
77.00	653.0
77.80	645.0
78.90	3761.0
79.90	1436.0
80.90	3859.0
81.90	1044.0
85.80	178.0
86.90	5004.0
87.90	4980.0
90.80	459.0
92.00	3221.0
93.00	5514.0
94.00	13203.0
95.00	118320.0
96.00	7416.0
97.00	235.0
103.90	456.0
104.70	206.0
105.80	647.0
107.00	110.0
109.90	104.0
110.90	202.0
113.00	176.0
114.80	171.0
116.00	465.0
116.80	926.0
117.90	388.0
118.90	694.0
124.90	113.0
127.80	551.0
128.90	230.0
129.80	493.0
131.00	164.0
134.80	225.0
137.00	190.0
140.90	1303.0
141.90	244.0
142.80	1629.0
145.00	250.0
145.90	256.0
146.90	149.0
147.80	309.0
149.70	180.0
154.80	268.0
156.80	277.0
158.90	151.0
160.70	156.0
172.10	814.0
172.90	872.0
173.90	90968.0
175.00	6630.0
175.90	87952.0
176.90	5774.0
178.00	208.0

Instrument :
MSVOA_V
ClientSampleId :
BFB380

m/z	Abundance
36.00	773.0
37.00	3897.0
38.00	3762.0
39.00	1857.0
40.00	297.0
41.00	152.0
42.30	102.0
42.80	157.0
43.90	1073.0
44.90	1018.0
47.00	1354.0
48.00	520.0
49.00	4308.0
50.00	18608.0
51.00	6026.0
52.10	280.0
53.00	164.0
55.00	371.0
55.90	1531.0
57.00	2789.0
57.90	135.0
60.00	836.0
61.00	4871.0
62.00	4912.0
63.00	4185.0
64.00	435.0
65.00	805.0
66.90	354.0
68.00	10335.0
69.00	10436.0
70.00	835.0
72.00	536.0
73.00	5262.0
74.00	17952.0
75.00	55320.0
76.00	4696.0
76.90	691.0
77.80	600.0
78.90	3660.0
79.90	1163.0
80.90	3774.0
81.90	925.0
85.80	187.0
86.90	4766.0
88.00	4625.0
90.80	379.0
92.00	3062.0
93.00	5115.0
94.00	12476.0
95.00	111808.0
96.00	6862.0
96.90	201.0
104.00	369.0
104.70	166.0
105.10	126.0
105.80	657.0
110.90	209.0
113.00	141.0
114.80	143.0
115.90	395.0
116.80	1003.0
117.90	360.0
118.90	699.0
123.90	108.0
127.70	468.0
128.90	253.0
129.80	568.0
130.90	128.0
134.80	259.0
136.90	202.0
140.90	1308.0
141.90	187.0
142.90	1599.0
145.00	242.0
145.90	248.0
146.80	140.0
147.80	267.0
149.80	154.0
154.70	239.0
156.80	197.0
158.80	176.0
160.70	191.0
170.90	107.0
172.10	737.0
172.90	863.0
173.90	88832.0
175.00	6258.0
175.90	85104.0
176.90	5463.0
178.00	204.0

Instrument :
MSVOA_V
ClientSampleId :
BFB380