

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092525\
 Data File : VV039188.D
 Acq On : 25 Sep 2025 17:47
 Operator : SY/MD
 Sample : Q3195-24
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EB-02-092225

Quant Time: Sep 26 01:35:14 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 24 08:08:08 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	4.603	168	315041	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	5.535	114	553359	50.000	ug/l	0.00
63) Chlorobenzene-d5	8.776	117	549470	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.175	152	261018	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	4.944	65	252908	55.467	ug/l	0.00
Spiked Amount	50.000	Range	81 - 118	Recovery	=	110.940%
35) Dibromofluoromethane	4.503	113	229182	51.518	ug/l	0.00
Spiked Amount	50.000	Range	80 - 119	Recovery	=	103.040%
50) Toluene-d8	7.240	98	600984	45.998	ug/l	0.00
Spiked Amount	50.000	Range	89 - 112	Recovery	=	92.000%
62) 4-Bromofluorobenzene	10.005	95	234432	43.585	ug/l	0.00
Spiked Amount	50.000	Range	85 - 114	Recovery	=	87.180%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092525\
Data File : VV039188.D
Acq On : 25 Sep 2025 17:47
Operator : SY/MD
Sample : Q3195-24
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EB-02-092225

Quant Time: Sep 26 01:35:14 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 24 08:08:08 2025
Response via : Initial Calibration




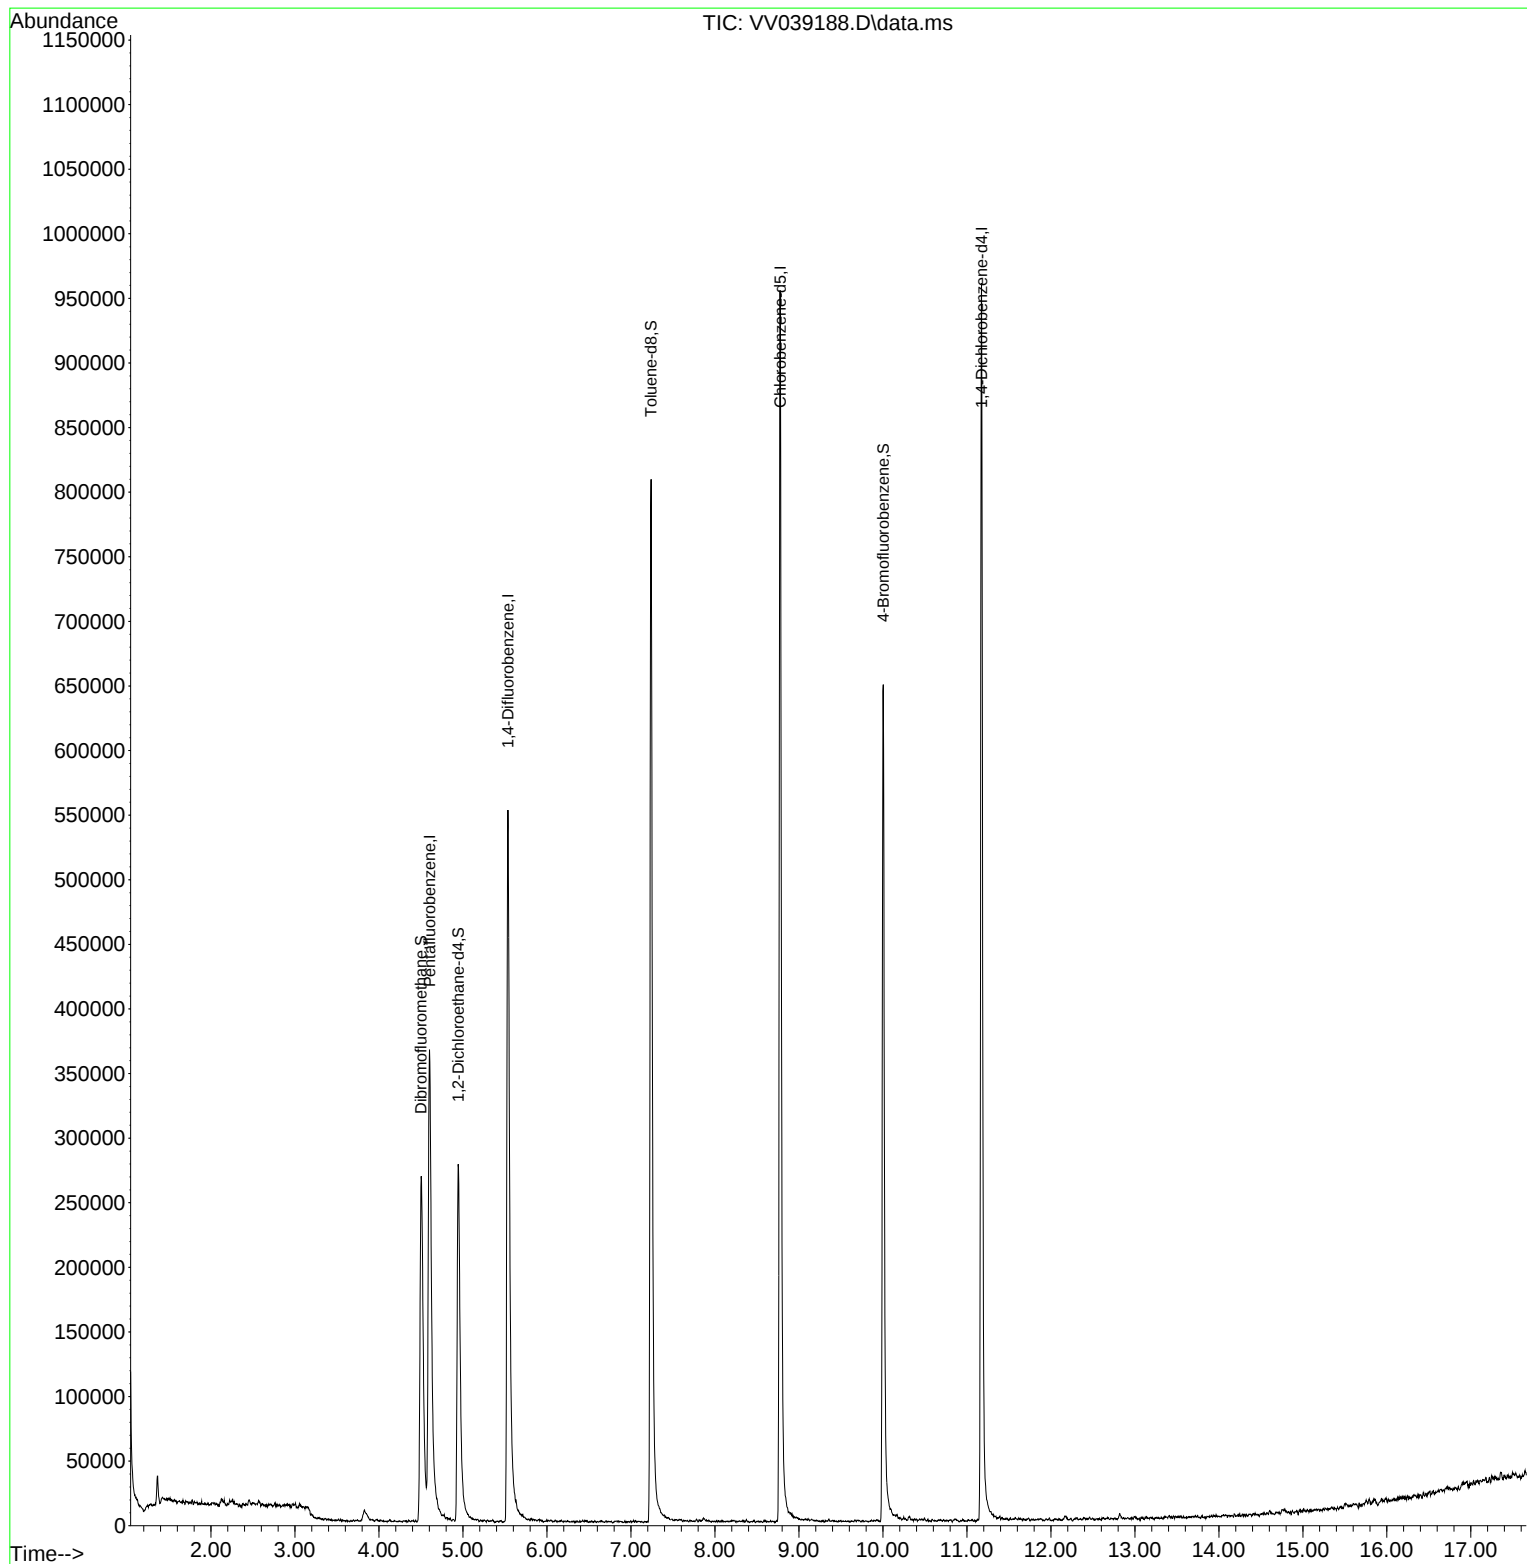


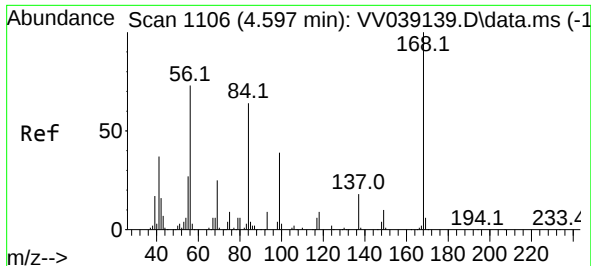

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 4.603 min Scan# 1106
Delta R.T. 0.006 min
Lab File: VV039188.D
Acq: 25 Sep 2025 17:47




Instrument :
MSVOA_V
ClientSampleId :
EB-02-092225


Tgt Ion:168 Resp: 315041
Ion Ratio Lower Upper
168 100
99 62.7 49.6 74.4

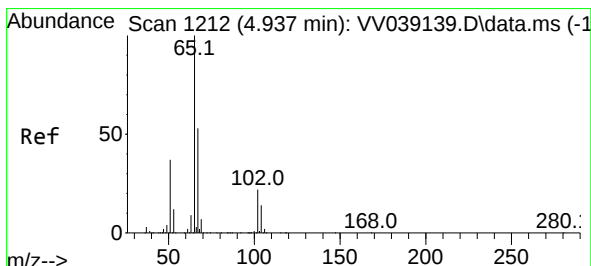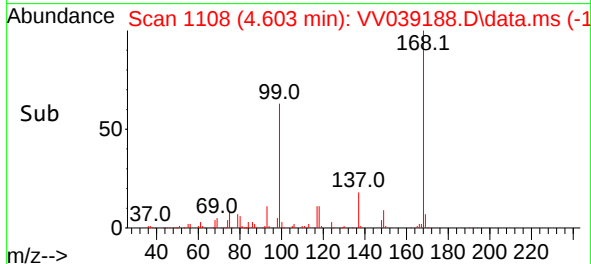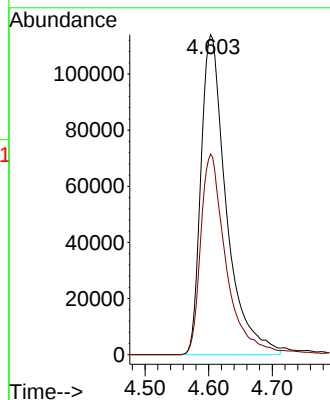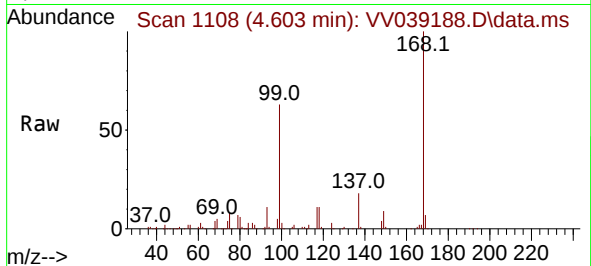

#33
1,2-Dichloroethane-d4
Concen: 55.467 ug/l
RT: 4.944 min Scan# 1214
Delta R.T. 0.006 min
Lab File: VV039188.D
Acq: 25 Sep 2025 17:47

Tgt Ion: 65 Resp: 252908
Ion Ratio Lower Upper
65 100
67 52.3 0.0 107.0

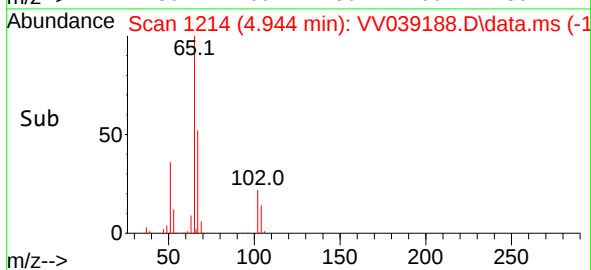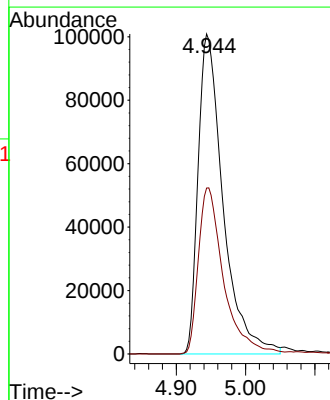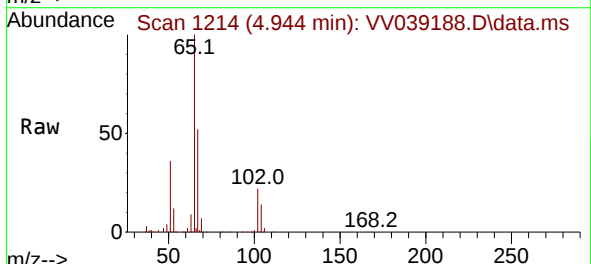

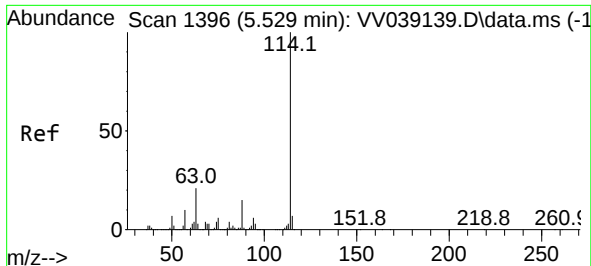

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 5.535 min Scan# 114

Delta R.T. 0.006 min

Lab File: VV039188.D

Acq: 25 Sep 2025 17:47

Instrument :

MSVOA_V

ClientSampleId :

EB-02-092225





Tgt Ion:114 Resp: 553359

Ion Ratio Lower Upper

114 100

63 20.8 0.0 42.6

88 15.4 0.0 30.8

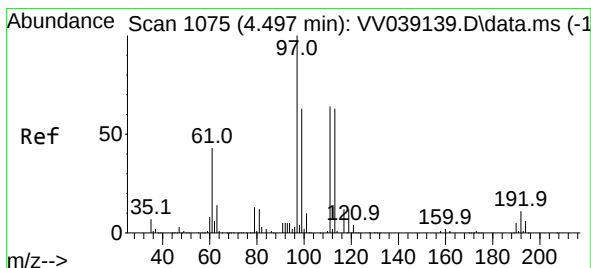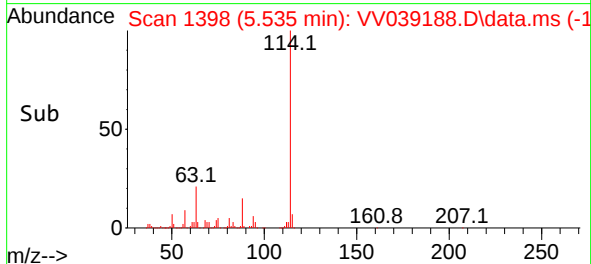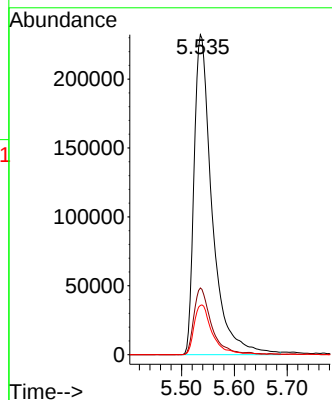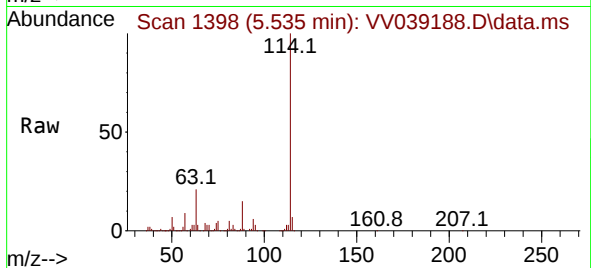

#35

Dibromofluoromethane

Concen: 51.518 ug/l

RT: 4.503 min Scan# 1077

Delta R.T. 0.006 min

Lab File: VV039188.D

Acq: 25 Sep 2025 17:47




Tgt Ion:113 Resp: 229182


Ion Ratio Lower Upper

113 100

111 102.3 82.4 123.6

192 17.8 13.8 20.8


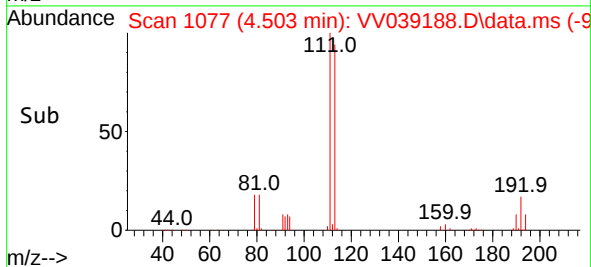
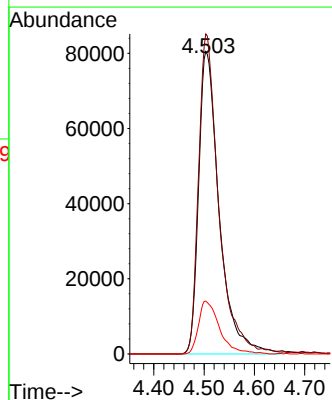
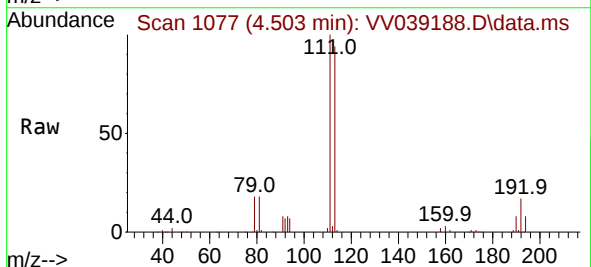


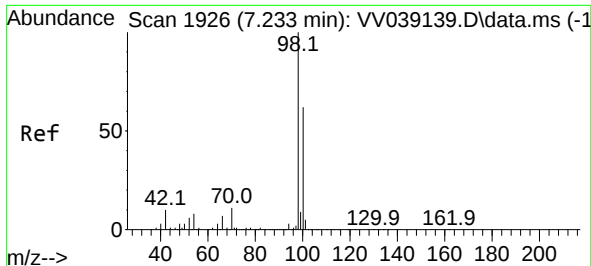

#50
Toluene-d8
Concen: 45.998 ug/l
RT: 7.240 min Scan# 1926
Delta R.T. 0.006 min
Lab File: VV039188.D
Acq: 25 Sep 2025 17:47




Instrument :
MSVOA_V
ClientSampleId :
EB-02-092225


Tgt Ion: 98 Resp: 600984
Ion Ratio Lower Upper
98 100
100 64.3 52.2 78.2

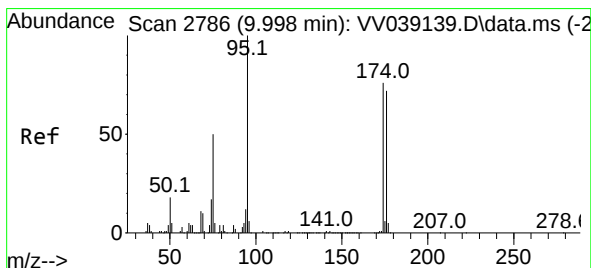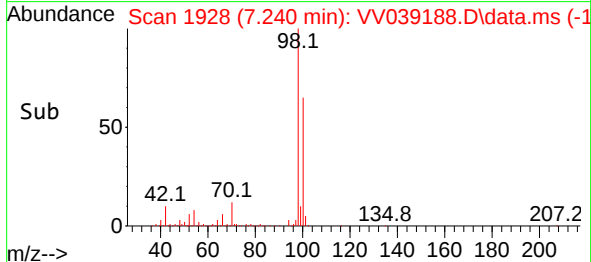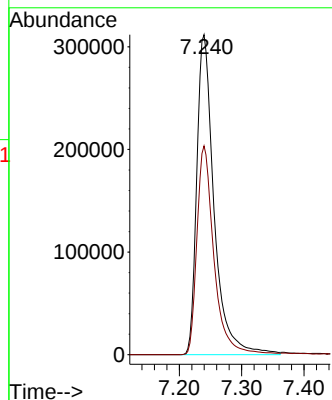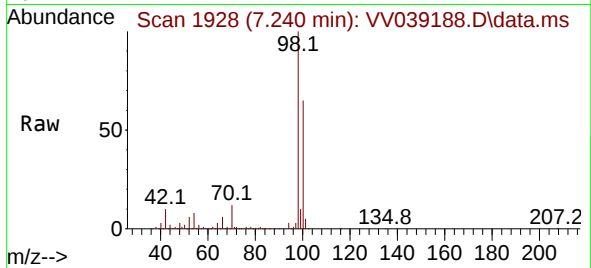

#62
4-Bromofluorobenzene
Concen: 43.585 ug/l
RT: 10.005 min Scan# 2788
Delta R.T. 0.006 min
Lab File: VV039188.D
Acq: 25 Sep 2025 17:47

Tgt Ion: 95 Resp: 234432
Ion Ratio Lower Upper
95 100
174 74.0 0.0 150.4
176 72.7 0.0 144.2


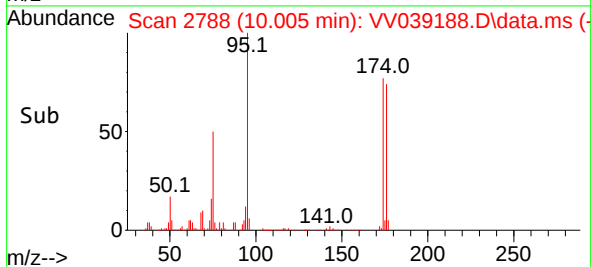
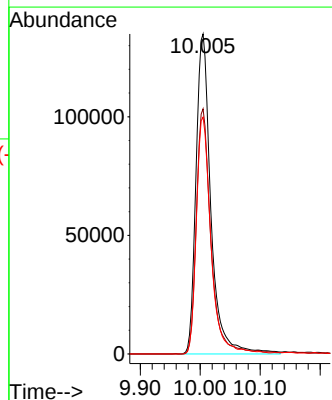
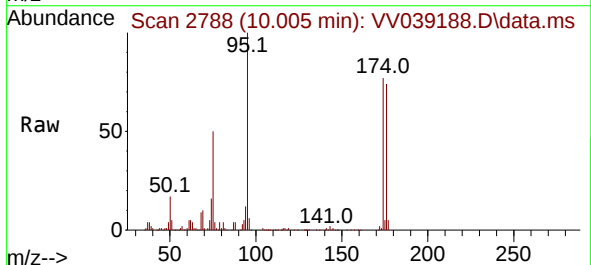


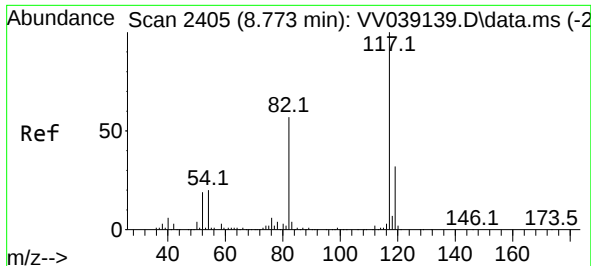

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 8.776 min Scan# 2405
Delta R.T. 0.003 min
Lab File: VV039188.D
Acq: 25 Sep 2025 17:47

Instrument :
MSVOA_V
ClientSampleId :
EB-02-092225

Tgt Ion:117 Resp: 549470
Ion Ratio Lower Upper
117 100
82 56.1 45.4 68.2
119 33.0 25.6 38.4

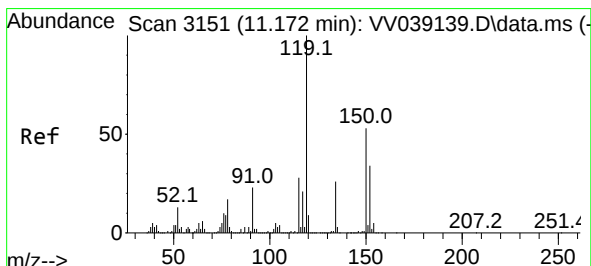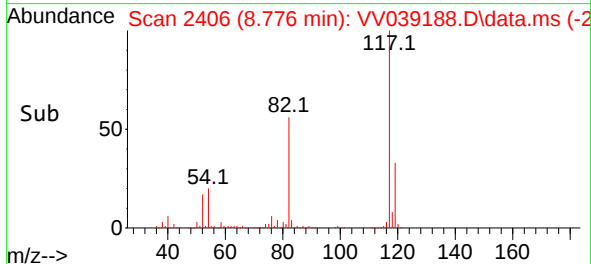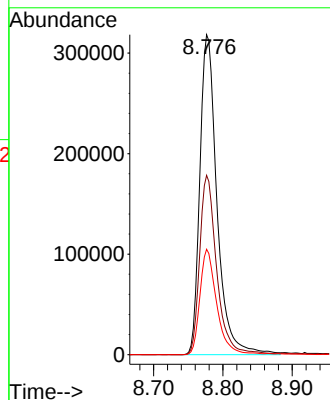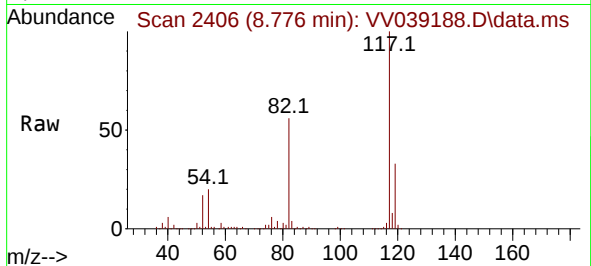

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.175 min Scan# 3152
Delta R.T. 0.003 min
Lab File: VV039188.D
Acq: 25 Sep 2025 17:47

Tgt Ion:152 Resp: 261018
Ion Ratio Lower Upper
152 100
115 61.2 44.8 134.4
150 158.0 0.0 353.8

