

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092525\
Data File : VV039194.D
Acq On : 25 Sep 2025 20:02
Operator : SY/MD
Sample : Q3195-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-23-092325

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M

Title : SW846 8260

Signal : TIC: VV039194.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.918	263	273	288	rBV	99924	181098	6.54%	1.061%
2	2.085	313	325	344	rBV	271267	543694	19.62%	3.187%
3	4.503	1059	1077	1095	rBV	452790	1195004	43.12%	7.004%
4	4.600	1096	1107	1149	rVB	595399	1644737	59.35%	9.640%
5	4.944	1202	1214	1258	rBV	466224	1156971	41.75%	6.781%
6	5.532	1385	1397	1436	rBV	947708	2189425	79.01%	12.832%
7	5.844	1483	1494	1514	rBV3	47614	117713	4.25%	0.690%
8	7.236	1915	1927	1965	rBV	1383046	2666853	96.24%	15.630%
9	8.776	2395	2406	2446	rBV	1624795	2771158	100.00%	16.242%
10	10.001	2777	2787	2821	rBV	1161223	1917977	69.21%	11.241%
11	11.172	3140	3151	3183	rBV	1628752	2677265	96.61%	15.691%




Sum of corrected areas: 17061895

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092525\
Data File : VV039194.D
Acq On : 25 Sep 2025 20:02
Operator : SY/MD
Sample : Q3195-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-23-092325

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

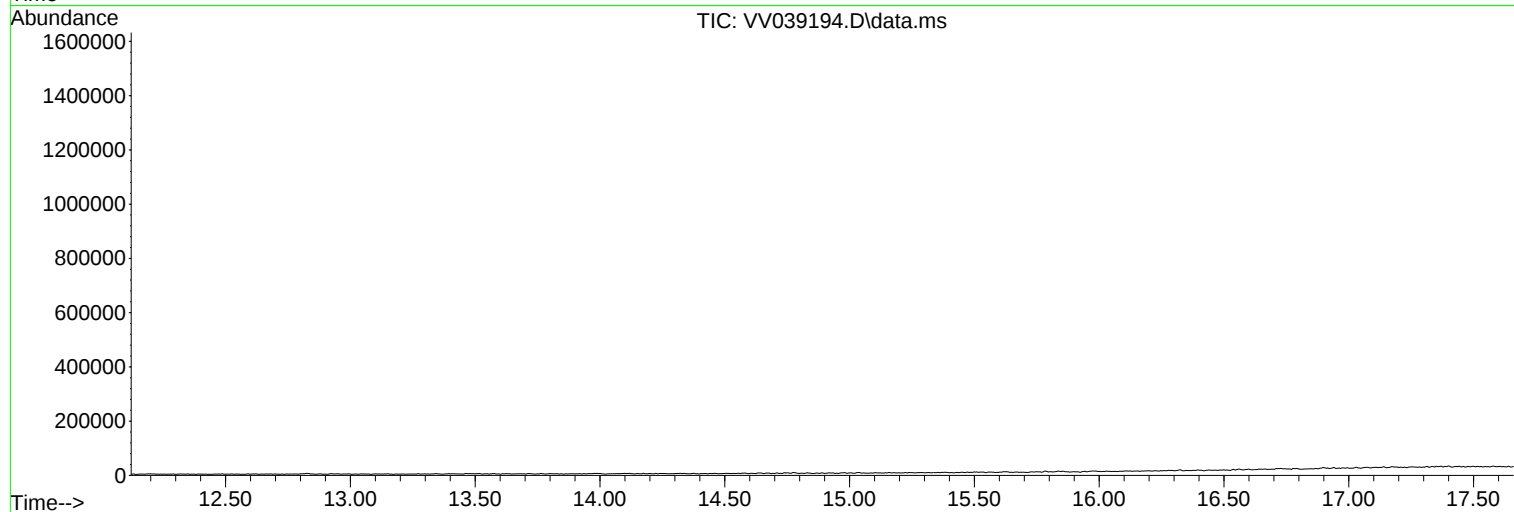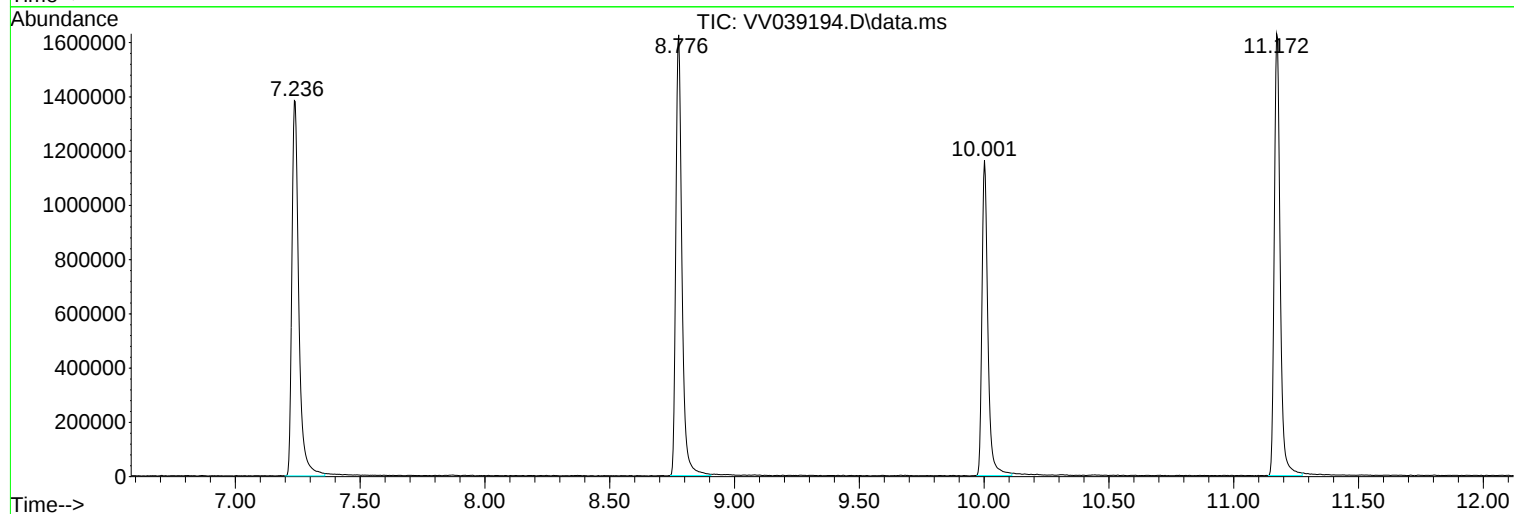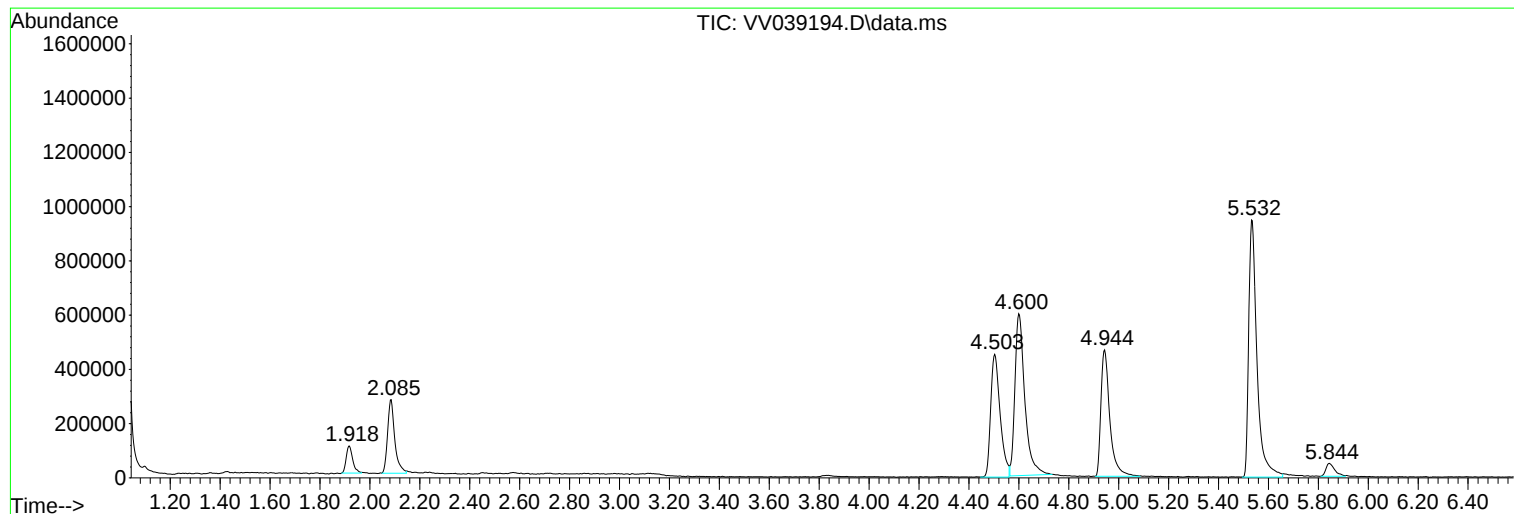

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092525\
Data File : VV039194.D
Acq On : 25 Sep 2025 20:02
Operator : SY/MD
Sample : Q3195-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-23-092325









Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethane, 1,2-dichloro-1,1,2-... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.918	5.51 ug/l	181098	Pentafluorobenzene	4.603

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethane, 1,2-dichloro-1,1,2-trifl...	152	C2HCl2F3	000354-23-4	90
2			Fluorodichloromethane	102	CHCl2F	000075-43-4	32
3			Cyclopropane, 1,2-dimethyl-3-met...	82	C6H10	062338-02-7	25
4			1-Bromo-2-chloro-1,1,2-trifluoro...	196	C2HBrClF3	000354-06-3	25
5			1,4-Pentadiene, 3-methyl-	82	C6H10	001115-08-8	9

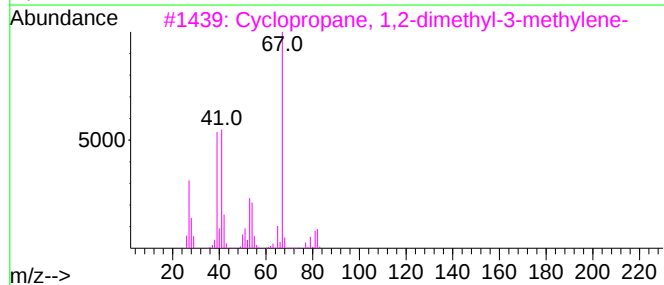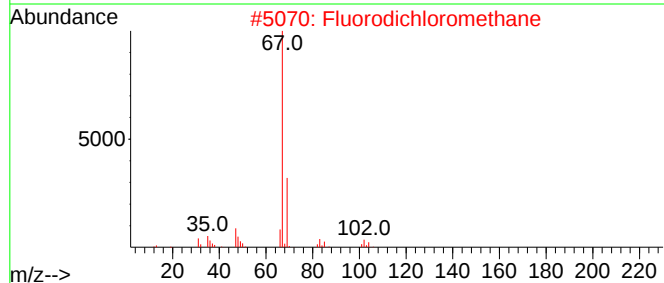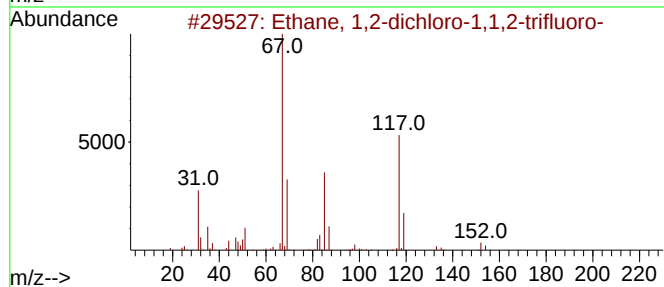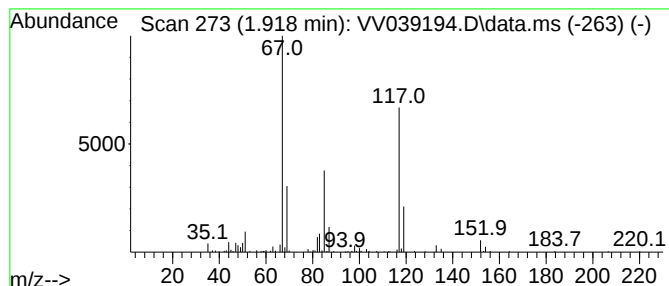

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092525\
Data File : VV039194.D
Acq On : 25 Sep 2025 20:02
Operator : SY/MD
Sample : Q3195-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-23-092325

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethane, 1,2-dic...	1.918	5.5	ug/l	181098	1	4.603	1644740	50.0