

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092618\
 Data File : VV007885.D
 Acq On : 26 Sep 2018 15:47
 Operator : SY/MD
 Sample : J5036-03
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C08W7

Quant Time: Sep 27 12:41:09 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092518WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 27 04:55:01 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	179592	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	171445	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	88371	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	47004	41.75	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	83.50%
7) Chloroethane-d5	1.59	69	43640	44.89	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	89.78%
11) 1,1-Dichloroethene-d2	2.14	63	78534	32.74	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.48%
21) 2-Butanone-d5	3.96	46	27805	36.65	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	36.65%#
24) Chloroform-d	4.41	84	106731	45.64	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.28%
26) 1,2-Dichloroethane-d4	5.09	65	79750	47.83	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.66%
32) Benzene-d6	5.11	84	215946	47.03	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.06%
36) 1,2-Dichloropropane-d6	6.13	67	69900	48.61	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.22%
41) Toluene-d8	7.36	98	208386	45.03	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.06%
43) trans-1,3-Dichloropropene-	7.67	79	30333	44.31	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.62%
47) 2-Hexanone-d5	8.14	63	49795	82.01	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	82.01%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	99325	46.80	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	92642	47.16	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.32%


Target Compounds					Ovalue
13) Acetone	2.19	43	14753	16.140 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092618\
Data File : VV007885.D
Acq On : 26 Sep 2018 15:47
Operator : SY/MD
Sample : J5036-03
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C08W7

Quant Time: Sep 27 12:41:09 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092518WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 27 04:55:01 2018
Response via : Initial Calibration

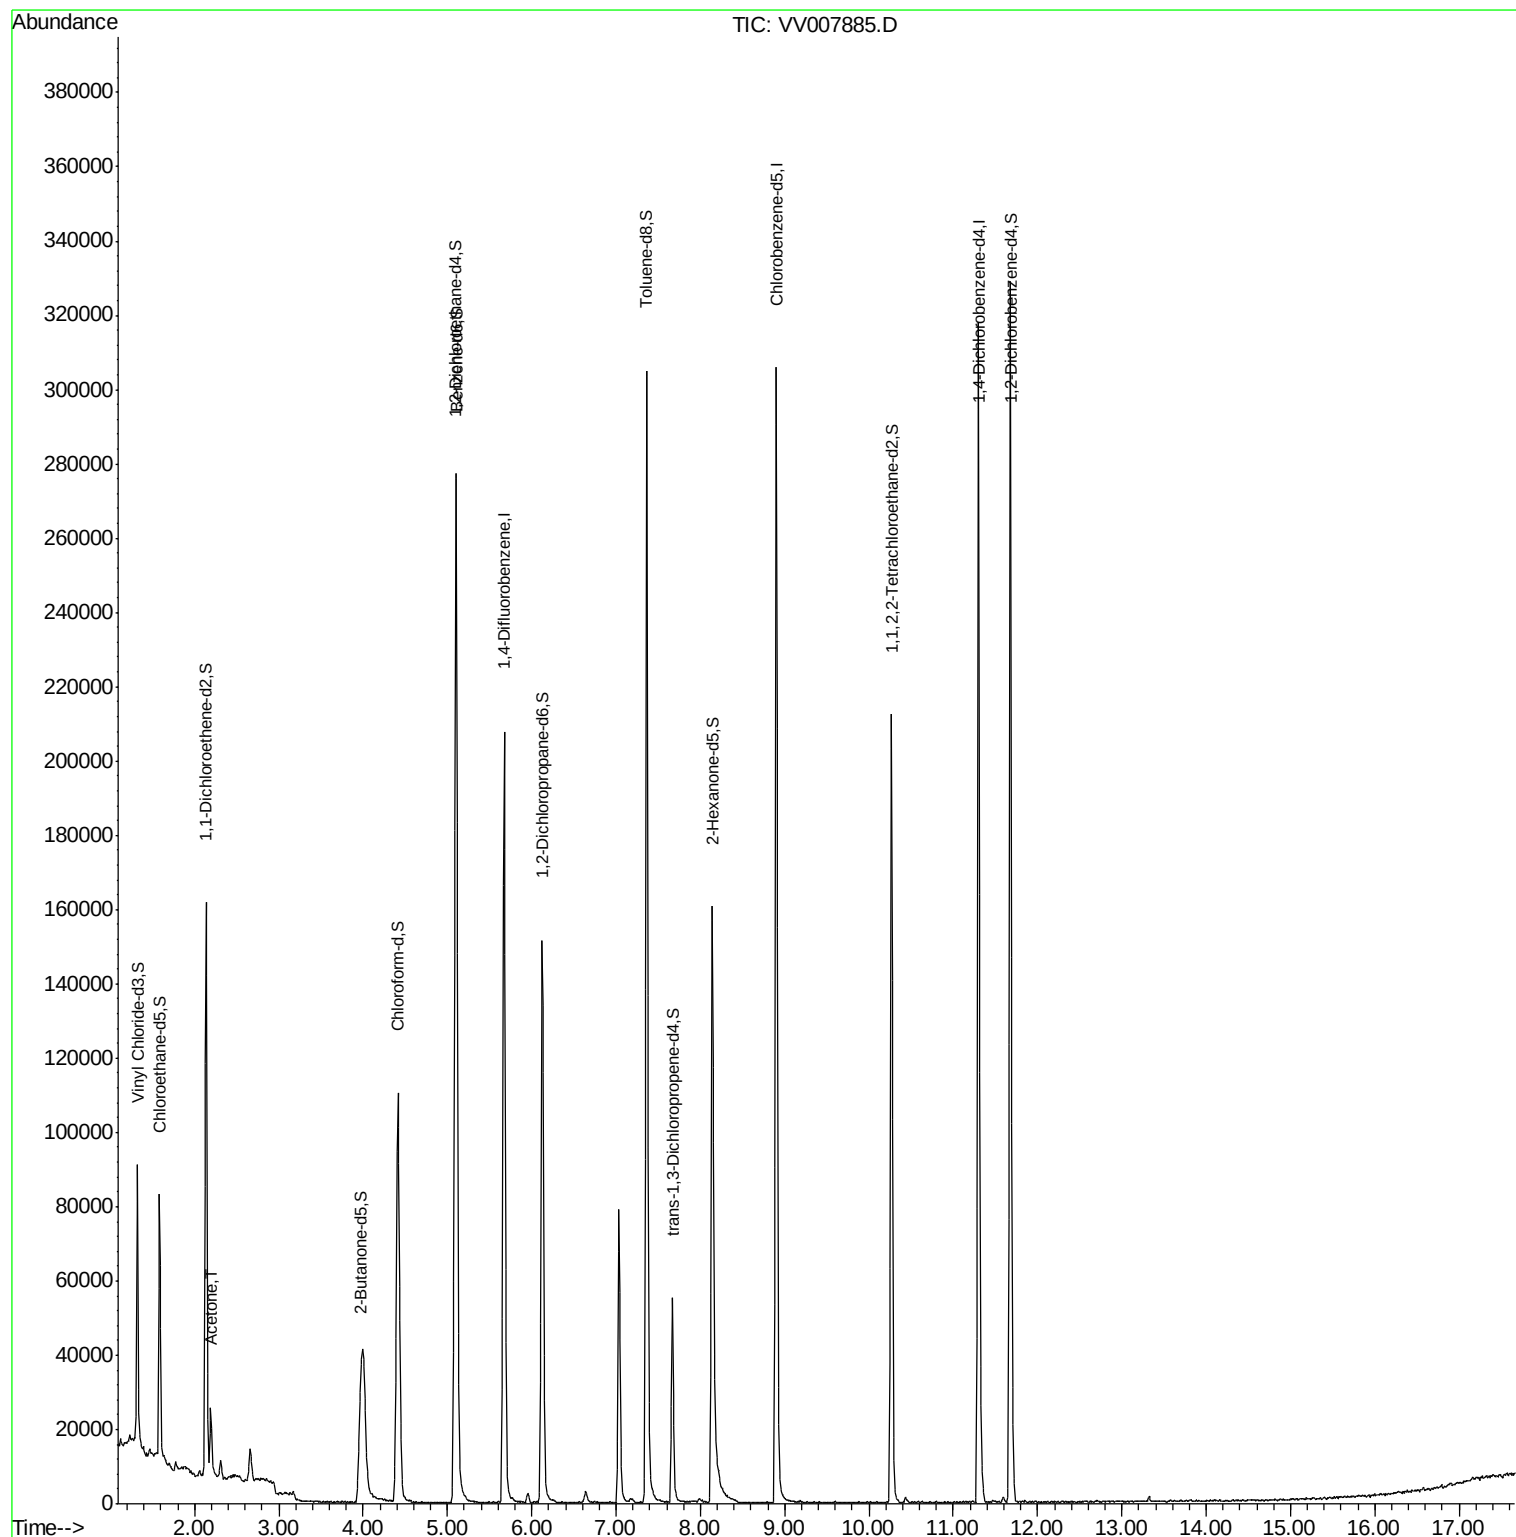

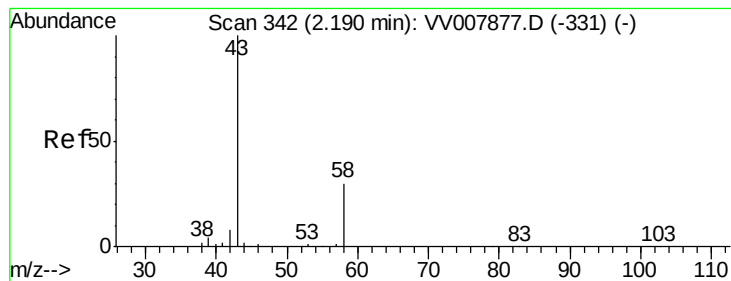

#13
 Acetone
 Concen: 16.140 ug/L
 RT: 2.19 min Scan# 343
 Delta R.T. 0.00 min
 Lab File: VV007885.D
 Acq: 26 Sep 2018 15:47

Instrument :
 MSVOA_V
 ClientSampleId :
 C08W7

Tot Ion: 43 Resp: 14753
 Ion Ratio Lower Upper
 43 100
 58 31.8 0.0 59.4

