

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092618\
 Data File : VV007886.D
 Acq On : 26 Sep 2018 16:12
 Operator : SY/MD
 Sample : J5036-04
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C08W8

Quant Time: Sep 27 12:41:34 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092518WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 27 04:55:01 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	181959	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	175032	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	89640	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	46182	40.49	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	80.98%
7) Chloroethane-d5	1.59	69	43516	44.18	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	88.36%
11) 1,1-Dichloroethene-d2	2.14	63	79957	32.90	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.80%
21) 2-Butanone-d5	3.96	46	28088	36.54	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	36.54%#
24) Chloroform-d	4.41	84	107212	45.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.50%
26) 1,2-Dichloroethane-d4	5.09	65	80140	47.43	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.86%
32) Benzene-d6	5.11	84	216722	46.23	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.46%
36) 1,2-Dichloropropane-d6	6.13	67	70189	47.81	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.62%
41) Toluene-d8	7.36	98	208549	44.14	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.28%
43) trans-1,3-Dichloropropene-	7.67	79	30727	43.97	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.94%
47) 2-Hexanone-d5	8.14	63	53511	86.32	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	86.32%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	100659	46.46	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.92%
64) 1,2-Dichlorobenzene-d4	11.68	152	94726	47.54	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.08%


Target Compounds					Ovalue
13) Acetone	2.19	43	14864	16.050 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092618\
Data File : VV007886.D
Acq On : 26 Sep 2018 16:12
Operator : SY/MD
Sample : J5036-04
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C08W8

Quant Time: Sep 27 12:41:34 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092518WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 27 04:55:01 2018
Response via : Initial Calibration

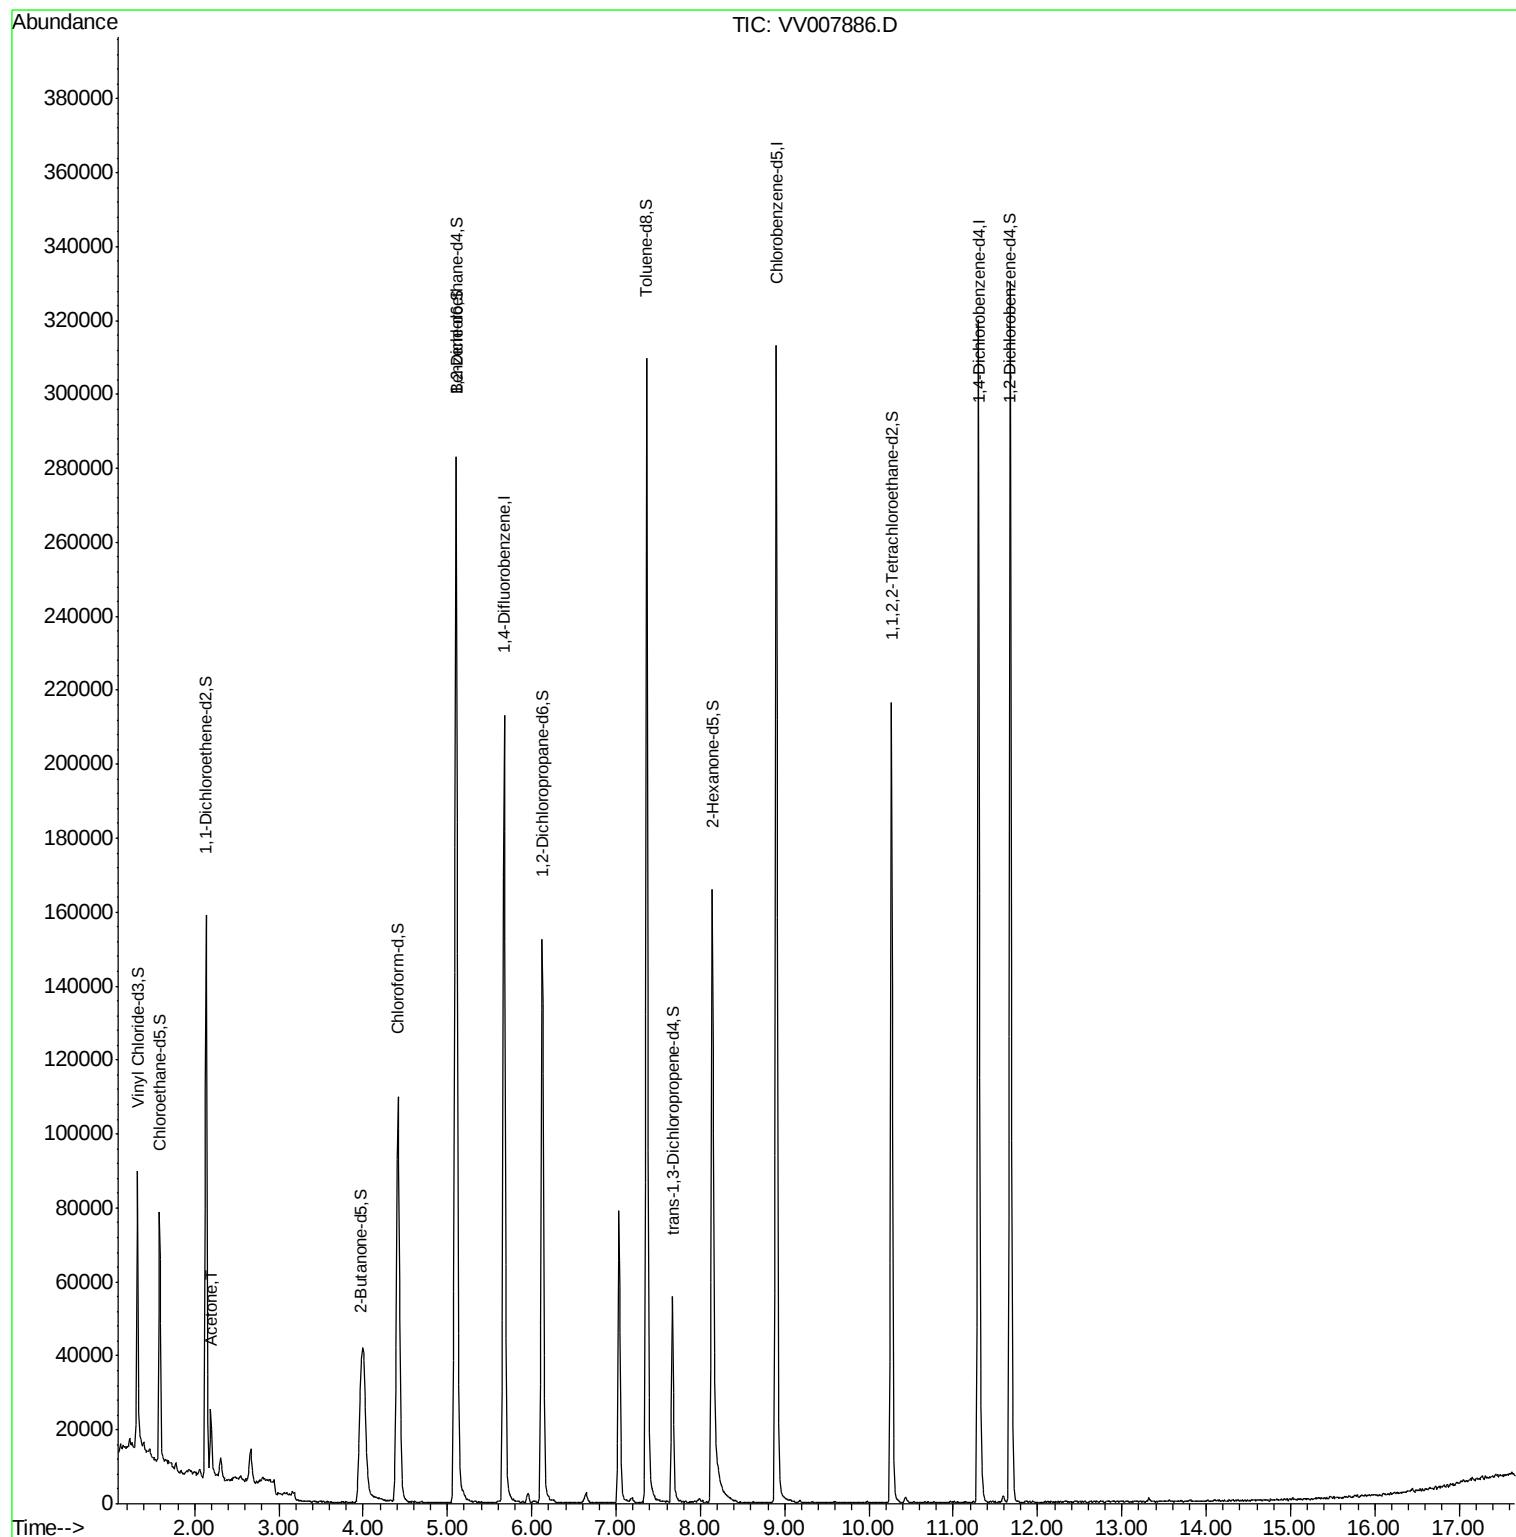

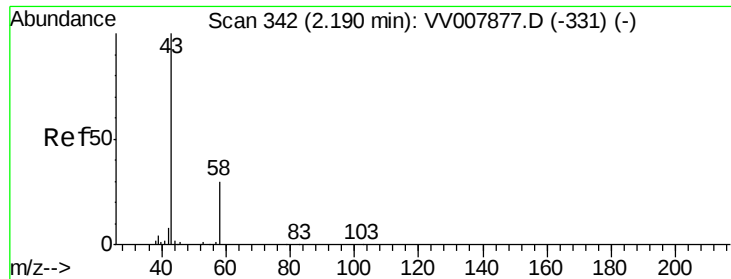

#13

Acetone

Concen: 16.050 ug/L

RT: 2.19 min Scan# 343

Delta R.T. 0.00 min

Lab File: VV007886.D

Acq: 26 Sep 2018 16:12

Instrument :
MSVOA_V
ClientSampleId :
C08W8

Tot Ion: 43 Resp: 14864

Ion Ratio Lower Upper

43 100

58 31.2 0.0 59.4

