


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092618\
Data File : VV007876.D
Acq On : 26 Sep 2018 11:17
Operator : SY/MD
Sample : BFB74
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB74

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092518WMA.M
Title : VOC Analysis
Last Update : Thu Sep 27 04:55:01 2018

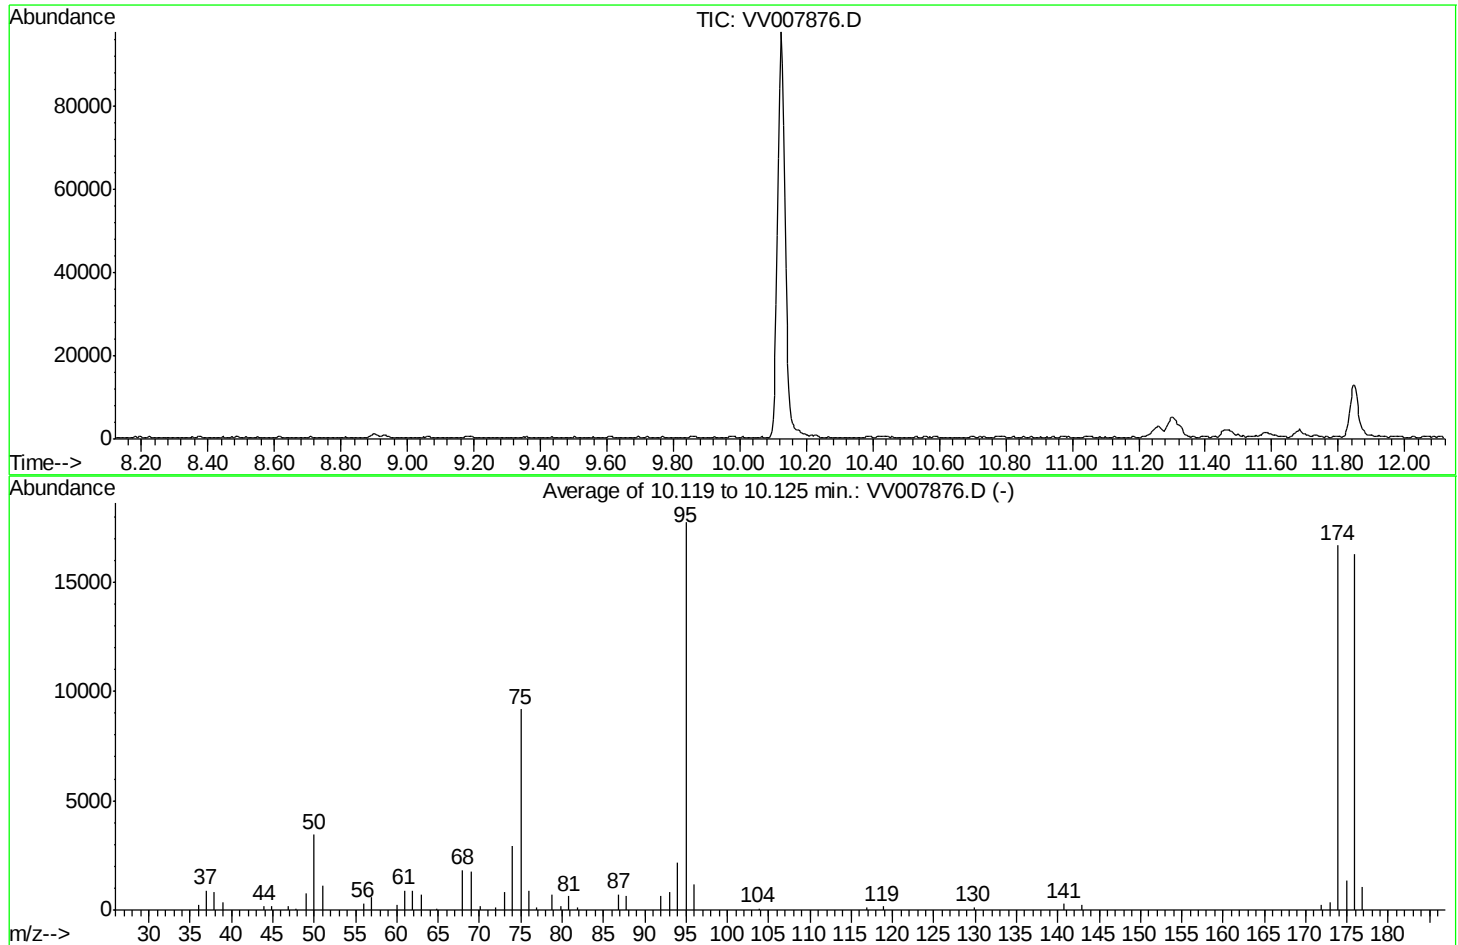

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	3438	PASS
75	95	30	80	51.8	9180	PASS
95	95	100	100	100.0	17730	PASS
96	95	5	9	6.7	1183	PASS
173	174	0.00	2	2.0	327	PASS
174	95	50	120	94.0	16674	PASS
175	174	5	9	8.1	1352	PASS
176	174	95	101	97.6	16278	PASS
177	176	5	9	6.5	1053	PASS

Scan 2798 (10.087 min): VV007876.D
BFB74

m/z	Abundance
39.90	108.0
43.90	242.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
36.00	215.0
36.90	868.0
37.90	807.0
38.90	326.0
39.90	138.0
44.00	486.0
44.90	144.0
46.90	165.0
48.90	724.0
50.00	3139.0
51.00	988.0
56.00	300.0
57.00	564.0
60.00	226.0
60.90	823.0
61.90	812.0
63.00	658.0
68.00	1704.0
69.00	1730.0
70.00	187.0
72.00	102.0
73.00	814.0
74.00	2707.0
75.00	8436.0
76.00	846.0
77.00	110.0
78.80	630.0
79.80	170.0
80.90	567.0
81.90	125.0
86.90	651.0
87.80	683.0
92.00	614.0
92.90	695.0
94.00	1976.0
95.00	16359.0
96.00	1069.0
116.90	130.0
118.80	161.0
129.80	162.0
140.80	239.0
142.90	205.0
171.80	224.0
173.00	293.0
173.90	14742.0
174.90	1160.0
175.90	14515.0
176.90	952.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
35.90	207.0
36.90	899.0
38.00	859.0
38.90	395.0
39.90	117.0
44.00	416.0
44.90	157.0
46.90	177.0
47.80	107.0
49.00	840.0
50.00	3549.0
51.00	1159.0
56.00	335.0
57.00	646.0
60.00	250.0
61.00	923.0
61.90	930.0
63.00	712.0
68.00	1897.0
69.00	1809.0
70.00	187.0
72.00	142.0
73.00	841.0
74.00	3018.0
75.00	9495.0
76.00	908.0
77.00	123.0
78.80	748.0
79.80	155.0
80.80	642.0
81.90	149.0
86.90	744.0
87.80	706.0
92.00	644.0
93.00	858.0
94.00	2219.0
95.00	18416.0
96.00	1218.0
103.80	104.0
116.90	138.0
118.80	164.0
129.80	162.0
140.80	286.0
142.80	253.0
171.80	260.0
173.00	343.0
173.90	17232.0
174.90	1393.0
175.90	16760.0
176.90	1075.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
35.90	201.0
36.90	898.0
38.00	868.0
38.90	414.0
44.00	360.0
44.90	151.0
46.90	182.0
47.90	125.0
48.90	809.0
50.00	3626.0
51.00	1160.0
55.90	309.0
57.00	628.0
60.00	250.0
61.00	960.0
61.90	950.0
63.00	727.0
64.80	104.0
68.00	1926.0
69.00	1746.0
70.10	184.0
71.90	177.0
73.00	844.0
74.00	3071.0
75.00	9610.0
76.00	862.0
76.90	129.0
78.80	765.0
79.80	147.0
80.80	664.0
81.80	137.0
86.90	768.0
87.80	634.0
92.00	625.0
93.00	957.0
94.00	2298.0
95.00	18416.0
96.00	1264.0
103.80	113.0
116.90	125.0
118.90	154.0
129.90	118.0
140.80	276.0
142.80	271.0
171.80	257.0
173.00	347.0
173.90	18048.0
174.90	1504.0
175.90	17560.0
176.90	1134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74