

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092619\
 Data File : VV012996.D
 Acq On : 26 Sep 2019 13:36
 Operator : SY/MD
 Sample : K4988-02RE
 Misc : 5.25G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ESNY5RE

Quant Time: Sep 27 04:00:55 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 27 02:13:48 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	628762	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	569073	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	216143	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	204388	20.95	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.80%
7) Chloroethane-d5	1.58	69	190431	24.14	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.56%
10) 1,1-Dichloroethene-d2	2.13	63	275216	16.96	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.84%
20) 2-Butanone-d5	3.95	46	108536	32.22	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	64.44%
24) Chloroform-d	4.40	84	405687	23.49	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.96%
26) 1,2-Dichloroethane-d4	5.08	65	242941	24.20	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.80%
29) Benzene-d6	5.10	84	799923	25.18	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.72%
33) 1,2-Dichloropropane-d6	6.12	67	270138	27.12	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	108.48%
37) Toluene-d8	7.36	98	663342	23.00	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.00%
38) trans-1,3-Dichloropropene-	7.66	79	85724	20.33	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.32%
39) 2-Hexanone-d5	8.14	63	75465	37.66	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	75.32%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	207972	21.99	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.96%
61) 1,2-Dichlorobenzene-d4	11.67	152	210865	25.11	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.44%


Target Compounds					Ovalue
13) Acetone	2.21	43	5569	1.555 ug/L	56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092619\
Data File : VV012996.D
Acq On : 26 Sep 2019 13:36
Operator : SY/MD
Sample : K4988-02RE
Misc : 5.25G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESNY5RE

Quant Time: Sep 27 04:00:55 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 27 02:13:48 2019
Response via : Initial Calibration

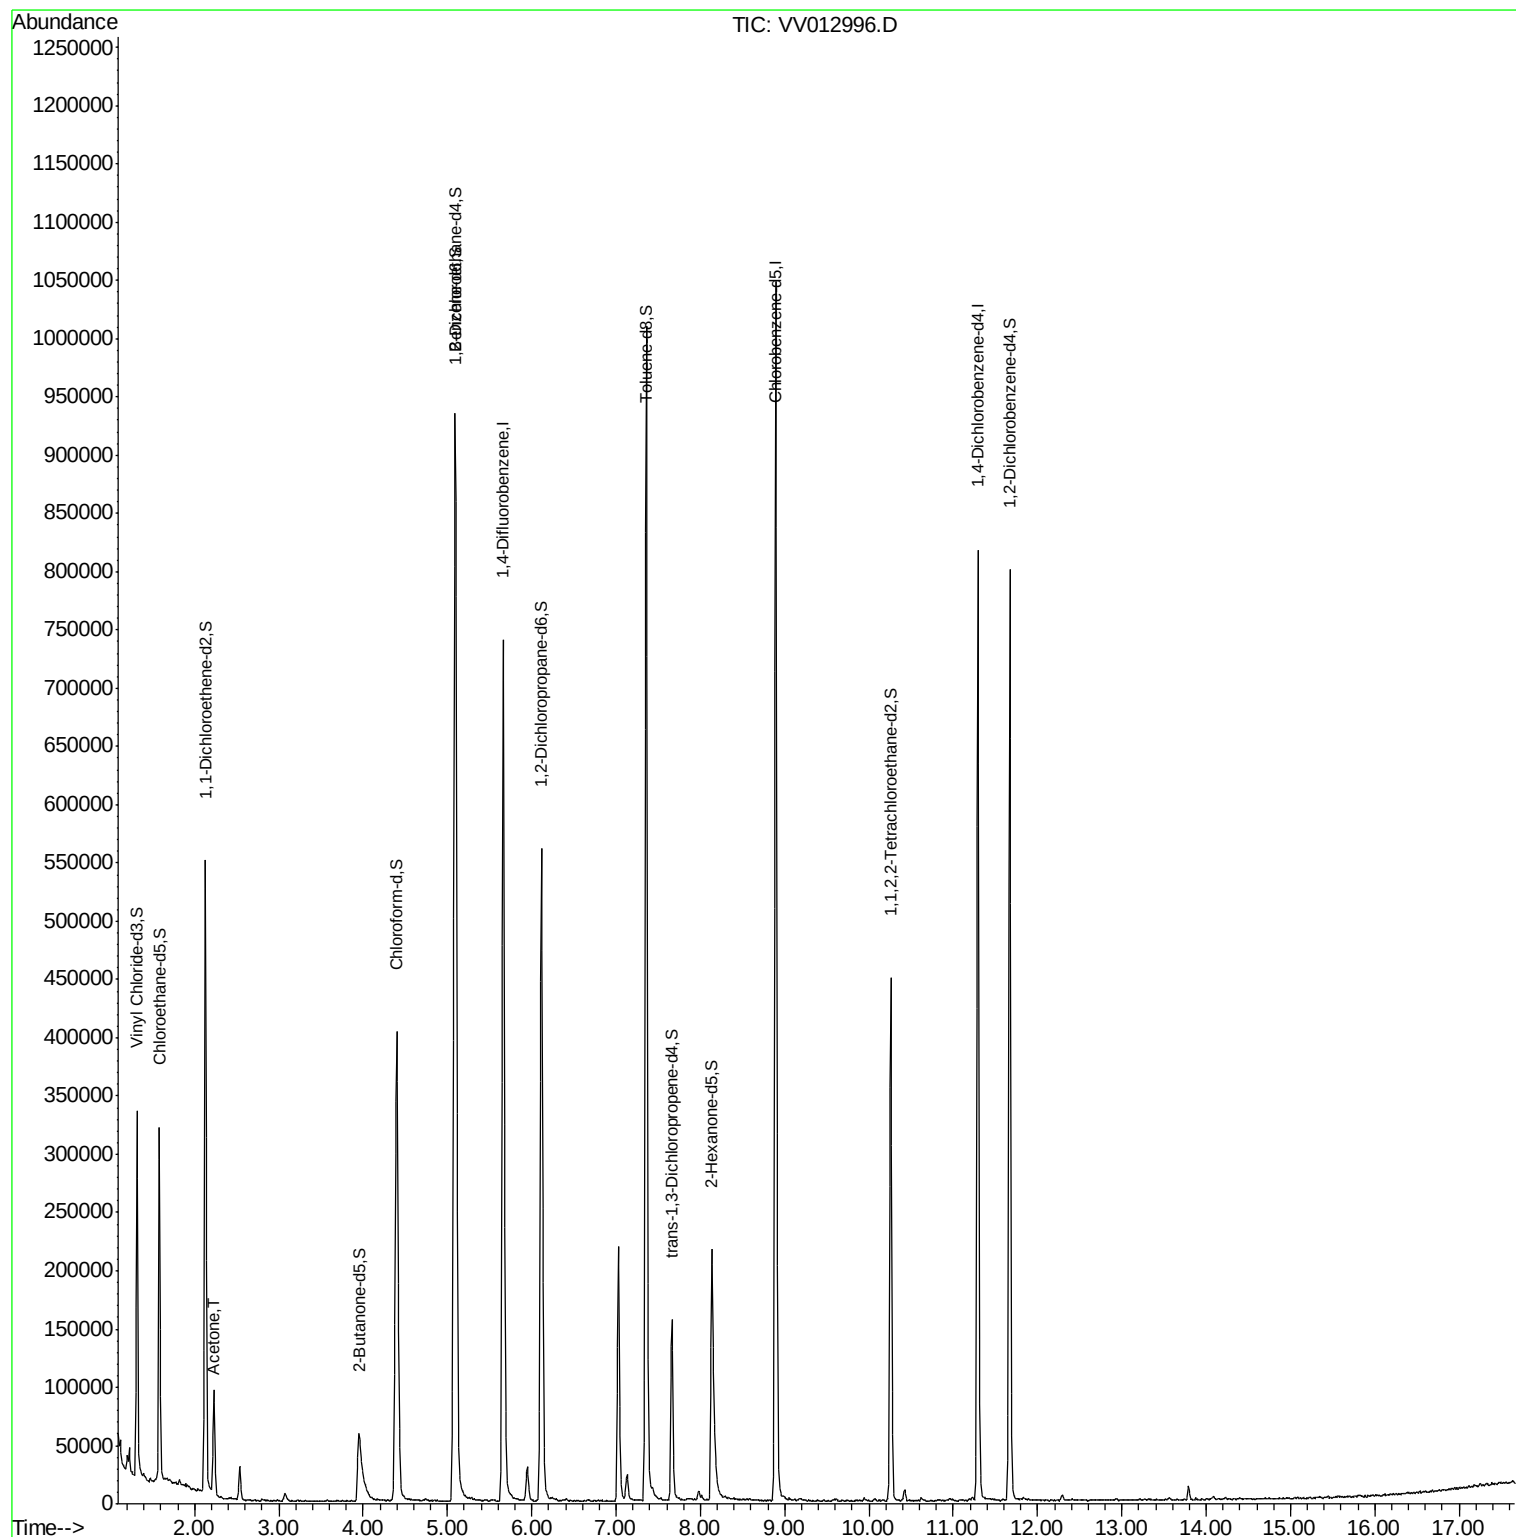

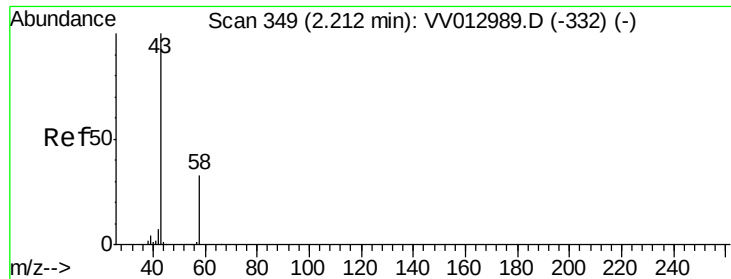

#13
Acetone
Concen: 1.555 ug/L
RT: 2.21 min Scan# 348
Delta R.T. -0.00 min
Lab File: VV012996.D
Acq: 26 Sep 2019 13:36

Instrument :
MSVOA_V
ClientSampleId :
ESNY5RE

Tot Ion: 43 Resp: 5569
Ion Ratio Lower Upper
43 100
58 7.6 0.0 65.0

