

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092623\
 Data File : VV032176.D
 Acq On : 26 Sep 2023 10:07
 Operator : SY/MD
 Sample : VV0926WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK201

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M

Title : VOC Analysis

Signal : TIC: VV032176.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rBV	107022	113508	13.62%	1.713%
2	1.532	146	153	167	rVB	93024	111118	13.34%	1.677%
3	2.060	308	317	334	rBV	174089	256004	30.72%	3.863%
4	2.307	392	394	399	rBV2	417	238	0.03%	0.004%
5	2.449	432	438	447	rVB6	1587	2815	0.34%	0.042%
6	2.539	464	466	468	rBV	290	130	0.02%	0.002%
7	2.703	512	517	522	rBV4	763	787	0.09%	0.012%
8	2.748	529	531	534	rBV2	150	108	0.01%	0.002%
9	2.777	538	540	546	rVB3	252	167	0.02%	0.003%
10	2.831	554	557	559	rVB2	353	208	0.02%	0.003%
11	2.915	581	583	589	rVB4	512	341	0.04%	0.005%
12	2.986	603	605	607	rBV	169	66	0.01%	0.001%
13	3.002	607	610	612	rBV2	123	89	0.01%	0.001%
14	3.175	661	664	665	rBV	166	76	0.01%	0.001%
15	3.343	715	716	719	rVB	151	74	0.01%	0.001%
16	3.359	719	721	725	rVB2	165	102	0.01%	0.002%
17	3.384	727	729	732	rVV2	163	76	0.01%	0.001%
18	3.420	739	740	744	rVB	215	70	0.01%	0.001%
19	3.442	744	747	749	rBV	185	107	0.01%	0.002%
20	3.513	767	769	772	rBV	102	62	0.01%	0.001%
21	3.532	772	775	779	rVB2	105	77	0.01%	0.001%
22	3.555	779	782	785	rVB2	109	63	0.01%	0.001%
23	3.568	785	786	790	rBV2	216	102	0.01%	0.002%
24	3.606	794	798	799	rBV	120	86	0.01%	0.001%
25	3.635	805	807	811	rVB	137	77	0.01%	0.001%
26	3.715	828	832	835	rBV2	267	149	0.02%	0.002%
27	3.789	846	855	893	rBV	73815	196481	23.58%	2.965%
28	4.252	983	999	1031	rBV	127792	330270	39.63%	4.983%
29	4.654	1122	1124	1128	rBV2	210	149	0.02%	0.002%
30	4.748	1151	1153	1156	rBV	192	96	0.01%	0.001%
31	4.796	1166	1168	1170	rBV	149	70	0.01%	0.001%
32	4.960	1201	1219	1246	rBV2	315023	833279	100.00%	12.573%
33	5.285	1318	1320	1326	rVB3	349	266	0.03%	0.004%
34	5.336	1333	1336	1339	rBV2	297	224	0.03%	0.003%
35	5.413	1355	1360	1361	rBV2	320	202	0.02%	0.003%
36	5.442	1367	1369	1372	rBV	182	122	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092623\
 Data File : VV032176.D
 Acq On : 26 Sep 2023 10:07
 Operator : SY/MD
 Sample : VV0926WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK201

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

37	5.539	1386	1399	1424	rBV	264423	549864	65.99%	8.297%
38	5.831	1480	1490	1504	rBV3	12385	25954	3.11%	0.392%
39	5.934	1519	1522	1524	rBV3	146	99	0.01%	0.001%
40	5.992	1527	1540	1566	rBV	186050	391838	47.02%	5.912%
41	6.256	1620	1622	1626	rBV	244	163	0.02%	0.002%
42	6.375	1657	1659	1663	rBV2	134	86	0.01%	0.001%
43	6.403	1665	1668	1671	rVV2	167	129	0.02%	0.002%
44	6.436	1675	1678	1681	rBV2	126	101	0.01%	0.002%
45	6.545	1710	1712	1714	rVB2	161	64	0.01%	0.001%
46	6.577	1718	1722	1724	rBV4	536	477	0.06%	0.007%
47	6.651	1741	1745	1746	rBV2	397	234	0.03%	0.004%
48	6.709	1759	1763	1767	rBV2	99	113	0.01%	0.002%
49	6.731	1767	1770	1772	rBV2	280	159	0.02%	0.002%
50	6.776	1780	1784	1787	rBV2	136	108	0.01%	0.002%
51	6.863	1804	1811	1816	rBV2	141	178	0.02%	0.003%
52	6.918	1816	1828	1857	rBV	100455	193691	23.24%	2.923%
53	7.246	1918	1930	1966	rBV	366429	656883	78.83%	9.912%
54	7.516	2011	2014	2016	rBV2	210	112	0.01%	0.002%
55	7.558	2017	2027	2052	rBV	67448	125382	15.05%	1.892%
56	7.767	2090	2092	2094	rBV2	144	85	0.01%	0.001%
57	7.818	2105	2108	2109	rBV	132	72	0.01%	0.001%
58	7.866	2121	2123	2124	rBV	153	63	0.01%	0.001%
59	7.921	2132	2140	2147	rBV3	653	771	0.09%	0.012%
60	8.027	2163	2173	2213	rBV	210866	415164	49.82%	6.264%
61	8.596	2344	2350	2352	rBV2	308	250	0.03%	0.004%
62	8.632	2359	2361	2364	rVB2	352	206	0.02%	0.003%
63	8.696	2379	2381	2383	rBV	194	106	0.01%	0.002%
64	8.718	2386	2388	2390	rVB	174	80	0.01%	0.001%
65	8.786	2398	2409	2437	rBV	405504	680291	81.64%	10.265%
66	9.018	2479	2481	2482	rBV	230	93	0.01%	0.001%
67	9.075	2496	2499	2500	rBV2	316	152	0.02%	0.002%
68	9.201	2534	2538	2543	rVB2	222	195	0.02%	0.003%
69	9.243	2549	2551	2553	rBV	173	78	0.01%	0.001%
70	9.265	2556	2558	2561	rVB2	163	69	0.01%	0.001%
71	9.329	2576	2578	2579	rBV2	151	71	0.01%	0.001%
72	9.378	2589	2593	2597	rBV2	136	153	0.02%	0.002%
73	9.490	2622	2628	2632	rBV5	767	903	0.11%	0.014%
74	9.763	2711	2713	2715	rBV	368	164	0.02%	0.002%
75	9.818	2728	2730	2736	rVB2	284	191	0.02%	0.003%
76	9.956	2771	2773	2774	rBV	171	71	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092623\
 Data File : VV032176.D
 Acq On : 26 Sep 2023 10:07
 Operator : SY/MD
 Sample : VV0926WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK201

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
 Title : VOC Analysis

77	9.969	2775	2777	2778	rVV	186	70	0.01%	0.001%
78	9.995	2782	2785	2789	rVB	169	105	0.01%	0.002%
79	10.156	2820	2835	2864	rBV	260268	416131	49.94%	6.279%
80	10.297	2876	2879	2881	rBV2	287	187	0.02%	0.003%
81	10.461	2926	2930	2932	rBV	141	120	0.01%	0.002%
82	10.490	2933	2939	2941	rBV2	514	611	0.07%	0.009%
83	10.538	2952	2954	2955	rBV2	185	83	0.01%	0.001%
84	10.673	2994	2996	3001	rBV2	210	154	0.02%	0.002%
85	10.860	3049	3054	3062	rVB2	653	948	0.11%	0.014%
86	10.982	3089	3092	3093	rBV	216	112	0.01%	0.002%
87	11.040	3107	3110	3111	rBV2	175	91	0.01%	0.001%
88	11.091	3123	3126	3129	rBV2	176	136	0.02%	0.002%
89	11.127	3133	3137	3145	rBV2	1099	1290	0.15%	0.019%
90	11.188	3145	3156	3178	rBV	438986	681333	81.77%	10.281%
91	11.413	3223	3226	3235	rVB3	348	429	0.05%	0.006%
92	11.461	3235	3241	3246	rBV2	260	324	0.04%	0.005%
93	11.564	3260	3273	3293	rBV	392104	609482	73.14%	9.196%
94	11.751	3329	3331	3336	rBV	269	151	0.02%	0.002%
95	11.812	3348	3350	3351	rBV	215	81	0.01%	0.001%
96	12.590	3586	3592	3599	rBV4	1405	1599	0.19%	0.024%
97	13.043	3731	3733	3736	rBV	311	177	0.02%	0.003%
98	13.207	3778	3784	3789	rBV4	2213	2604	0.31%	0.039%
99	13.448	3851	3859	3872	rBV	9043	14778	1.77%	0.223%
100	13.689	3927	3934	3942	rVB4	2535	3701	0.44%	0.056%




Sum of corrected areas: 6627419

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092623\
Data File : VV032176.D
Acq On : 26 Sep 2023 10:07
Operator : SY/MD
Sample : VV0926WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK201

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

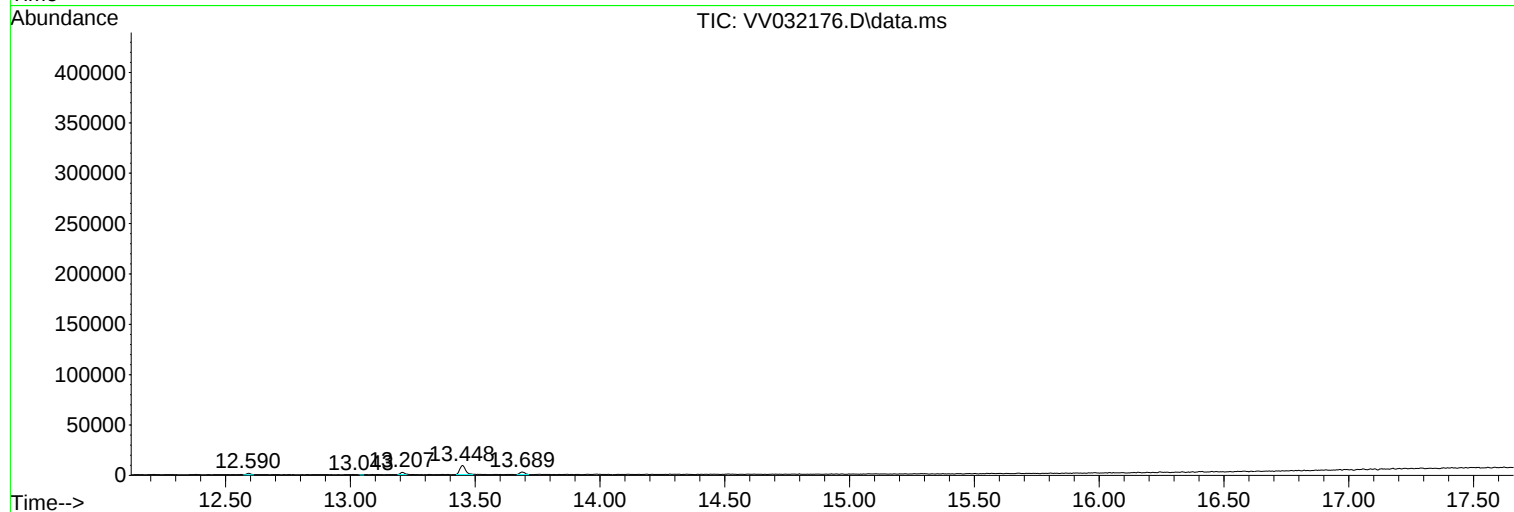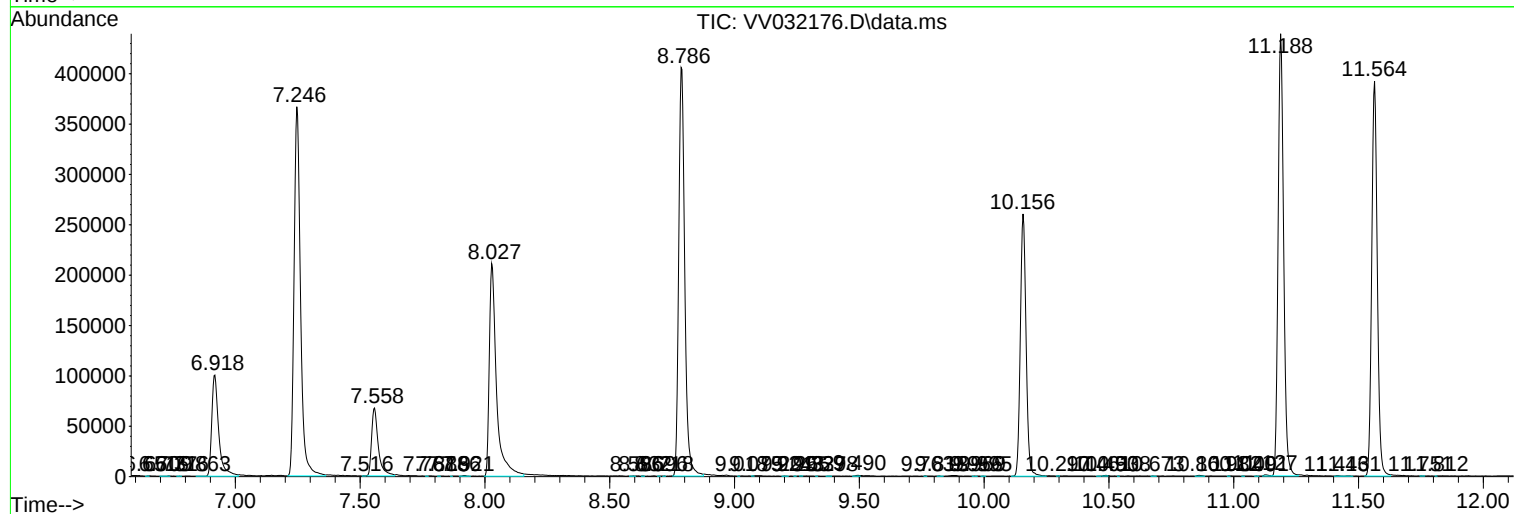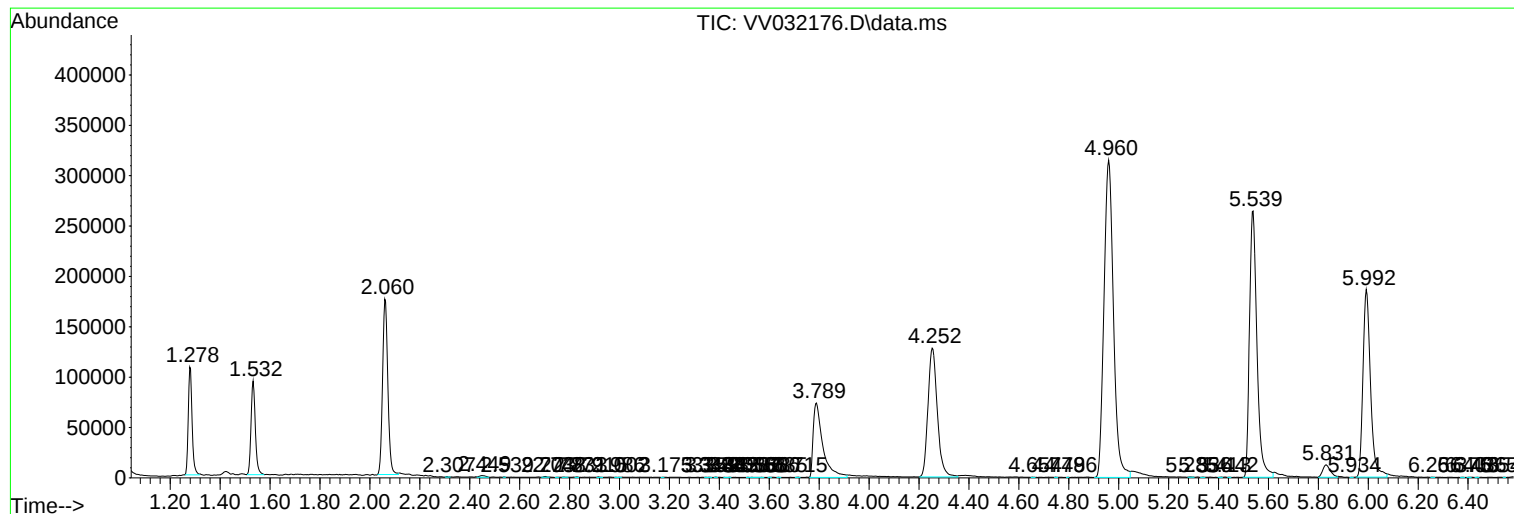

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092623\
Data File : VV032176.D
Acq On : 26 Sep 2023 10:07
Operator : SY/MD
Sample : VV0926WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK201

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092623\
Data File : VV032176.D
Acq On : 26 Sep 2023 10:07
Operator : SY/MD
Sample : VV0926WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK201

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc