


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV092623\  
Data File : VV032173.D  
Acq On : 26 Sep 2023 08:42  
Operator : SY/MD  
Sample : BFB217  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB217

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM092523WMA.M  
Title : VOC Analysis  
Last Update : Tue Sep 26 01:18:56 2023

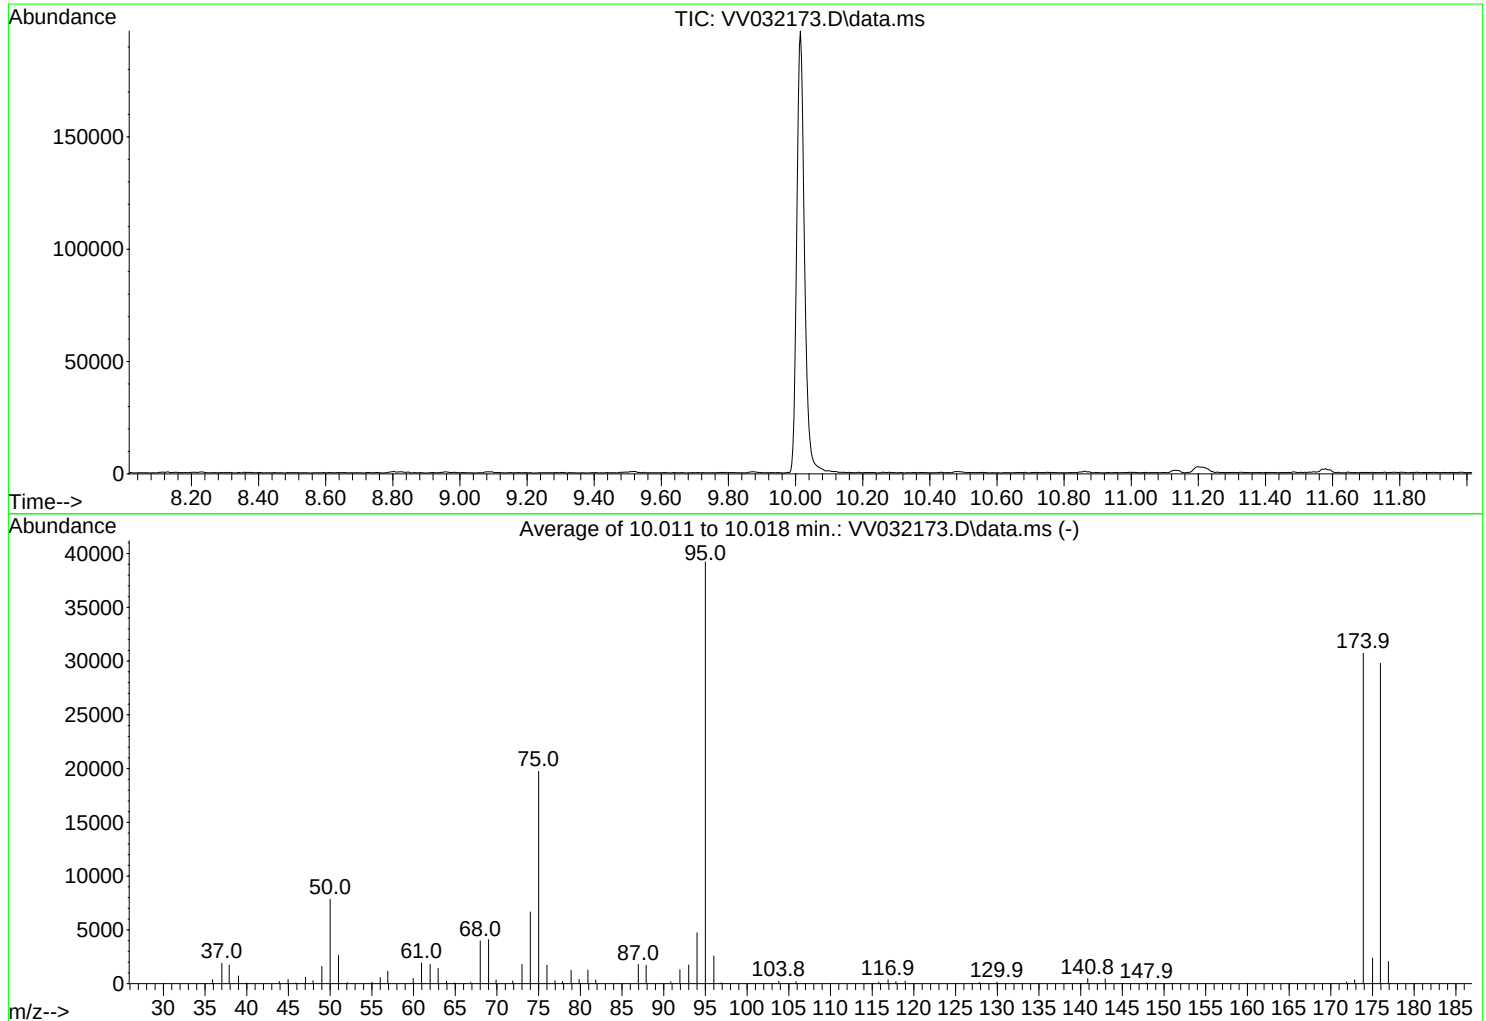

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2780

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 20.0  | 7857  | PASS      |
| 75     | 95      | 30     | 80     | 50.4  | 19757 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 39232 | PASS      |
| 96     | 95      | 5      | 9      | 6.6   | 2577  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.2   | 361   | PASS      |
| 174    | 95      | 50     | 120    | 78.3  | 30728 | PASS      |
| 175    | 174     | 5      | 9      | 7.8   | 2386  | PASS      |
| 176    | 174     | 95     | 105    | 97.0  | 29797 | PASS      |
| 177    | 176     | 5      | 10     | 6.9   | 2054  | PASS      |

| m/z   | Abundance |
|-------|-----------|
| 40.00 | 138.0     |
| 41.00 | 114.0     |
| 43.90 | 421.0     |

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB217

| m/z    | Abundance |
|--------|-----------|
| 35.90  | 373.0     |
| 37.00  | 1926.0    |
| 37.90  | 1738.0    |
| 39.00  | 713.0     |
| 40.00  | 197.0     |
| 43.90  | 659.0     |
| 45.00  | 343.0     |
| 45.90  | 108.0     |
| 47.00  | 646.0     |
| 47.90  | 302.0     |
| 49.00  | 1550.0    |
| 50.00  | 7999.0    |
| 51.00  | 2754.0    |
| 52.10  | 101.0     |
| 55.00  | 138.0     |
| 56.00  | 560.0     |
| 56.90  | 1200.0    |
| 59.90  | 518.0     |
| 61.00  | 1964.0    |
| 62.00  | 1863.0    |
| 62.90  | 1410.0    |
| 63.90  | 214.0     |
| 66.80  | 134.0     |
| 68.00  | 4052.0    |
| 69.00  | 4111.0    |
| 69.90  | 336.0     |
| 71.90  | 235.0     |
| 73.00  | 1833.0    |
| 74.00  | 6841.0    |
| 75.00  | 19712.0   |
| 76.00  | 1774.0    |
| 77.00  | 293.0     |
| 77.90  | 180.0     |
| 78.90  | 1279.0    |
| 79.80  | 396.0     |
| 80.90  | 1292.0    |
| 81.80  | 338.0     |
| 86.90  | 1847.0    |
| 87.90  | 1655.0    |
| 90.80  | 170.0     |
| 91.90  | 1382.0    |
| 93.00  | 1810.0    |
| 94.00  | 4685.0    |
| 95.00  | 39480.0   |
| 96.00  | 2650.0    |
| 103.80 | 239.0     |
| 105.80 | 208.0     |
| 115.80 | 126.0     |
| 116.90 | 375.0     |
| 117.80 | 219.0     |
| 118.90 | 230.0     |
| 127.90 | 129.0     |
| 129.90 | 154.0     |
| 140.90 | 428.0     |
| 143.00 | 401.0     |
| 147.90 | 101.0     |
| 171.90 | 166.0     |
| 172.90 | 381.0     |
| 173.90 | 29912.0   |
| 175.00 | 2479.0    |
| 175.90 | 29128.0   |
| 176.90 | 2006.0    |

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB217

| m/z    | Abundance |
|--------|-----------|
| 35.90  | 385.0     |
| 37.00  | 1935.0    |
| 37.90  | 1814.0    |
| 39.00  | 734.0     |
| 40.00  | 193.0     |
| 43.90  | 641.0     |
| 44.90  | 390.0     |
| 45.90  | 108.0     |
| 47.00  | 631.0     |
| 47.90  | 286.0     |
| 49.00  | 1675.0    |
| 50.00  | 8108.0    |
| 51.00  | 2709.0    |
| 52.00  | 117.0     |
| 55.00  | 133.0     |
| 56.00  | 567.0     |
| 56.90  | 1226.0    |
| 60.00  | 501.0     |
| 60.90  | 2007.0    |
| 62.00  | 1839.0    |
| 63.00  | 1485.0    |
| 64.00  | 220.0     |
| 64.90  | 101.0     |
| 66.80  | 141.0     |
| 68.00  | 4055.0    |
| 69.00  | 4183.0    |
| 69.90  | 358.0     |
| 71.90  | 257.0     |
| 73.00  | 1865.0    |
| 74.00  | 6897.0    |
| 75.00  | 20432.0   |
| 76.00  | 1772.0    |
| 76.90  | 289.0     |
| 77.80  | 206.0     |
| 78.90  | 1258.0    |
| 79.90  | 402.0     |
| 80.90  | 1295.0    |
| 81.90  | 357.0     |
| 86.90  | 1816.0    |
| 87.90  | 1758.0    |
| 90.90  | 176.0     |
| 91.90  | 1348.0    |
| 93.00  | 1776.0    |
| 94.00  | 4948.0    |
| 95.00  | 40464.0   |
| 96.00  | 2641.0    |
| 96.90  | 122.0     |
| 103.80 | 233.0     |
| 105.90 | 199.0     |
| 115.80 | 143.0     |
| 116.90 | 388.0     |
| 117.80 | 200.0     |
| 118.90 | 228.0     |
| 127.90 | 125.0     |
| 129.90 | 149.0     |
| 140.80 | 485.0     |
| 143.00 | 463.0     |
| 147.90 | 103.0     |
| 171.90 | 162.0     |
| 172.90 | 377.0     |
| 173.90 | 31800.0   |
| 175.00 | 2479.0    |
| 175.90 | 30808.0   |
| 176.90 | 2145.0    |

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB217

| m/z    | Abundance |
|--------|-----------|
| 35.90  | 371.0     |
| 37.00  | 1833.0    |
| 37.90  | 1642.0    |
| 39.00  | 679.0     |
| 39.90  | 205.0     |
| 43.90  | 582.0     |
| 45.00  | 438.0     |
| 47.10  | 572.0     |
| 48.00  | 248.0     |
| 49.00  | 1602.0    |
| 50.00  | 7463.0    |
| 51.00  | 2409.0    |
| 52.00  | 120.0     |
| 55.00  | 130.0     |
| 56.00  | 533.0     |
| 56.90  | 1057.0    |
| 60.00  | 440.0     |
| 60.90  | 1829.0    |
| 62.00  | 1706.0    |
| 63.00  | 1381.0    |
| 64.00  | 190.0     |
| 64.90  | 108.0     |
| 66.90  | 135.0     |
| 68.00  | 3810.0    |
| 69.00  | 3979.0    |
| 69.90  | 315.0     |
| 71.90  | 263.0     |
| 73.00  | 1662.0    |
| 74.00  | 6288.0    |
| 75.00  | 19128.0   |
| 76.00  | 1579.0    |
| 76.90  | 269.0     |
| 77.80  | 209.0     |
| 78.90  | 1164.0    |
| 79.90  | 390.0     |
| 80.90  | 1192.0    |
| 81.90  | 347.0     |
| 87.00  | 1677.0    |
| 87.90  | 1708.0    |
| 90.90  | 193.0     |
| 92.00  | 1148.0    |
| 93.00  | 1623.0    |
| 94.00  | 4573.0    |
| 95.00  | 37752.0   |
| 96.00  | 2439.0    |
| 96.90  | 109.0     |
| 103.80 | 211.0     |
| 105.90 | 170.0     |
| 115.80 | 160.0     |
| 116.90 | 324.0     |
| 117.90 | 157.0     |
| 119.00 | 245.0     |
| 127.80 | 125.0     |
| 130.00 | 154.0     |
| 140.90 | 497.0     |
| 142.90 | 469.0     |
| 171.90 | 170.0     |
| 172.80 | 325.0     |
| 173.90 | 30472.0   |
| 175.00 | 2201.0    |
| 176.00 | 29456.0   |
| 176.90 | 2010.0    |

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB217