

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092625\
 Data File : VV039215.D
 Acq On : 26 Sep 2025 16:05
 Operator : SY/MD
 Sample : Q3195-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MW-31D-091825

Quant Time: Sep 29 07:52:22 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 24 08:08:08 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	4.600	168	523421	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	5.535	114	967034	50.000	ug/l	0.00
63) Chlorobenzene-d5	8.776	117	980974	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.175	152	469900	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	4.944	65	446631	58.958	ug/l	0.00
Spiked Amount	50.000	Range	81 - 118	Recovery	= 117.920%	
35) Dibromofluoromethane	4.500	113	425088	54.680	ug/l	0.00
Spiked Amount	50.000	Range	80 - 119	Recovery	= 109.360%	
50) Toluene-d8	7.236	98	1101338	48.235	ug/l	0.00
Spiked Amount	50.000	Range	89 - 112	Recovery	= 96.460%	
62) 4-Bromofluorobenzene	10.001	95	412962	43.934	ug/l	0.00
Spiked Amount	50.000	Range	85 - 114	Recovery	= 87.860%	
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.098	85	167927	20.267	ug/l	100
3) Chloromethane	1.098	50	40046	4.502	ug/l #	43
6) Chloroethane	1.600	64	312	Below Cal	#	44
7) Trichlorofluoromethane	1.915	101	13858	1.005	ug/l	98
8) Diethyl Ether	2.085	74	16067	3.139	ug/l #	1
9) 1,1,2-Trichlorotrifluo...	2.079	101	18545285	2260.702	ug/l	98
12) 1,1-Dichloroethene	2.082	96	135533	17.174	ug/l #	74
13) Acrolein	2.002	56	376	1.353	ug/l #	54
16) Acetone	2.082	43	172991	31.190	ug/l #	85
20) Methylene Chloride	2.461	84	2813	Below Cal	#	88
21) trans-1,2-Dichloroethene	2.706	96	2188	0.260	ug/l	88
24) 1,1-Dichloroethane	3.121	63	146490	8.881	ug/l	99
27) cis-1,2-Dichloroethene	3.841	96	7318	0.790	ug/l	70
31) Cyclohexane	4.596	56	12108	0.896	ug/l #	1
32) 1,1,1-Trichloroethane	4.513	97	121865	8.173	ug/l	97
36) 1,1-Dichloropropene	4.600	75	48605	4.135	ug/l #	49
38) Carbon Tetrachloride	4.600	117	53629	3.733	ug/l #	18
39) Methylcyclohexane	5.828	83	30697	2.163	ug/l #	1
41) Methacrylonitrile	4.162	41	20	1.913	ug/l #	19
44) Trichloroethene	5.828	130	2364403	267.708	ug/l	98
49) 1,4-Dioxane	6.333	88	841	5.912	ug/l #	54
51) 4-Methyl-2-Pentanone	7.236	43	4297	0.336	ug/l #	1
58) 2-Chloroethyl Vinyl ether	6.818	63	114	9.639	ug/l #	47
59) 2-Hexanone	8.130	43	43	2.330	ug/l	89
64) Tetrachloroethene	7.911	164	2084	0.254	ug/l	89
70) Styrene	9.558	104	76	1.564	ug/l #	45
76) 1,2,3-Trichloropropane	10.001	75	209031	19.538	ug/l #	56
81) trans-1,4-Dichloro-2-b...	10.001	75	209031	46.904	ug/l #	13
92) 1,2-Dibromo-3-Chloropr...	12.352	75	75	Below Cal	#	5


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092625\
Data File : VV039215.D
Acq On : 26 Sep 2025 16:05
Operator : SY/MD
Sample : Q3195-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-31D-091825

Quant Time: Sep 29 07:52:22 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 24 08:08:08 2025
Response via : Initial Calibration




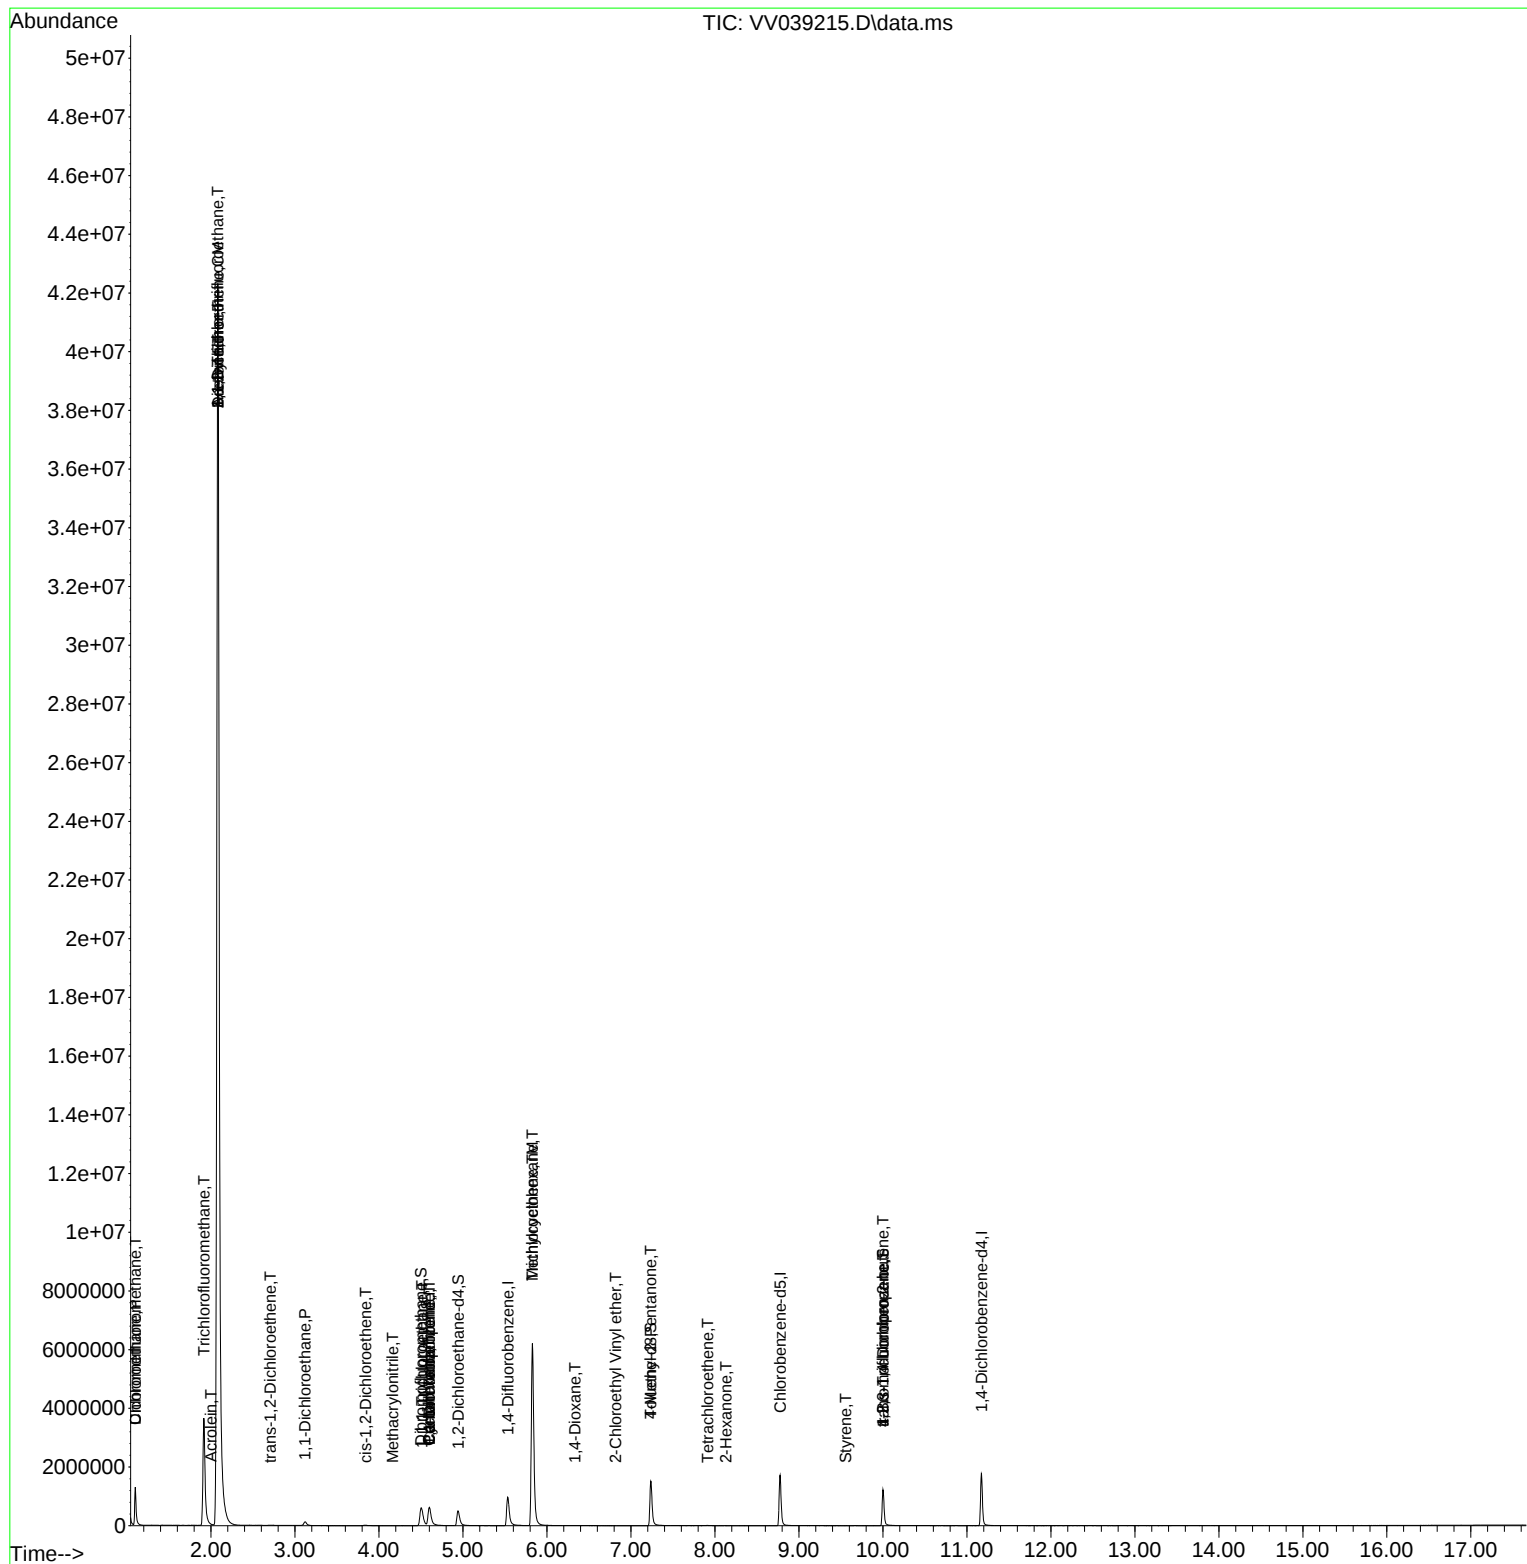


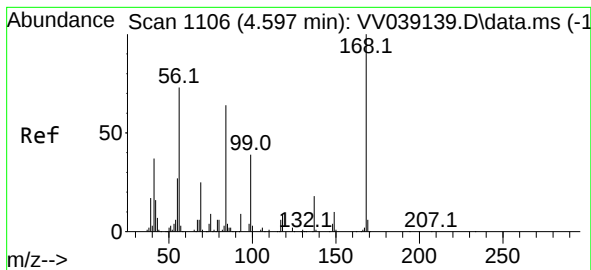

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 4.600 min Scan# 11
Delta R.T. 0.003 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05




Instrument :
MSVOA_V
ClientSampleId :
MW-31D-091825


Tgt Ion:168 Resp: 523421
Ion Ratio Lower Upper
168 100
99 61.2 49.6 74.4

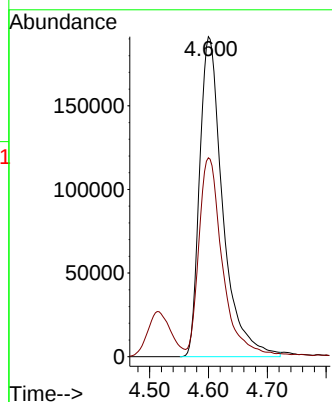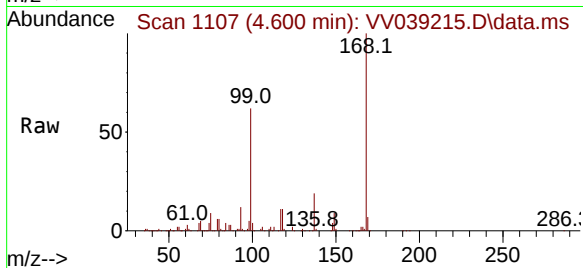

#2
Dichlorodifluoromethane
Concen: 20.267 ug/l
RT: 1.098 min Scan# 18
Delta R.T. -0.023 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05

Tgt Ion: 85 Resp: 167927
Ion Ratio Lower Upper
85 100
87 31.7 16.0 47.9


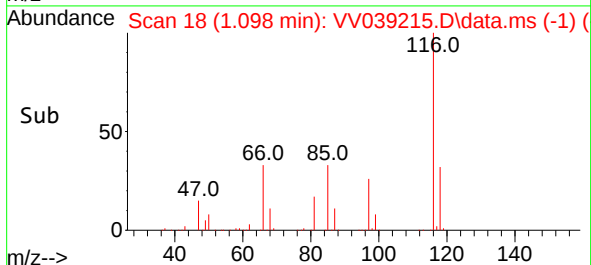

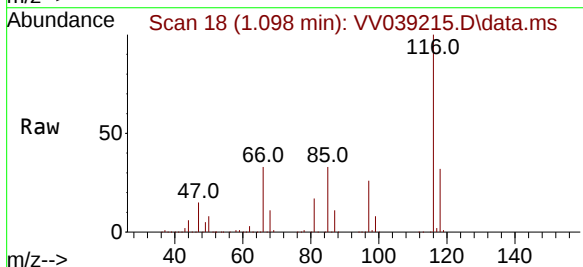


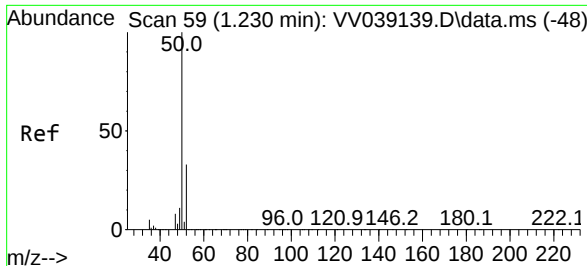

#3
Chloromethane
Concen: 4.502 ug/l
RT: 1.098 min Scan# 11
Delta R.T. -0.132 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05




Instrument :
MSVOA_V
ClientSampleId :
MW-31D-091825


Tgt Ion: 50 Resp: 40046
Ion Ratio Lower Upper
50 100
52 0.7 26.0 39.0#

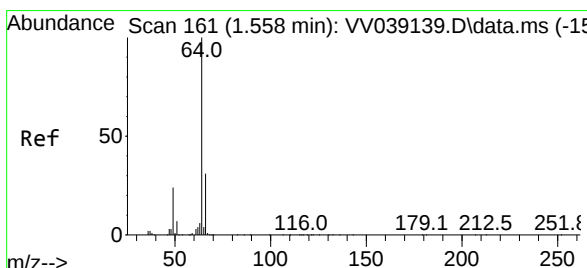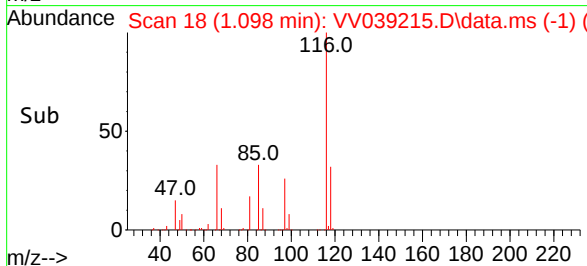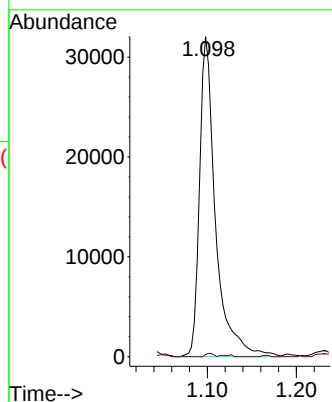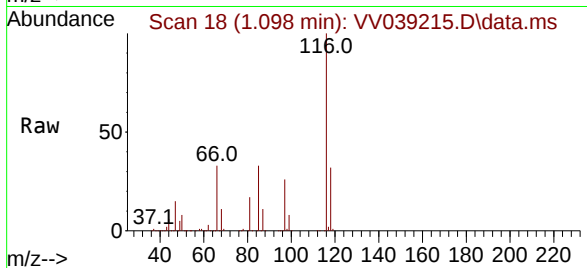

#6
Chloroethane
Concen: Below Cal
RT: 1.600 min Scan# 174
Delta R.T. 0.042 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05

Tgt Ion: 64 Resp: 312
Ion Ratio Lower Upper
64 100
66 0.0 24.6 36.8#


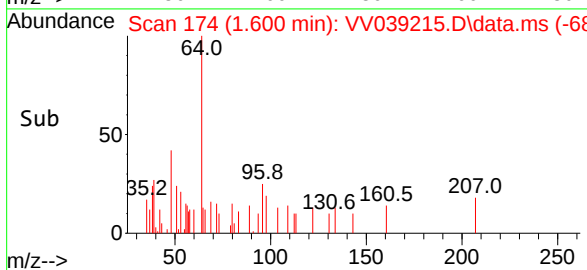
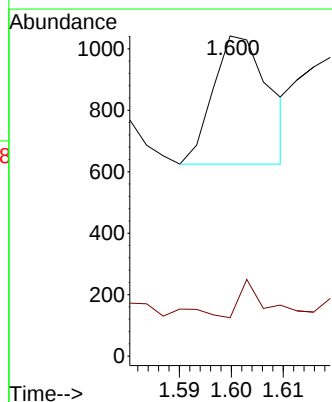
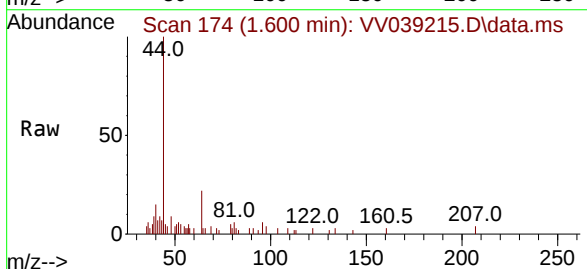


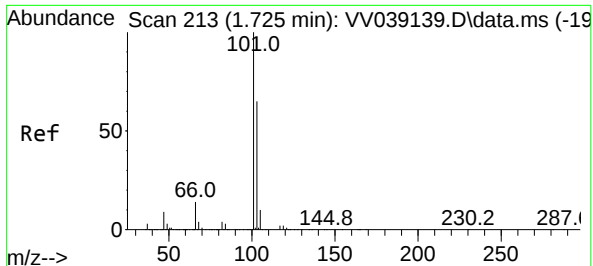

#7
 Trichlorofluoromethane
 Concen: 1.005 ug/l
 RT: 1.915 min Scan# 213
 Delta R.T. 0.190 min
 Lab File: VV039215.D
 Acq: 26 Sep 2025 16:05




Instrument :
 MSVOA_V
 ClientSampleId :
 MW-31D-091825


Tgt Ion:101 Resp: 13858
 Ion Ratio Lower Upper
 101 100
 103 63.2 52.0 78.0

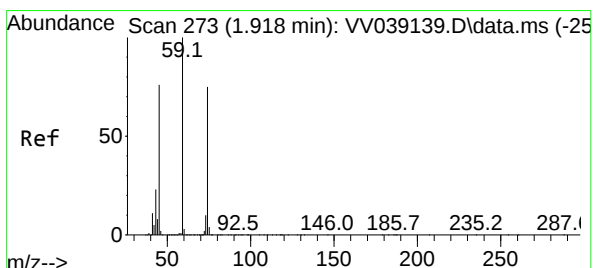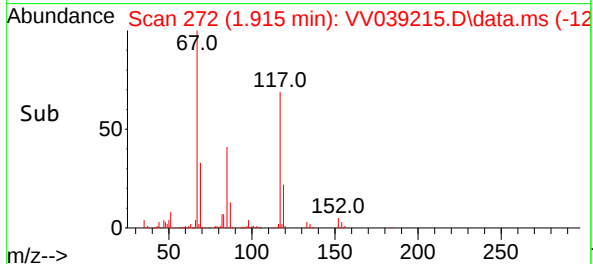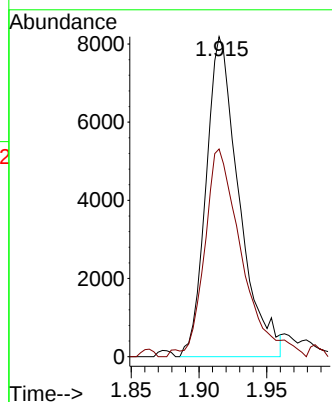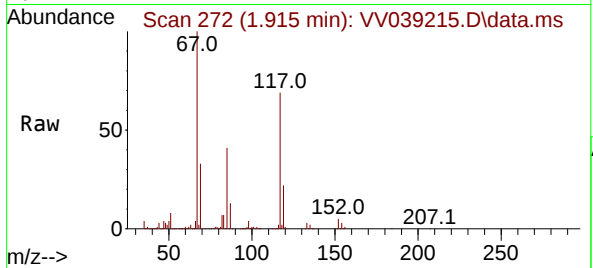

#8
 Diethyl Ether
 Concen: 3.139 ug/l
 RT: 2.085 min Scan# 325
 Delta R.T. 0.167 min
 Lab File: VV039215.D
 Acq: 26 Sep 2025 16:05

Tgt Ion: 74 Resp: 16067
 Ion Ratio Lower Upper
 74 100
 45 0.8 49.6 148.8#


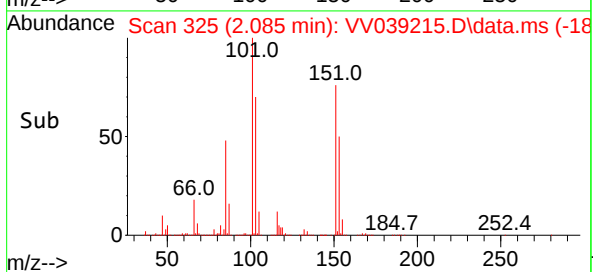
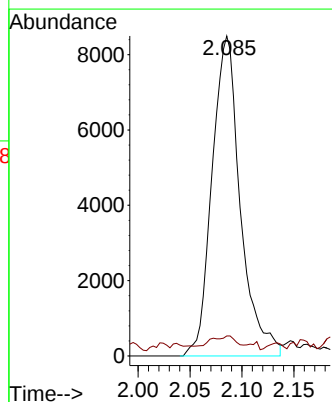
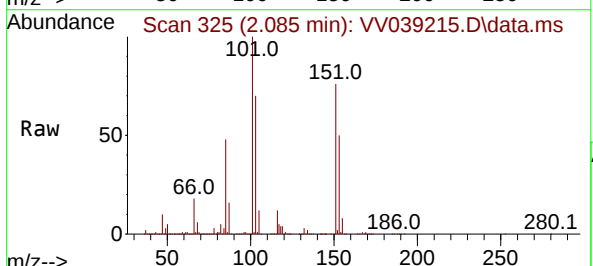




#9
 1,1,2-Trichlorotrifluoroethane
 Concen: 2260.702 ug/l
 RT: 2.079 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: VV039215.D
 Acq: 26 Sep 2025 16:05




Instrument :
 MSVOA_V
 ClientSampleId :
 MW-31D-091825


Tgt Ion:101 Resp:18545285
 Ion Ratio Lower Upper
 101 100
 85 45.9 36.2 54.2
 151 73.1 56.3 84.5

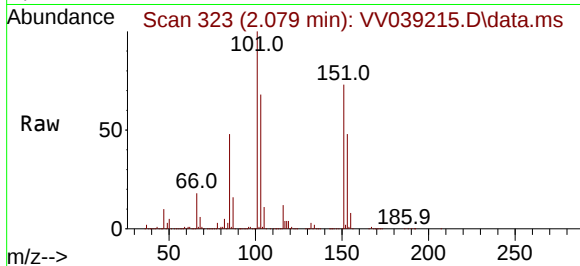

#12
 1,1-Dichloroethene
 Concen: 17.174 ug/l
 RT: 2.082 min Scan# 324
 Delta R.T. -0.000 min
 Lab File: VV039215.D
 Acq: 26 Sep 2025 16:05

Tgt Ion: 96 Resp: 135533
 Ion Ratio Lower Upper
 96 100
 61 130.1 136.0 204.0#
 98 50.7 51.0 76.6#

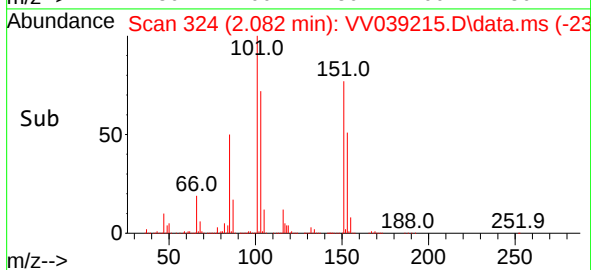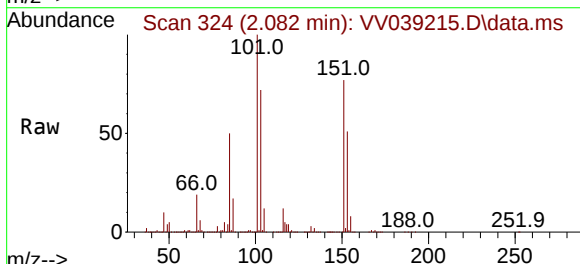



#13

Acrolein

Concen: 1.353 ug/l

RT: 2.002 min Scan# 299

Delta R.T. -0.007 min

Lab File: VV039215.D

Acq: 26 Sep 2025 16:05

Instrument :

MSVOA_V

ClientSampleId :





MW-31D-091825

Tgt Ion: 56 Resp: 376

Ion Ratio Lower Upper

56 100

55 32.7 56.2 84.4#

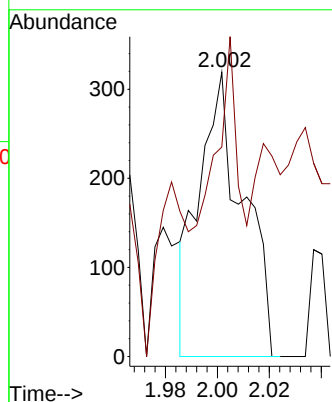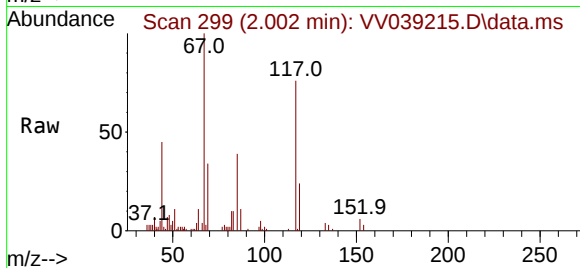

#16

Acetone

Concen: 31.190 ug/l

RT: 2.082 min Scan# 324

Delta R.T. -0.036 min

Lab File: VV039215.D




Acq: 26 Sep 2025 16:05


Tgt Ion: 43 Resp: 172991

Ion Ratio Lower Upper

43 100

58 23.8 25.8 38.6#


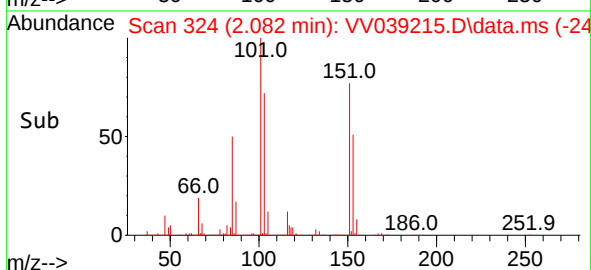

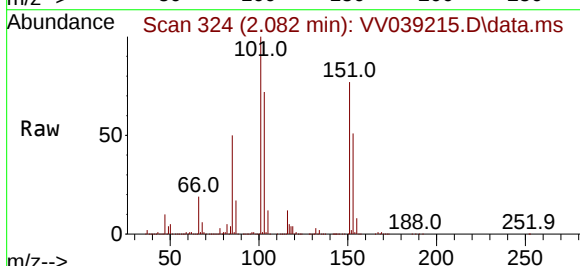




#20
Methylene Chloride
Concen: Below Cal
RT: 2.461 min Scan# 440
Delta R.T. 0.006 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05




Instrument :
MSVOA_V
ClientSampleId :
MW-31D-091825


Tgt Ion:	84	Resp:	2813
Ion	Ratio	Lower	Upper
84	100		
49	120.7	102.8	154.2
51	23.2	31.9	47.9#
86	74.4	51.2	76.8

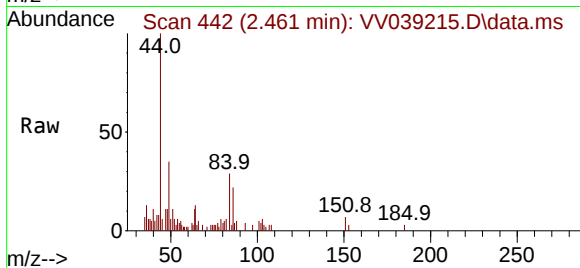

#21
trans-1,2-Dichloroethene
Concen: 0.260 ug/l
RT: 2.706 min Scan# 518
Delta R.T. 0.006 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05

Tgt Ion:	96	Resp:	2188
Ion	Ratio	Lower	Upper
96	100		
61	124.6	112.8	169.2
98	69.7	51.1	76.7


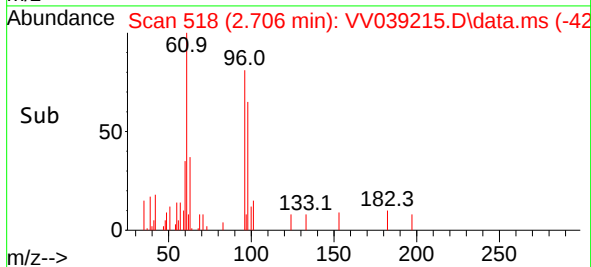

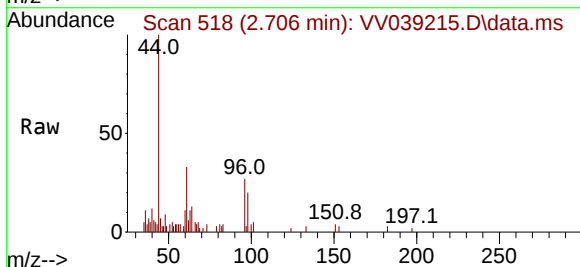




#24
 1,1-Dichloroethane
 Concen: 8.881 ug/l
 RT: 3.121 min Scan# 645
 Delta R.T. 0.006 min
 Lab File: VV039215.D
 Acq: 26 Sep 2025 16:05




Instrument :
 MSVOA_V
 ClientSampleId :
 MW-31D-091825


Tgt Ion: 63 Resp: 146490
 Ion Ratio Lower Upper
 63 100
 98 7.2 3.4 10.2
 100 4.5 2.2 6.6

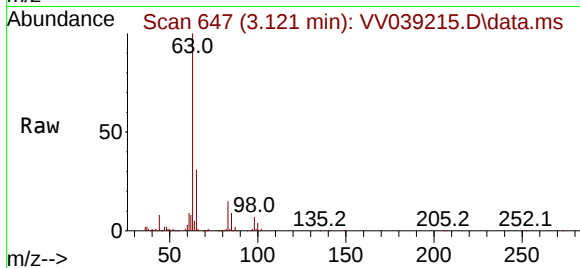

#27
 cis-1,2-Dichloroethene
 Concen: 0.790 ug/l
 RT: 3.841 min Scan# 871
 Delta R.T. 0.022 min
 Lab File: VV039215.D
 Acq: 26 Sep 2025 16:05

Tgt Ion: 96 Resp: 7318
 Ion Ratio Lower Upper
 96 100
 61 112.0 0.0 286.4
 98 32.4 0.0 126.6

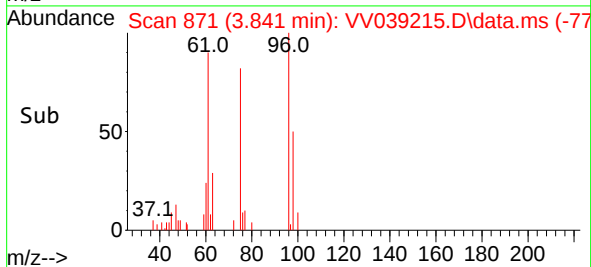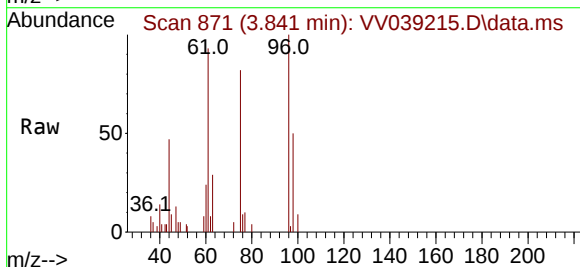



#31

Cyclohexane

Concen: 0.896 ug/l

RT: 4.596 min Scan# 1101

Delta R.T. 0.016 min

Lab File: VV039215.D

Acq: 26 Sep 2025 16:05

Instrument :

MSVOA_V

ClientSampleId :

MW-31D-091825





Tgt Ion: 56 Resp: 12108

Ion Ratio Lower Upper

56 100

69 197.2 26.2 39.2#

84 145.6 70.3 105.5#

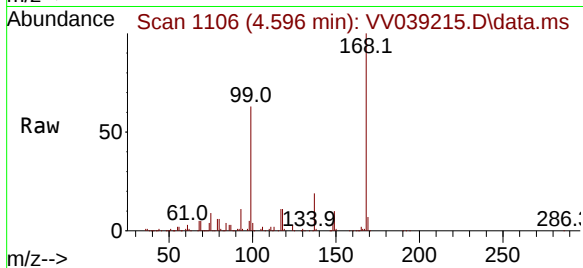

#32

1,1,1-Trichloroethane

Concen: 8.173 ug/l

RT: 4.513 min Scan# 1080

Delta R.T. 0.003 min

Lab File: VV039215.D

Acq: 26 Sep 2025 16:05




Tgt Ion: 97 Resp: 121865


Ion Ratio Lower Upper

97 100

99 61.4 49.6 74.4

61 39.8 34.5 51.7


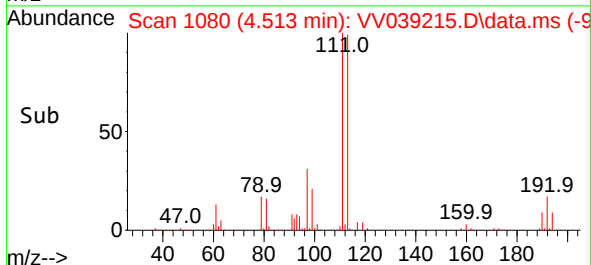
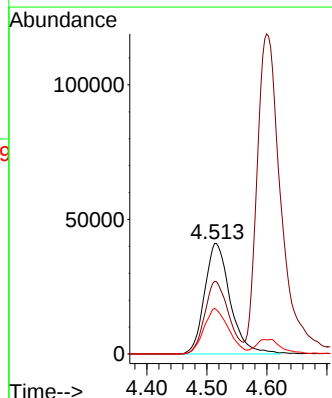
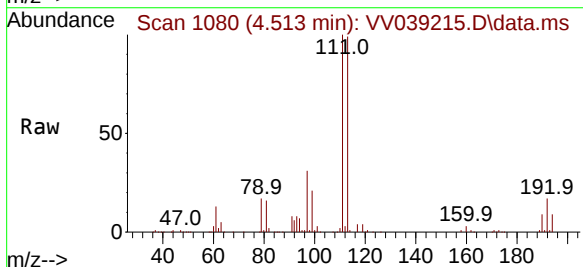




#33
1,2-Dichloroethane-d4
Concen: 58.958 ug/l
RT: 4.944 min Scan# 11
Delta R.T. 0.006 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05




Instrument :
MSVOA_V
ClientSampleId :
MW-31D-091825


Tgt Ion: 65 Resp: 446631
Ion Ratio Lower Upper
65 100
67 54.0 0.0 107.0

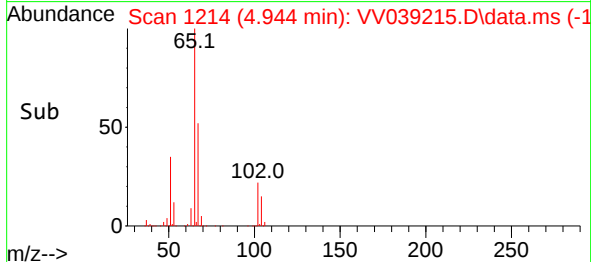

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 5.535 min Scan# 1398
Delta R.T. 0.006 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05

Tgt Ion: 114 Resp: 967034
Ion Ratio Lower Upper
114 100
63 19.2 0.0 42.6
88 15.7 0.0 30.8


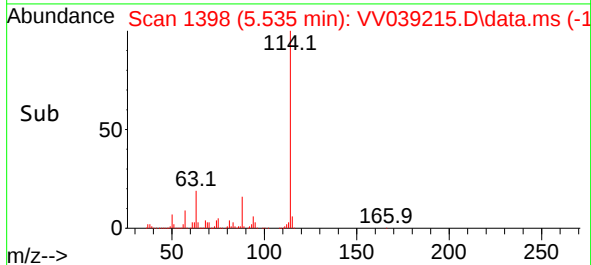

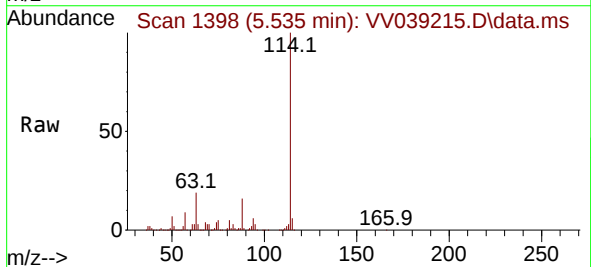




#35
Dibromofluoromethane
Concen: 54.680 ug/l
RT: 4.500 min Scan# 1107
Delta R.T. 0.003 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05




Instrument :
MSVOA_V
ClientSampleId :
MW-31D-091825


Tgt Ion:113 Resp: 425088
Ion Ratio Lower Upper
113 100
111 102.1 82.4 123.6
192 17.5 13.8 20.8

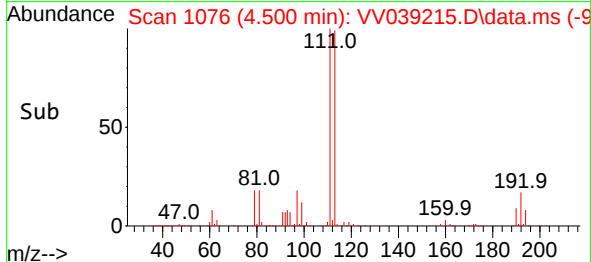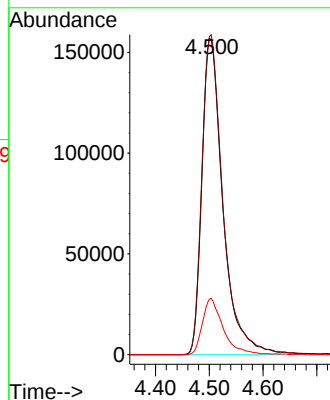

#36
1,1-Dichloropropene
Concen: 4.135 ug/l
RT: 4.600 min Scan# 1107
Delta R.T. -0.141 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05

Tgt Ion: 75 Resp: 48605
Ion Ratio Lower Upper
75 100
110 8.8 18.1 54.1#
77 0.1 24.8 37.2#


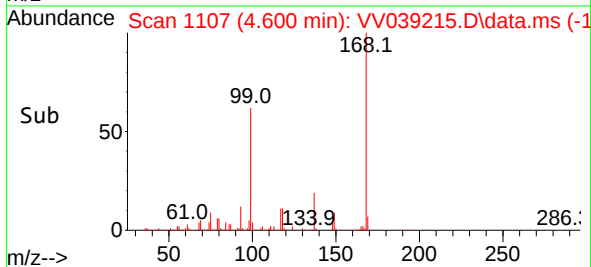
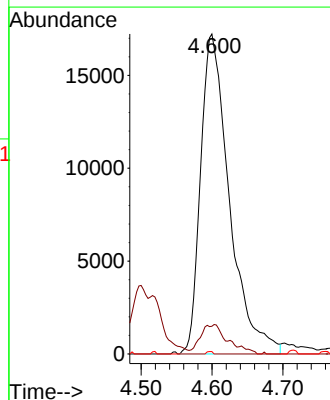
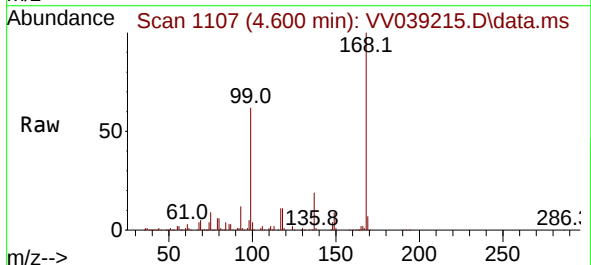


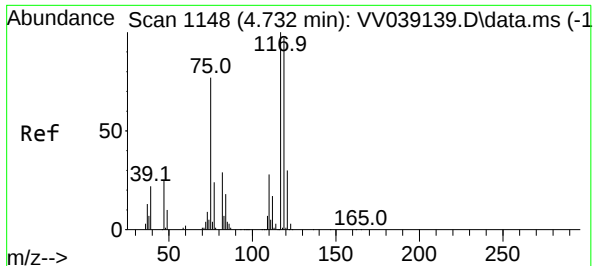

#38
Carbon Tetrachloride
Concen: 3.733 ug/l
RT: 4.600 min Scan# 1148
Delta R.T. -0.132 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05




Instrument :
MSVOA_V
ClientSampleId :
MW-31D-091825


Tgt Ion:117 Resp: 53629
Ion Ratio Lower Upper
117 100
119 7.4 77.2 115.8#
121 0.0 24.2 36.2#

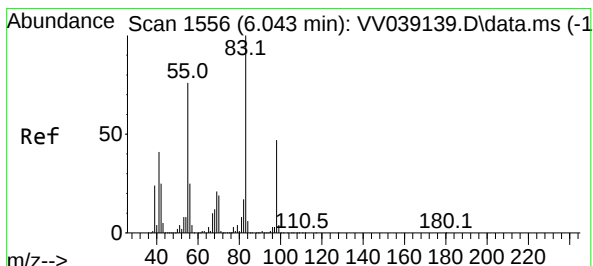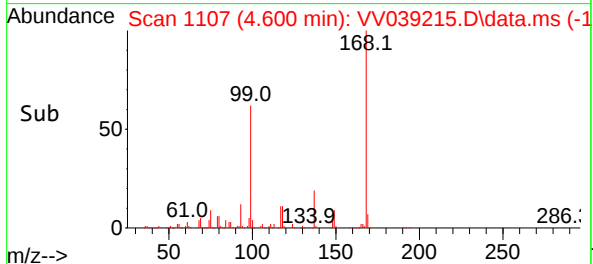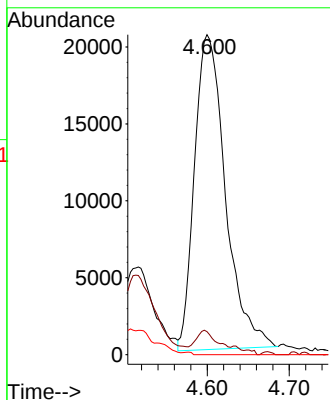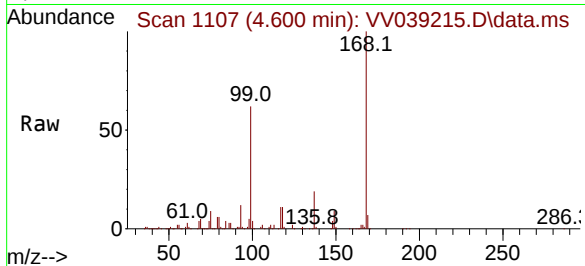

#39
Methylcyclohexane
Concen: 2.163 ug/l
RT: 5.828 min Scan# 1489
Delta R.T. -0.215 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05

Tgt Ion: 83 Resp: 30697
Ion Ratio Lower Upper
83 100
55 1.2 60.5 90.7#
98 178.7 37.8 56.6#


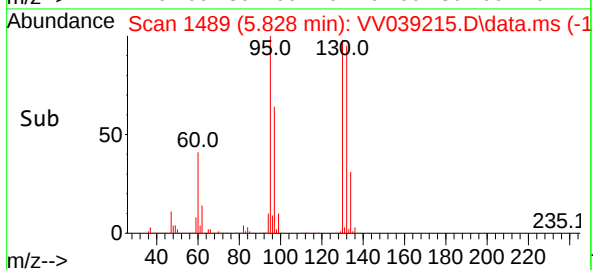
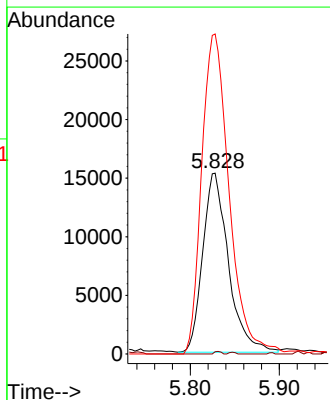
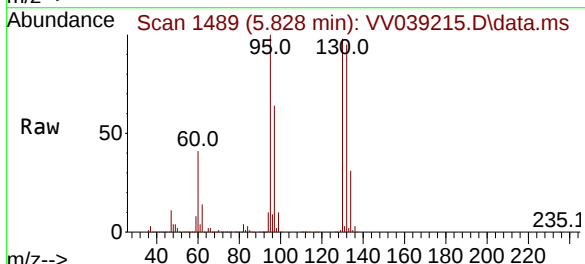




#41
Methacrylonitrile
Concen: 1.913 ug/l
RT: 4.162 min Scan# 91
Delta R.T. 0.009 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05




Instrument :
MSVOA_V
ClientSampleId :
MW-31D-091825


Tgt Ion:	41	Resp:	20
Ion	Ratio	Lower	Upper
41	100		
39	0.0	42.2	63.2#
67	0.0	67.9	101.9#
52	0.0	26.7	40.1#

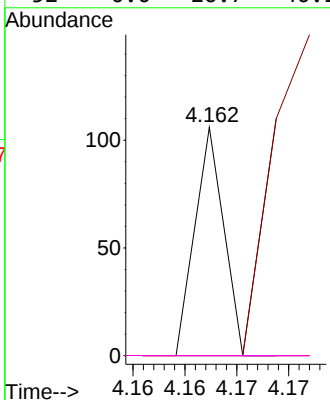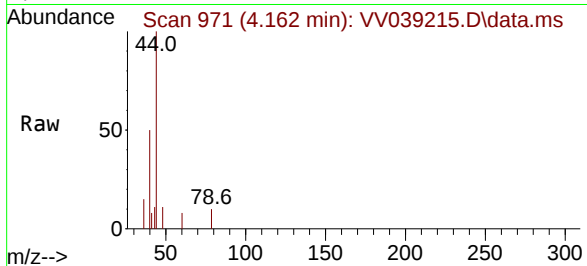

#44
Trichloroethene
Concen: 267.708 ug/l
RT: 5.828 min Scan# 1489
Delta R.T. -0.000 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05

Tgt Ion:	130	Resp:	2364403
Ion	Ratio	Lower	Upper
130	100		
95	101.6	0.0	199.2

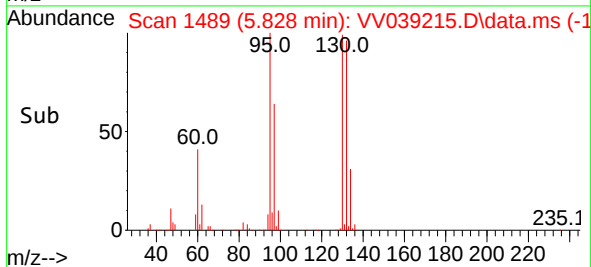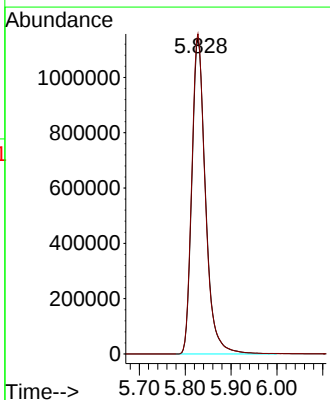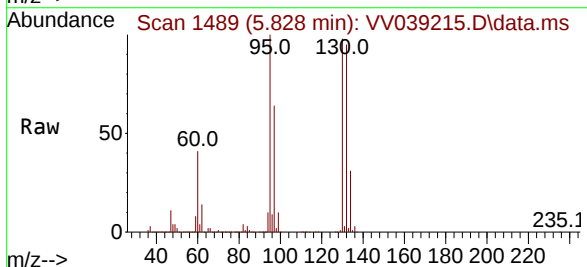



#49

1,4-Dioxane

Concen: 5.912 ug/l

RT: 6.333 min Scan# 1

Delta R.T. 0.045 min

Lab File: VV039215.D

Acq: 26 Sep 2025 16:05

Instrument :

MSVOA_V

ClientSampleId :

MW-31D-091825





Tgt Ion: 88 Resp: 841

Ion Ratio Lower Upper

88 100

43 34.6 25.1 37.7

58 14.6 53.6 80.4#



#50

Toluene-d8

Concen: 48.235 ug/l

RT: 7.236 min Scan# 1927

Delta R.T. 0.003 min

Lab File: VV039215.D




Acq: 26 Sep 2025 16:05


Tgt Ion: 98 Resp: 1101338

Ion Ratio Lower Upper

98 100

100 64.2 52.2 78.2


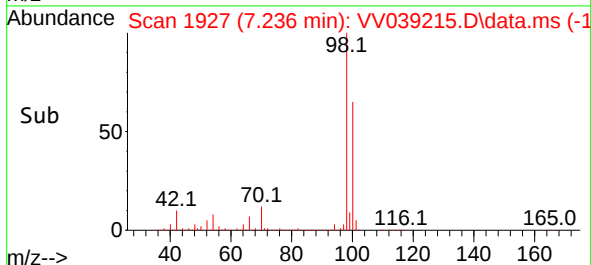
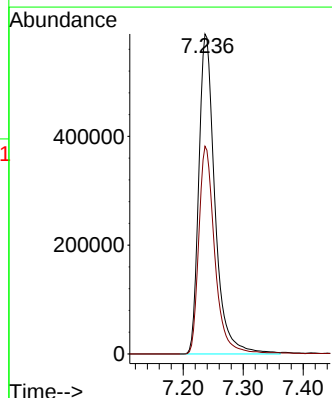
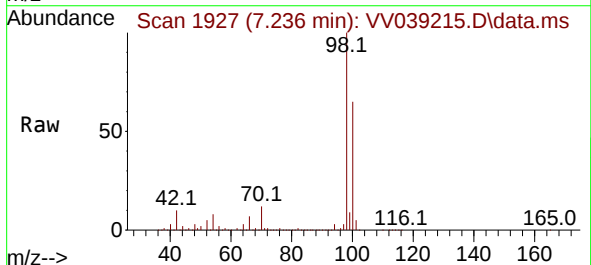




#51
4-Methyl-2-Pentanone
Concen: 0.336 ug/l
RT: 7.236 min Scan# 1927
Delta R.T. 0.090 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05




Instrument :
MSVOA_V
ClientSampleId :
MW-31D-091825


Tgt Ion: 43 Resp: 4297
Ion Ratio Lower Upper
43 100
58 213.0 32.3 48.5#

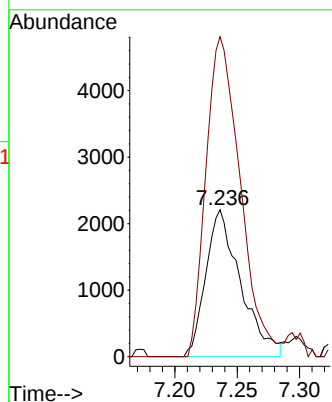

#58
2-Chloroethyl Vinyl ether
Concen: 9.639 ug/l
RT: 6.818 min Scan# 1797
Delta R.T. 0.009 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05

Tgt Ion: 63 Resp: 114
Ion Ratio Lower Upper
63 100
106 0.0 22.1 33.1#


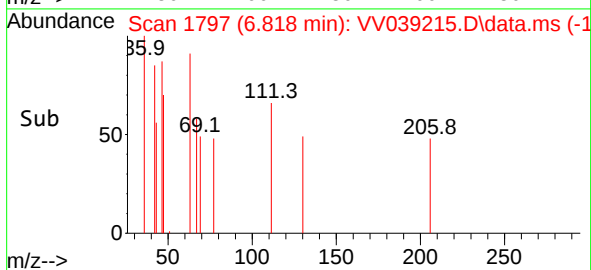
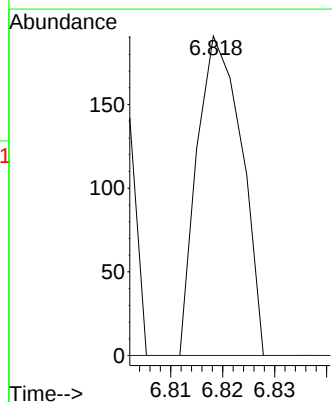
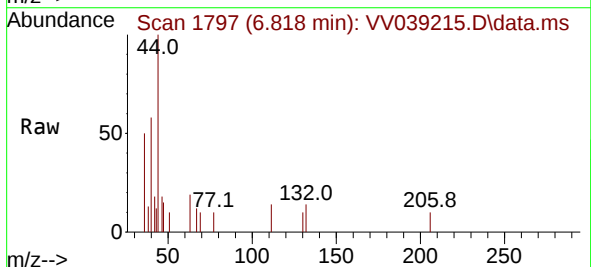




#59
2-Hexanone
Concen: 2.330 ug/l
RT: 8.130 min Scan# 2183
Delta R.T. 0.071 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05




Instrument :
MSVOA_V
ClientSampleId :
MW-31D-091825


Tgt Ion: 43 Resp: 43
Ion Ratio Lower Upper
43 100
58 48.8 28.3 85.0

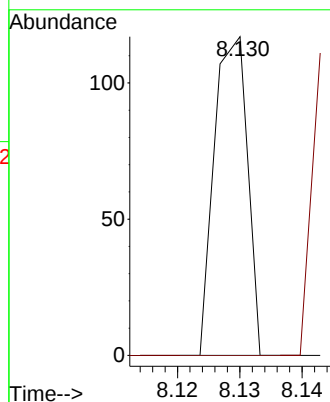

#62
4-Bromofluorobenzene
Concen: 43.934 ug/l
RT: 10.001 min Scan# 2787
Delta R.T. 0.003 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05

Tgt Ion: 95 Resp: 412962
Ion Ratio Lower Upper
95 100
174 75.6 0.0 150.4
176 72.9 0.0 144.2


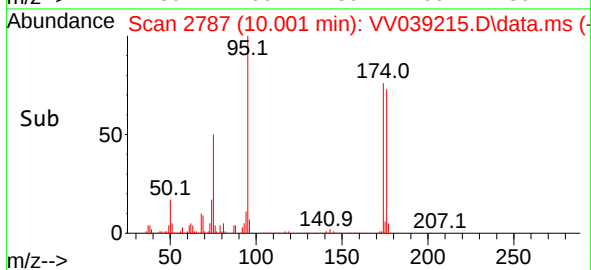
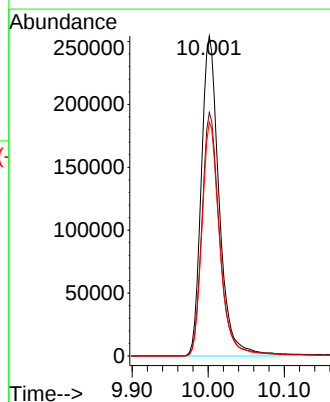
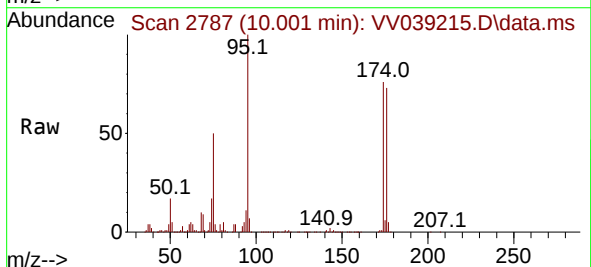




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 8.776 min Scan# 2405
Delta R.T. 0.003 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05




Instrument :
MSVOA_V
ClientSampleId :
MW-31D-091825


Tgt Ion:117 Resp: 980974
Ion Ratio Lower Upper
117 100
82 54.2 45.4 68.2
119 32.0 25.6 38.4



#64
Tetrachloroethene
Concen: 0.254 ug/l
RT: 7.911 min Scan# 2137
Delta R.T. 0.016 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05

Tgt Ion:164 Resp: 2084
Ion Ratio Lower Upper
164 100
166 115.9 101.6 152.4
129 102.9 78.5 117.7
131 113.8 76.8 115.2


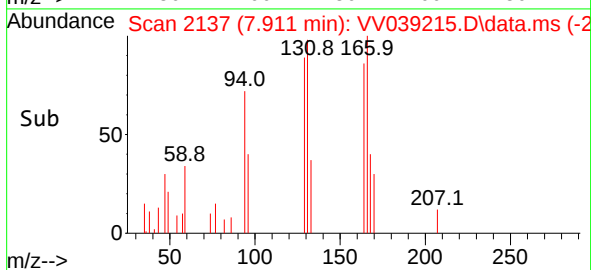






#70
Styrene
Concen: 1.564 ug/l
RT: 9.558 min Scan# 2649
Delta R.T. 0.074 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05




Instrument :
MSVOA_V
ClientSampleId :
MW-31D-091825


Tgt Ion:104 Resp: 76
Ion Ratio Lower Upper
104 100
78 27.6 39.8 59.6#
103 0.0 43.4 65.2#



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.175 min Scan# 3152
Delta R.T. 0.003 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05

Tgt Ion:152 Resp: 469900
Ion Ratio Lower Upper
152 100
115 62.1 44.8 134.4
150 157.2 0.0 353.8



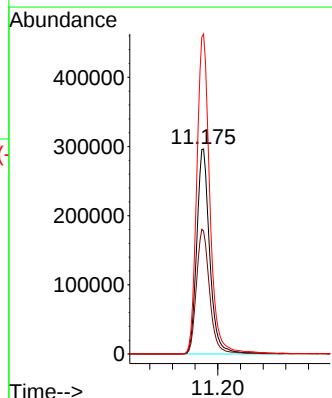





#76
1,2,3-Trichloropropane
Concen: 19.538 ug/l
RT: 10.001 min Scan# 21
Delta R.T. -0.193 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05




Instrument :
MSVOA_V
ClientSampleId :
MW-31D-091825


Tgt Ion: 75 Resp: 209031
Ion Ratio Lower Upper
75 100
77 1.4 11.3 33.8#

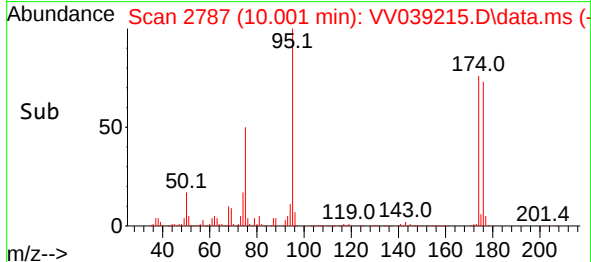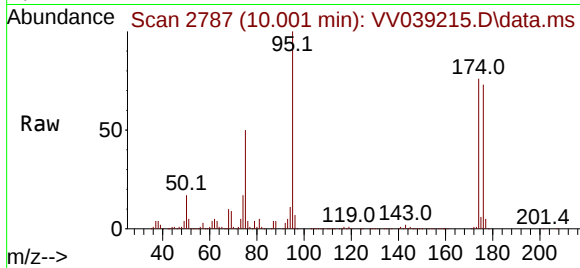

#81
trans-1,4-Dichloro-2-butene
Concen: 46.904 ug/l
RT: 10.001 min Scan# 2787
Delta R.T. 0.074 min
Lab File: VV039215.D
Acq: 26 Sep 2025 16:05

Tgt Ion: 75 Resp: 209031
Ion Ratio Lower Upper
75 100
53 0.5 72.5 108.7#
89 0.0 37.2 55.8#

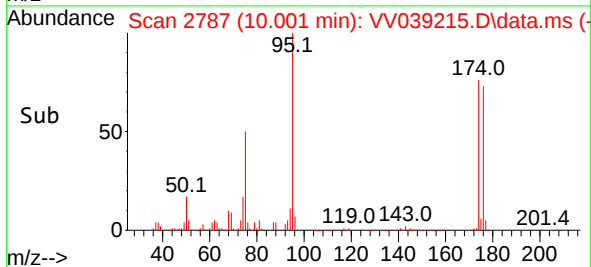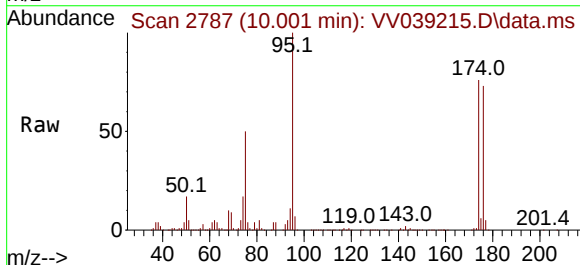



#92
 1,2-Dibromo-3-Chloropropane
 Concen: Below Cal
 RT: 12.352 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV039215.D
 Acq: 26 Sep 2025 16:05

Instrument :
 MSVOA_V
 ClientSampleId :
 MW-31D-091825

Tgt Ion	Ratio	Lower	Upper
75	100		
155	0.0	38.6	115.8#
157	0.0	49.5	148.3#

