
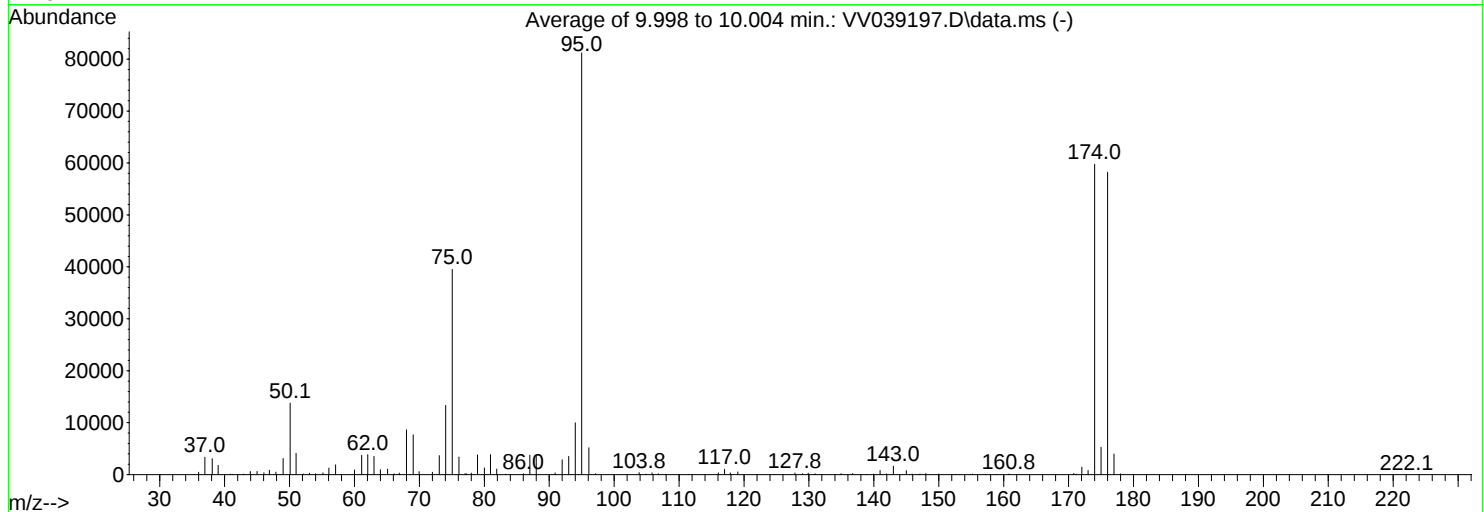


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092625\
Data File : VV039197.D
Acq On : 26 Sep 2025 08:14
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M
Title : SW846 8260
Last Update : Wed Sep 24 08:08:08 2025

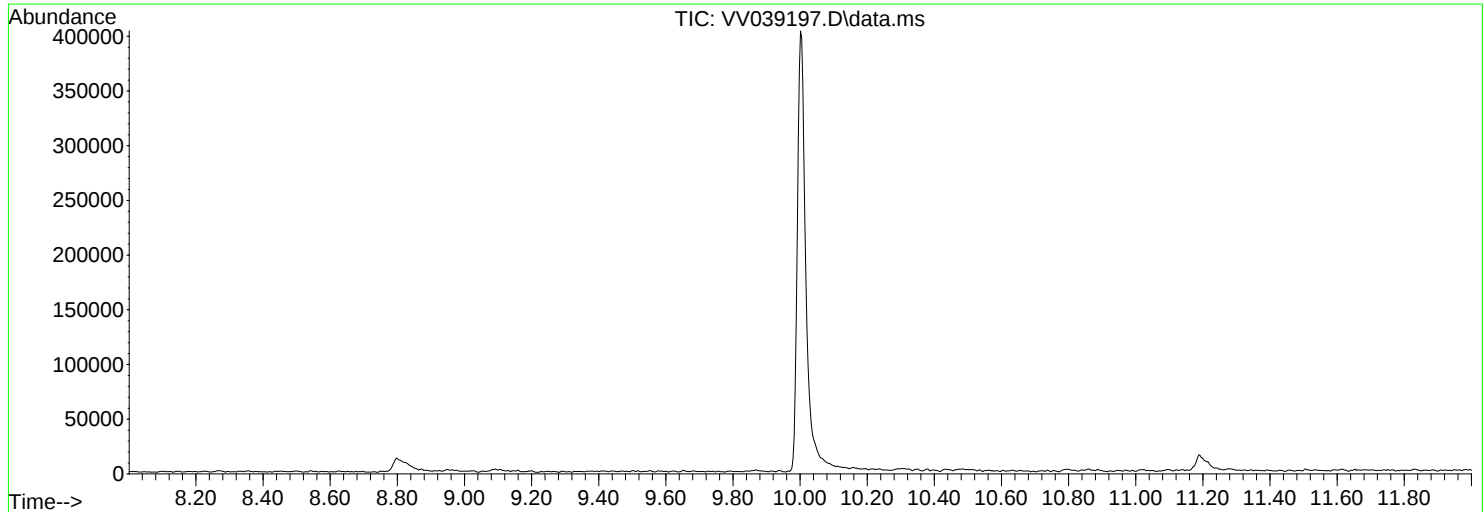

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2772

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	13756	PASS
75	95	30	60	48.7	39531	PASS
95	95	100	100	100.0	81205	PASS
96	95	5	9	6.4	5186	PASS
173	174	0.00	2	1.4	815	PASS
174	95	50	100	73.6	59763	PASS
175	174	5	9	8.8	5272	PASS
176	174	95	101	97.4	58227	PASS
177	176	5	9	6.8	3983	PASS