

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092718\
 Data File : VV007902.D
 Acq On : 27 Sep 2018 12:31
 Operator : SY/MD
 Sample : J5063-02
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAC23

Quant Time: Sep 28 01:52:54 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 28 00:42:21 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	92195	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	85840	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	43988	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	23172	4.69	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.80%
7) Chloroethane-d5	1.59	69	21171	4.96	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.20%
11) 1,1-Dichloroethene-d2	2.14	63	37479	3.36	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.20%
20) 2-Butanone-d5	3.97	46	66022	44.41	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.82%
24) Chloroform-d	4.41	84	51615	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.60%
26) 1,2-Dichloroethane-d4	5.09	65	28810	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.00%
32) Benzene-d6	5.10	84	103114	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.60%
36) 1,2-Dichloropropane-d6	6.12	67	31823	4.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.00%
41) Toluene-d8	7.36	98	97717	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.60%
43) trans-1,3-Dichloropropene-	7.67	79	10751	4.30	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.00%
46) 2-Hexanone-d5	8.14	63	49340	44.69	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.38%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	22546	4.50	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	40735	4.78	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.60%


Target Compounds					Ovalue
13) Acetone	2.22	43	5916	5.462 ug/L	98
30) Cyclohexane	4.73	56	2491	0.257 ug/L	95
31) Carbon tetrachloride	4.88	117	8273	0.909 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092718\
Data File : VV007902.D
Acq On : 27 Sep 2018 12:31
Operator : SY/MD
Sample : J5063-02
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAC23

Quant Time: Sep 28 01:52:54 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 28 00:42:21 2018
Response via : Initial Calibration

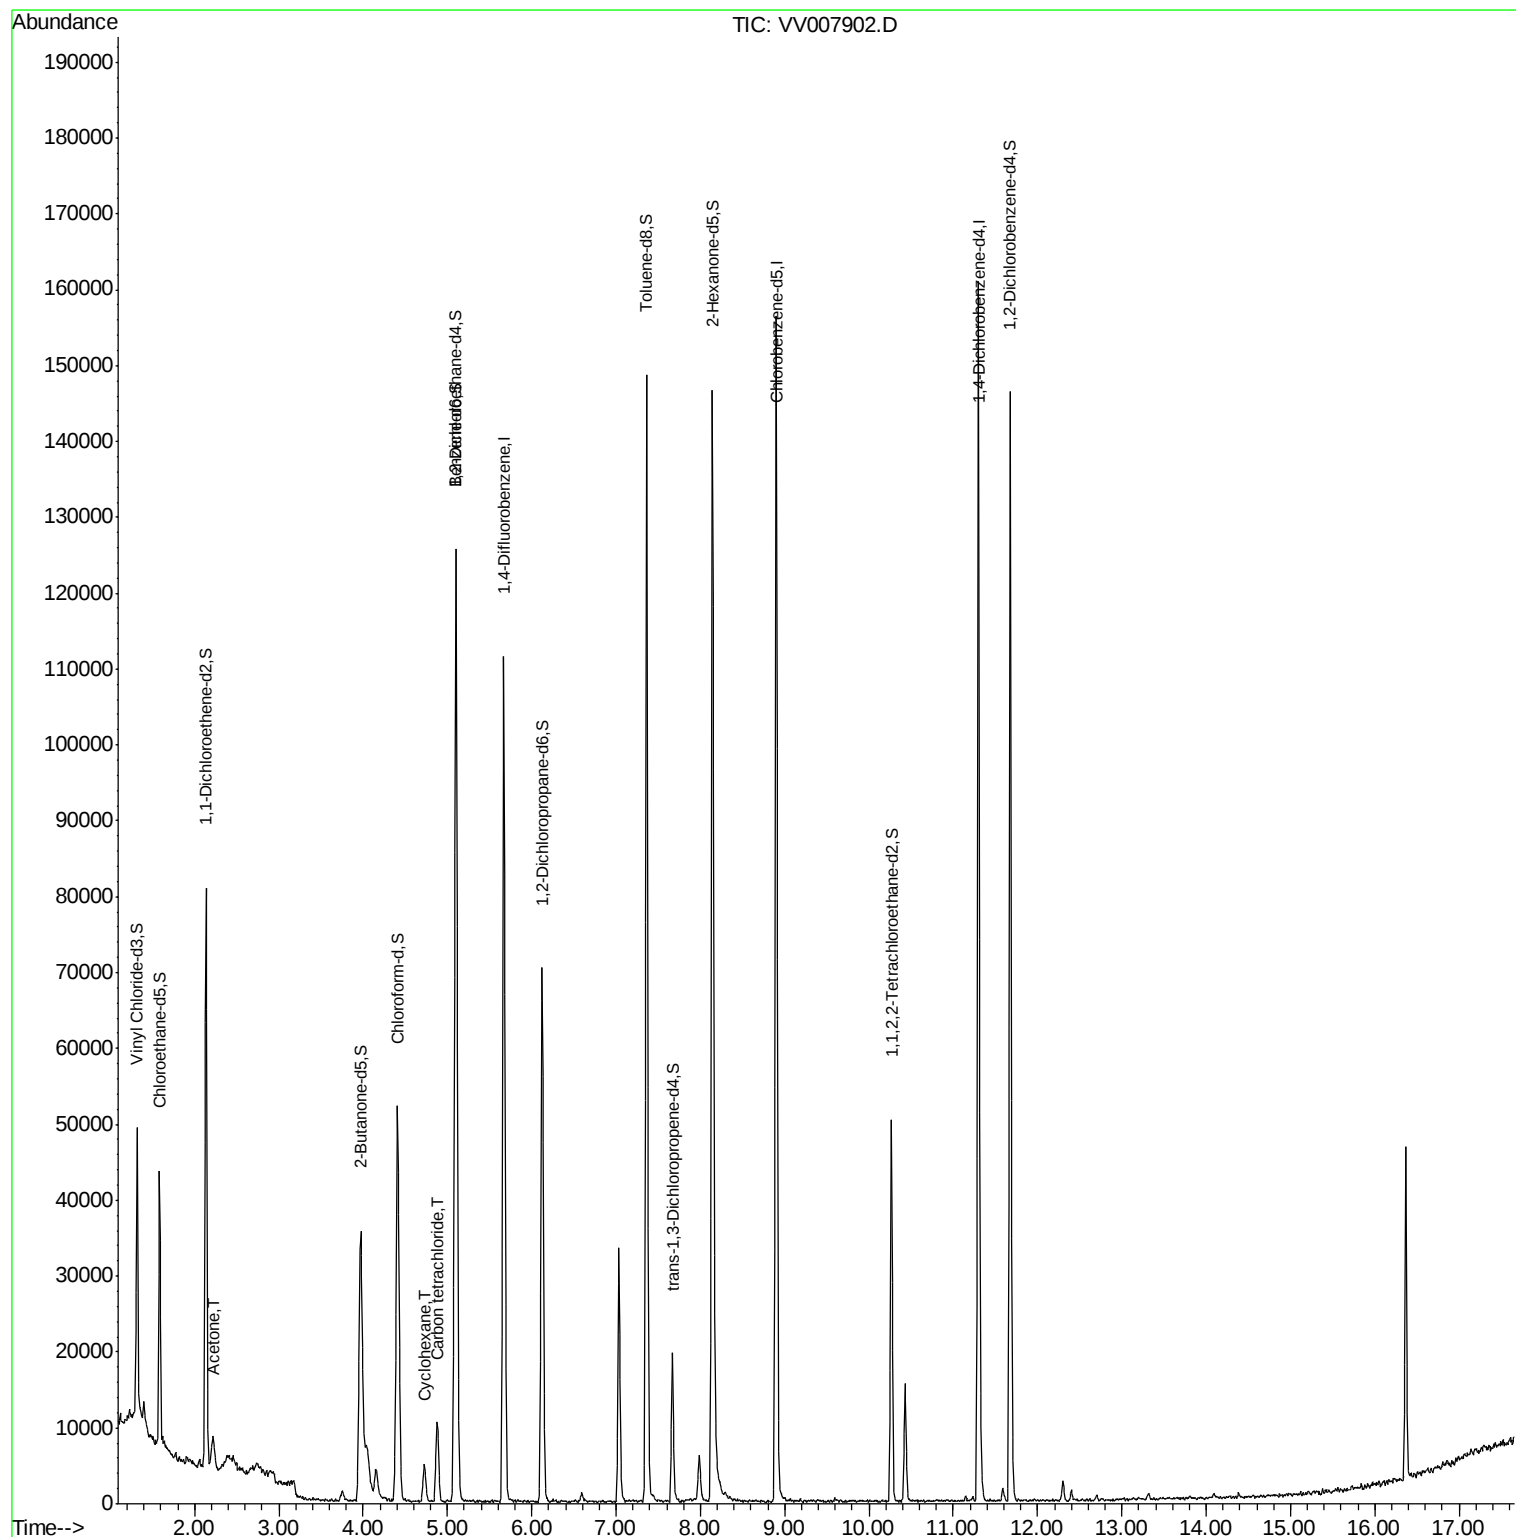

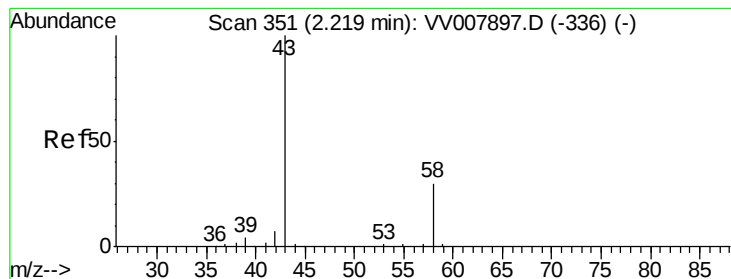

#13

Acetone

Concen: 5.462 ug/L

RT: 2.22 min Scan# 351

Delta R.T. 0.00 min

Lab File: VV007902.D

Acq: 27 Sep 2018 12:31

Instrument :

MSVOA_V

ClientSampled :


GAC23

Tot Ion: 43 Resp: 5916

Ion Ratio Lower Upper

43 100

58 30.1 0.0 62.0

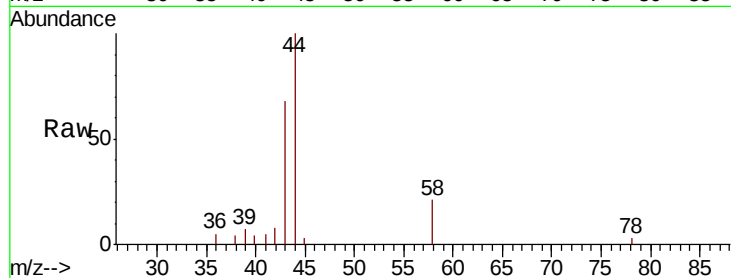

Abundance Ion 43.05 (42.75 to 43.75): VV007897.D (-336) (-)



Ion 58.05 (57.75 to 58.75): VV007897.D (-336) (-)

2.22

2.25

2.30

Time-->

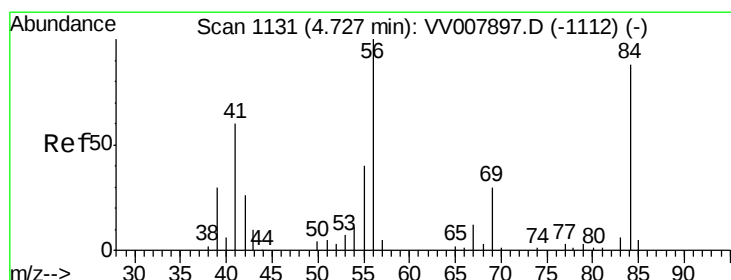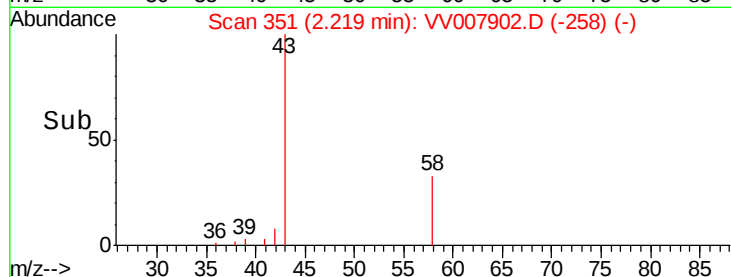

#30

Cyclohexane

Concen: 0.257 ug/L

RT: 4.73 min Scan# 1132

Delta R.T. 0.00 min

Lab File: VV007902.D

Acq: 27 Sep 2018 12:31


Tgt Ion: 56 Resp: 2491

Ion Ratio Lower Upper

56 100

69 32.2 24.2 36.4

84 82.3 69.8 104.8

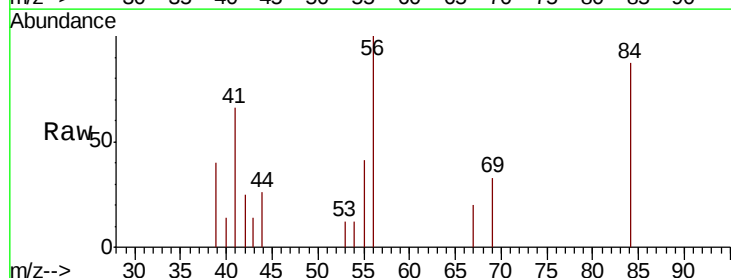

Abundance Ion 56.10 (55.80 to 56.80): VV007897.D (-1112) (-)


Ion 69.15 (68.85 to 69.85): VV007897.D (-1112) (-)


Ion 84.15 (83.85 to 84.85): VV007897.D (-1112) (-)

4.73

4.75

Time-->

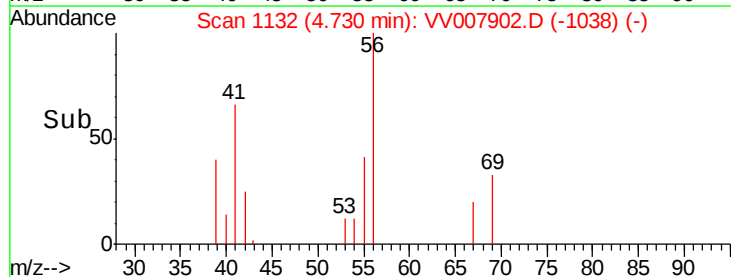

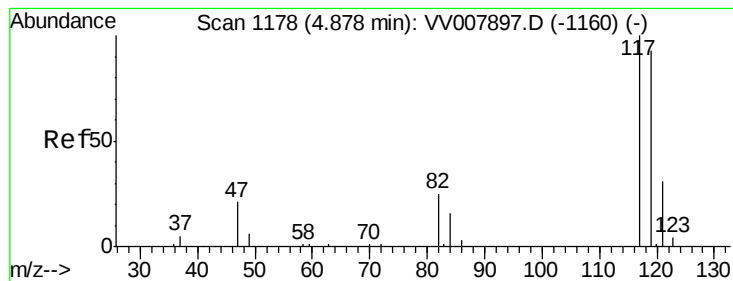

#31

Carbon tetrachloride

Concen: 0.909 ug/L

RT: 4.88 min Scan# 1179

Delta R.T. 0.00 min

Lab File: VV007902.D

Acq: 27 Sep 2018 12:31

Instrument :

MSVOA_V

ClientSampleId :

GAC23

Tot Ion:117 Resp: 8273

Ion Ratio Lower Upper

117 100

119 92.5 77.8 116.8

