

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092718\
 Data File : VV007905.D
 Acq On : 27 Sep 2018 13:53
 Operator : SY/MD
 Sample : J5063-05
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAC26

Quant Time: Sep 28 02:05:41 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 28 00:42:21 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	85699	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	80480	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	41105	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	22384	4.87	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.40%
7) Chloroethane-d5	1.59	69	20467	5.16	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.20%
11) 1,1-Dichloroethene-d2	2.14	63	38023	3.66	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.20%
20) 2-Butanone-d5	3.96	46	64823	46.91	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.82%
24) Chloroform-d	4.41	84	51482	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.40%
26) 1,2-Dichloroethane-d4	5.09	65	28766	5.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.00%
32) Benzene-d6	5.10	84	100100	5.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.20%
36) 1,2-Dichloropropane-d6	6.13	67	31703	5.20	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.00%
41) Toluene-d8	7.36	98	94530	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
43) trans-1,3-Dichloropropene-	7.67	79	10856	4.63	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.60%
46) 2-Hexanone-d5	8.14	63	47889	46.26	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.52%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	22706	4.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	39701	4.99	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.80%


Target Compounds					Ovalue
13) Acetone	2.21	43	5010	4.976 ug/L	99
30) Cyclohexane	4.72	56	1681	0.185 ug/L	91
31) Carbon tetrachloride	4.88	117	270997	31.765 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092718\
Data File : VV007905.D
Acq On : 27 Sep 2018 13:53
Operator : SY/MD
Sample : J5063-05
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAC26

Quant Time: Sep 28 02:05:41 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 28 00:42:21 2018
Response via : Initial Calibration

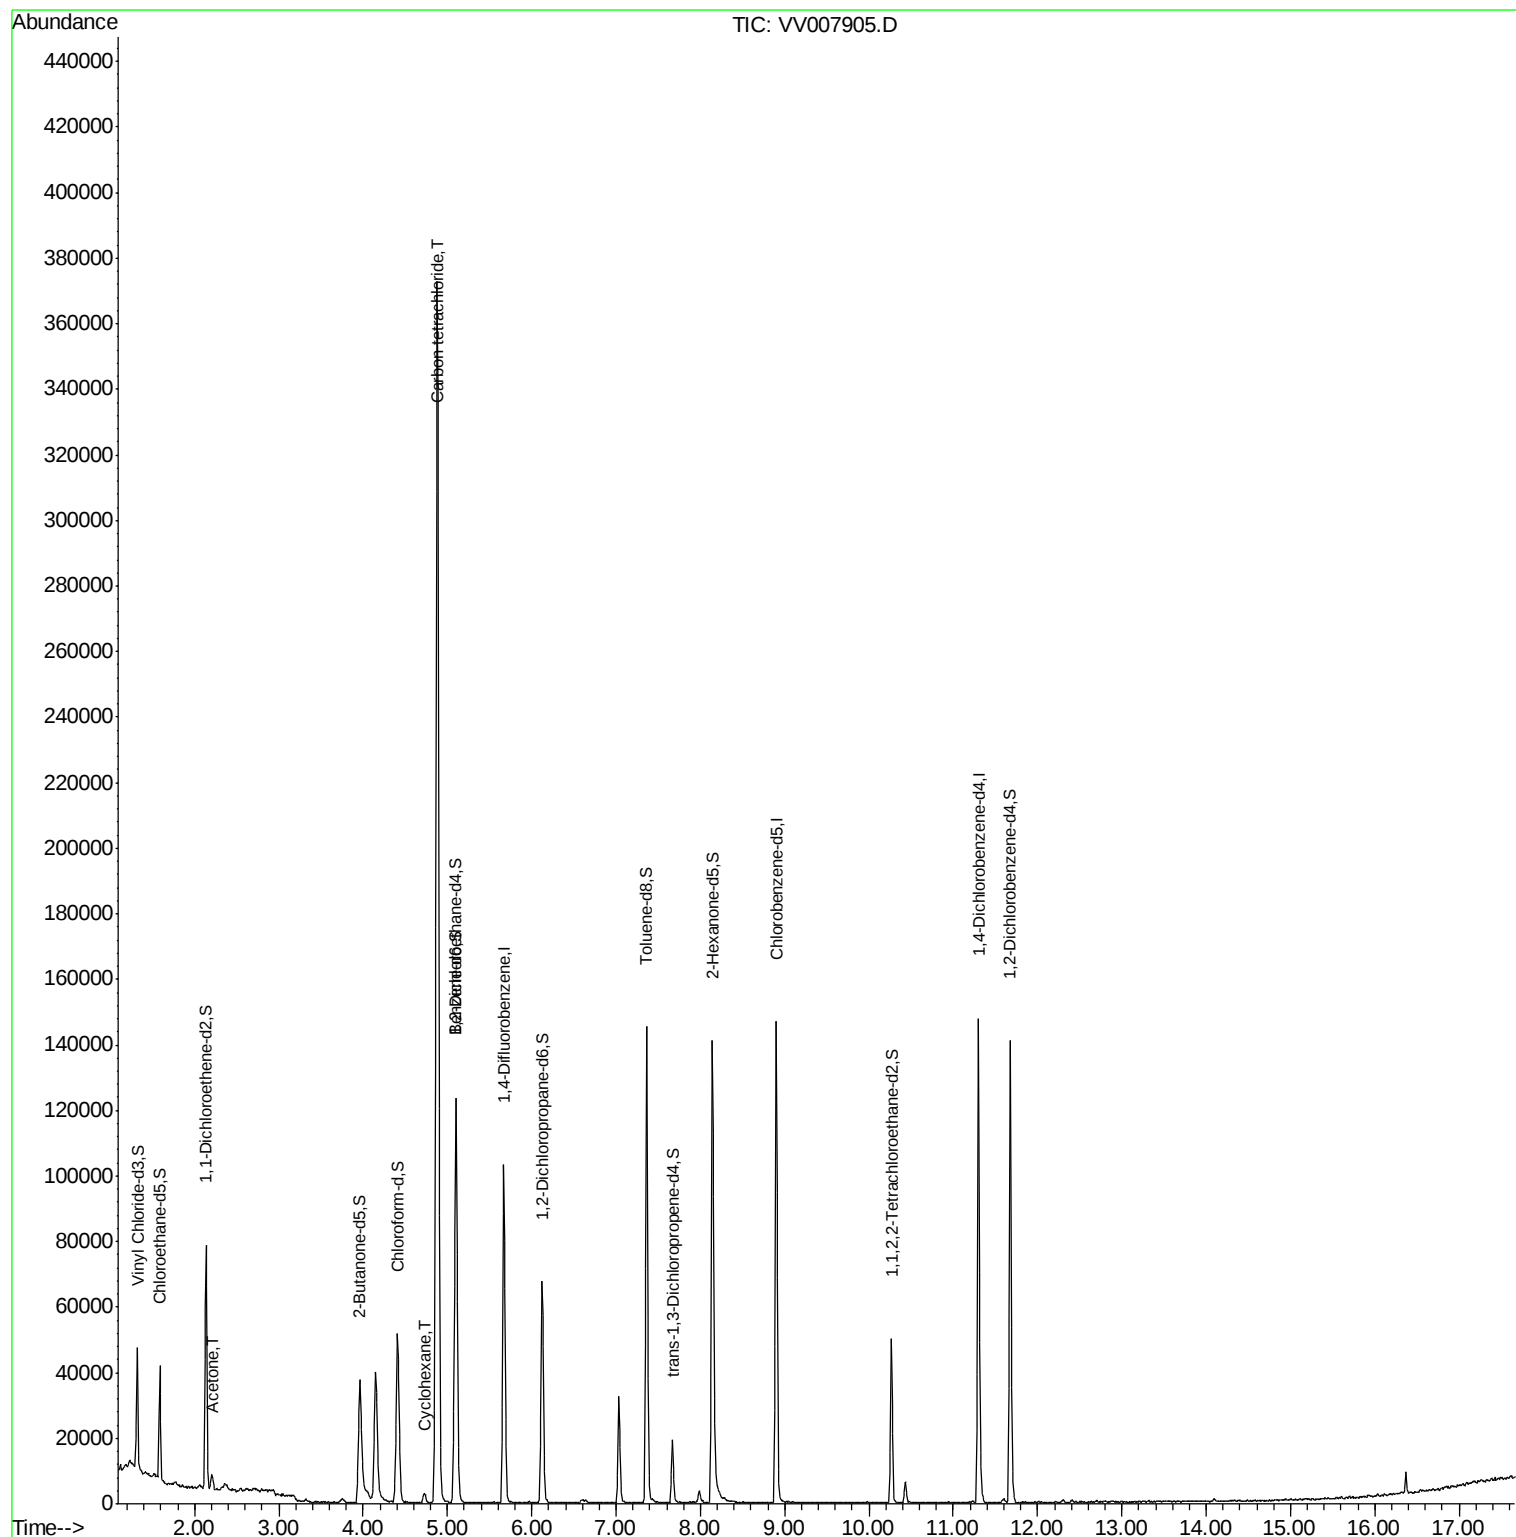

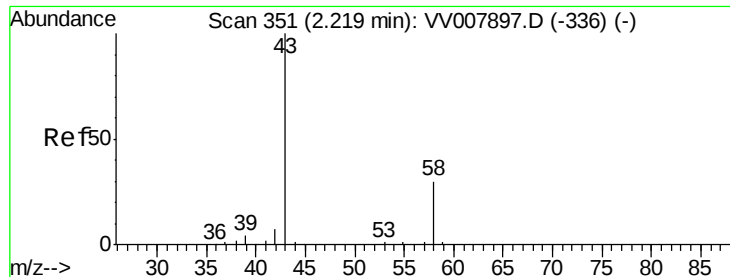

#13

Acetone

Concen: 4.976 ug/L

RT: 2.21 min Scan# 347

Delta R.T. -0.01 min

Lab File: VV007905.D

Acq: 27 Sep 2018 13:53

Instrument :

MSVOA_V

ClientSampled :


GAC26

Tot Ion: 43 Resp: 5010

Ion Ratio Lower Upper




43 100

58 31.4 0.0 62.0

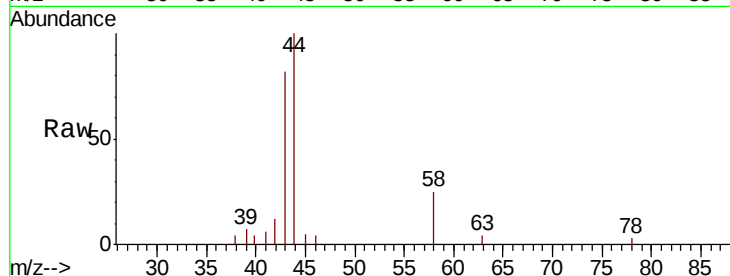

Abundance Ion 43.05 (42.75 to 43.75): VV007897.D (-336) (-)

Ion 58.05 (57.75 to 58.75): VV007897.D (-336) (-)

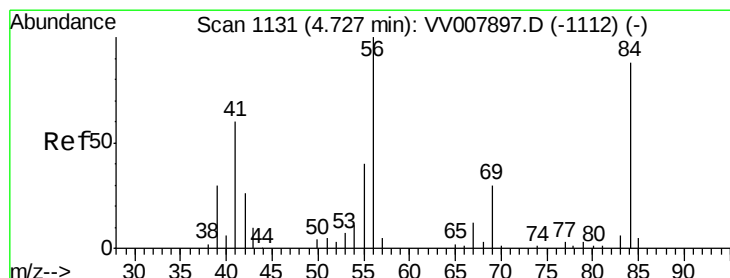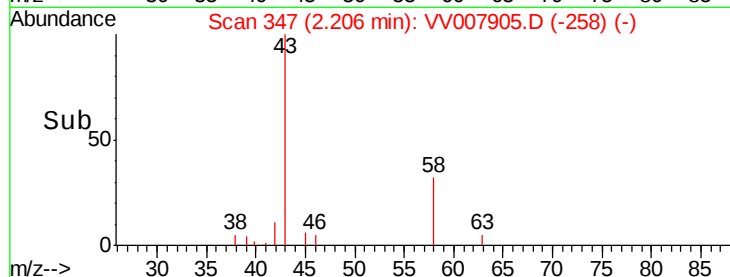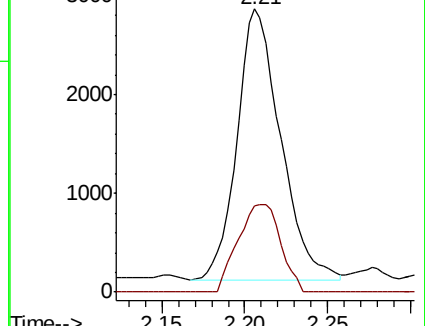

#30

Cyclohexane

Concen: 0.185 ug/L

RT: 4.72 min Scan# 1129

Delta R.T. -0.01 min

Lab File: VV007905.D

Acq: 27 Sep 2018 13:53


Tgt Ion: 56 Resp: 1681

Ion Ratio Lower Upper

56 100

69 34.7 24.2 36.4



84 78.2 69.8 104.8

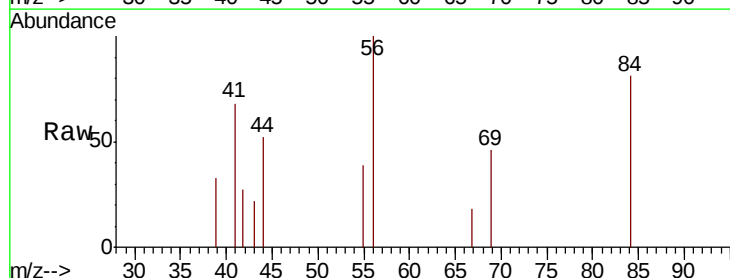


Abundance Ion 56.10 (55.80 to 56.80): VV007897.D (-1112) (-)

Ion 69.15 (68.85 to 69.85): VV007897.D (-1112) (-)

Ion 84.15 (83.85 to 84.85): VV007897.D (-1112) (-)

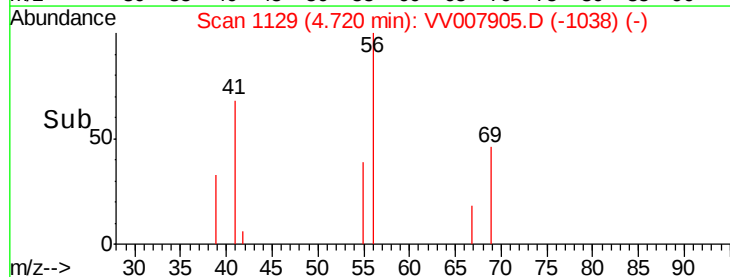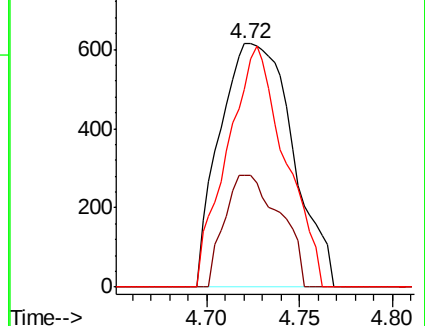

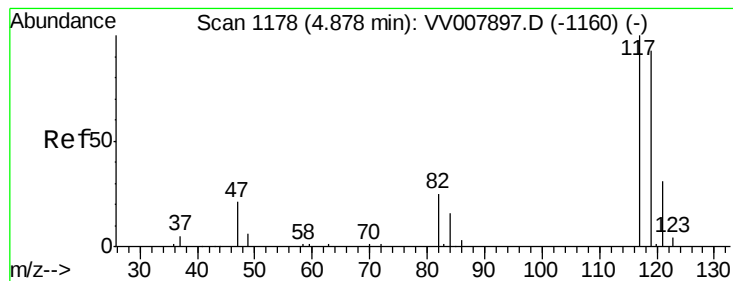

#31

Carbon tetrachloride

Concen: 31.765 ug/L

RT: 4.88 min Scan# 1179

Delta R.T. 0.00 min

Lab File: VV007905.D

Acq: 27 Sep 2018 13:53

Instrument :

MSVOA_V

ClientSampleId :

GAC26

Tot Ion:117 Resp: 270997

Ion Ratio Lower Upper

117 100

119 96.8 77.8 116.8

