

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092718\
 Data File : VV007922.D
 Acq On : 27 Sep 2018 22:07
 Operator : SY/MD
 Sample : J4989-18
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ET0S9

Quant Time: Sep 28 04:04:00 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 28 03:46:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	89932	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	85968	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	42545	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	21363	4.43	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.60%
7) Chloroethane-d5	1.58	69	19228	4.62	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.40%
11) 1,1-Dichloroethene-d2	2.13	63	35442	3.26	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.20%
20) 2-Butanone-d5	3.98	46	67026	46.22	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.44%
24) Chloroform-d	4.41	84	48839	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.00%
26) 1,2-Dichloroethane-d4	5.09	65	27274	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.40%
32) Benzene-d6	5.10	84	95939	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.40%
36) 1,2-Dichloropropane-d6	6.13	67	30037	4.62	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.40%
41) Toluene-d8	7.36	98	89656	4.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.80%
43) trans-1,3-Dichloropropene-	7.67	79	10049	4.01	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.20%
46) 2-Hexanone-d5	8.14	63	47763	43.19	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.38%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	21943	4.37	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	37756	4.58	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.60%


Target Compounds					Ovalue
13) Acetone	2.23	43	19250	18.220 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092718\
Data File : VV007922.D
Acq On : 27 Sep 2018 22:07
Operator : SY/MD
Sample : J4989-18
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETOS9

Quant Time: Sep 28 04:04:00 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 28 03:46:50 2018
Response via : Initial Calibration

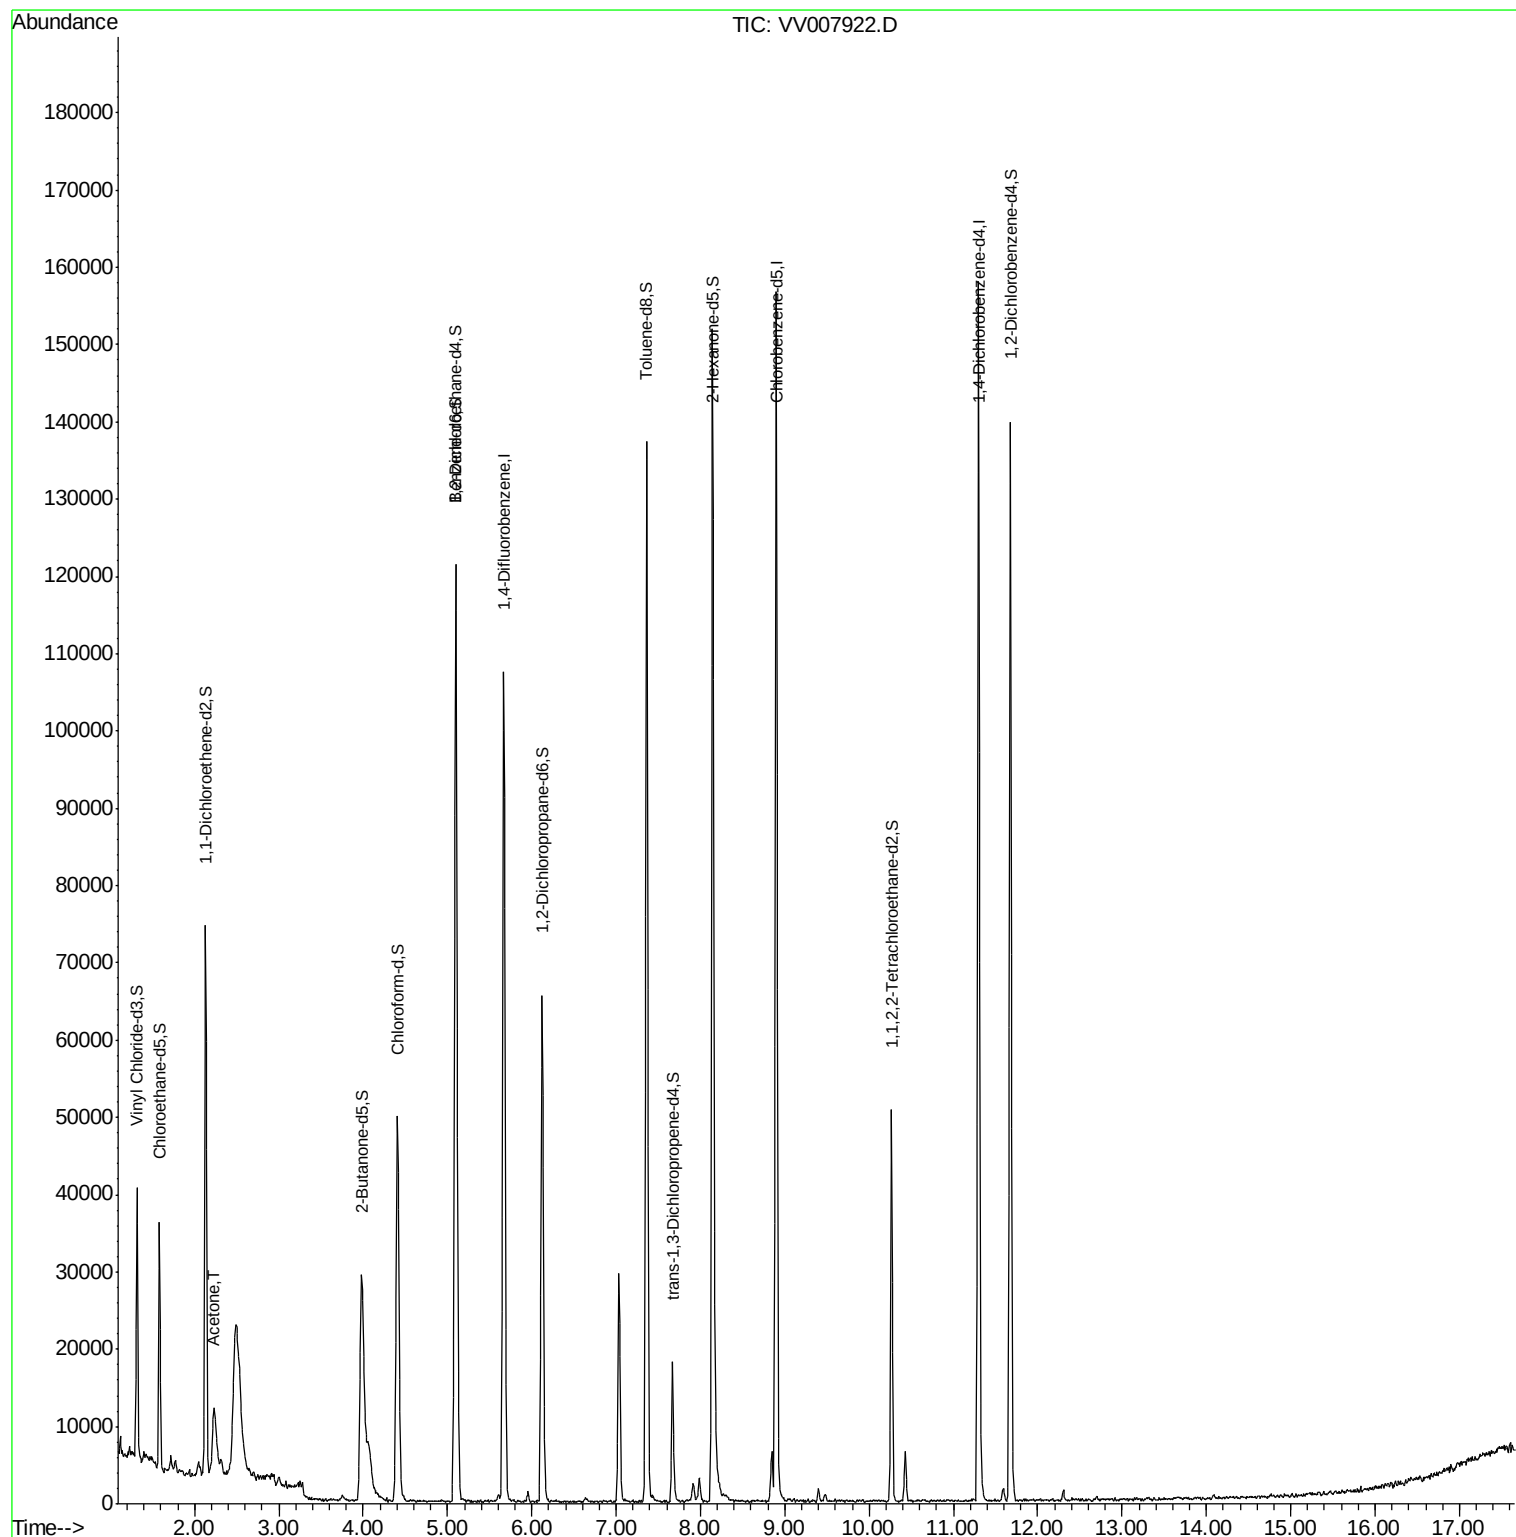

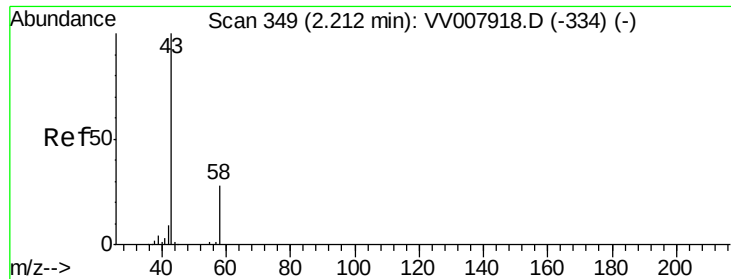

#13
 Acetone
 Concen: 18.220 ug/L
 RT: 2.23 min Scan# 354
 Delta R.T. 0.02 min
 Lab File: VV007922.D
 Acq: 27 Sep 2018 22:07

Instrument :
 MSVOA_V
 ClientSampleId :
 ET0S9

Tot Ion: 43 Resp: 19250
 Ion Ratio Lower Upper
 43 100
 58 30.8 0.0 62.0

