

Data File : VV007924.D
Acq On : 27 Sep 2018 23:02
Operator : SY/MD
Sample : J5063-11
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAC32

Quant Time: Oct 01 04:07:30 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 28 03:46:50 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	86730	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	79345	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	38665	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	20479	4.40	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.00%
7) Chloroethane-d5	1.59	69	19702	4.90	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.00%
11) 1,1-Dichloroethene-d2	2.14	63	35220	3.35	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.00%
20) 2-Butanone-d5	3.96	46	66595	47.62	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.24%
24) Chloroform-d	4.41	84	48990	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.60%
26) 1,2-Dichloroethane-d4	5.09	65	27329	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.80%
32) Benzene-d6	5.10	84	94936	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.20%
36) 1,2-Dichloropropane-d6	6.12	67	30367	5.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.20%
41) Toluene-d8	7.36	98	87672	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.00%
43) trans-1,3-Dichloropropene-	7.67	79	9921	4.29	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.80%
46) 2-Hexanone-d5	8.14	63	47238	46.28	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.56%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	22169	4.78	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	36708	4.90	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.00%


Target Compounds						Qvalue
31) Carbon tetrachloride	4.88	117	295872	35.176	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV007924.D
Acq On : 27 Sep 2018 23:02
Operator : SY/MD
Sample : J5063-11
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAC32

Quant Time: Oct 01 04:07:30 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 28 03:46:50 2018
Response via : Initial Calibration

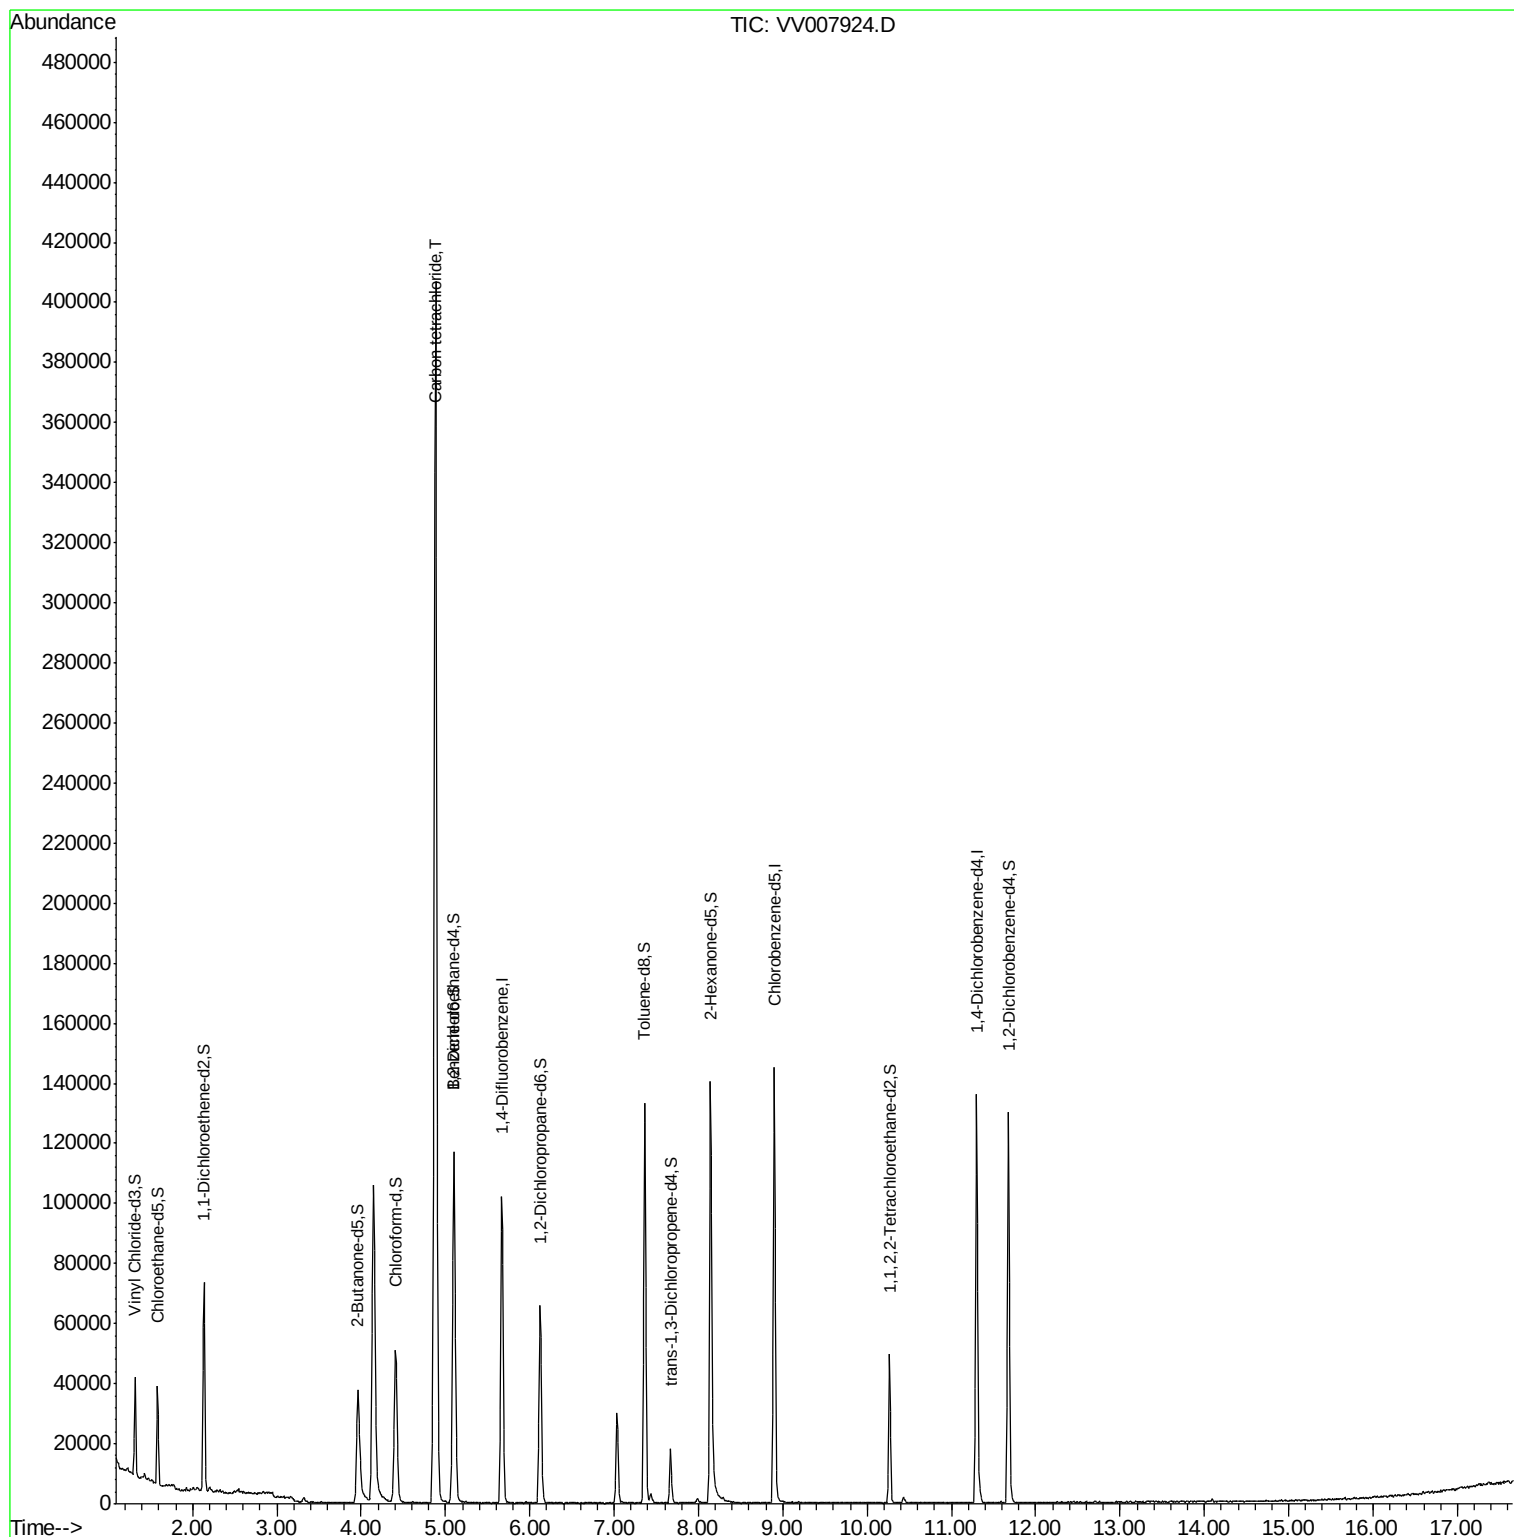

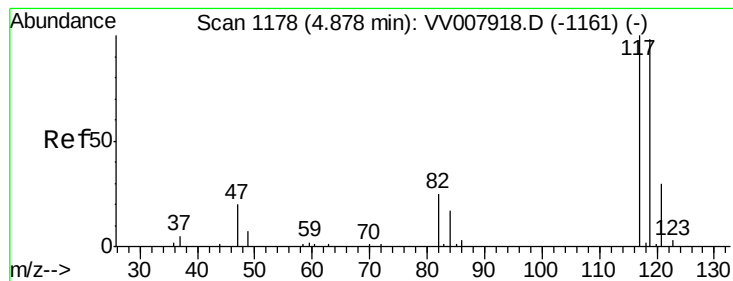

#31

Carbon tetrachloride

Concen: 35.176 ug/L

RT: 4.88 min Scan# 1179

Delta R.T. 0.00 min

Lab File: VV007924.D

Acq: 27 Sep 2018 23:02

Instrument :

MSVOA_V

ClientSampleId :

GAC32

Tgt Ion:117 Resp: 295872

Ion Ratio Lower Upper

117 100

119 95.2 77.8 116.8

