

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092718\
 Data File : VV007925.D
 Acq On : 27 Sep 2018 23:29
 Operator : SY/MD
 Sample : J5063-12
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAC33

Quant Time: Sep 28 04:12:40 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 28 03:46:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	88689	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	83522	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	40340	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	20694	4.35	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.00%
7) Chloroethane-d5	1.59	69	19643	4.78	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.60%
11) 1,1-Dichloroethene-d2	2.14	63	34965	3.26	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.20%
20) 2-Butanone-d5	3.96	46	63092	44.12	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.24%
24) Chloroform-d	4.41	84	48786	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.00%
26) 1,2-Dichloroethane-d4	5.09	65	27152	4.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.20%
32) Benzene-d6	5.10	84	94539	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.80%
36) 1,2-Dichloropropane-d6	6.12	67	29869	4.72	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.40%
41) Toluene-d8	7.36	98	88616	4.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.20%
43) trans-1,3-Dichloropropene-	7.67	79	9715	3.99	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.80%
46) 2-Hexanone-d5	8.14	63	45741	42.58	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.16%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	21802	4.47	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	37231	4.77	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.40%


Target Compounds					Ovalue
31) Carbon tetrachloride	4.88	117	570187	64.400 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092718\
Data File : VV007925.D
Acq On : 27 Sep 2018 23:29
Operator : SY/MD
Sample : J5063-12
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAC33

Quant Time: Sep 28 04:12:40 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 28 03:46:50 2018
Response via : Initial Calibration

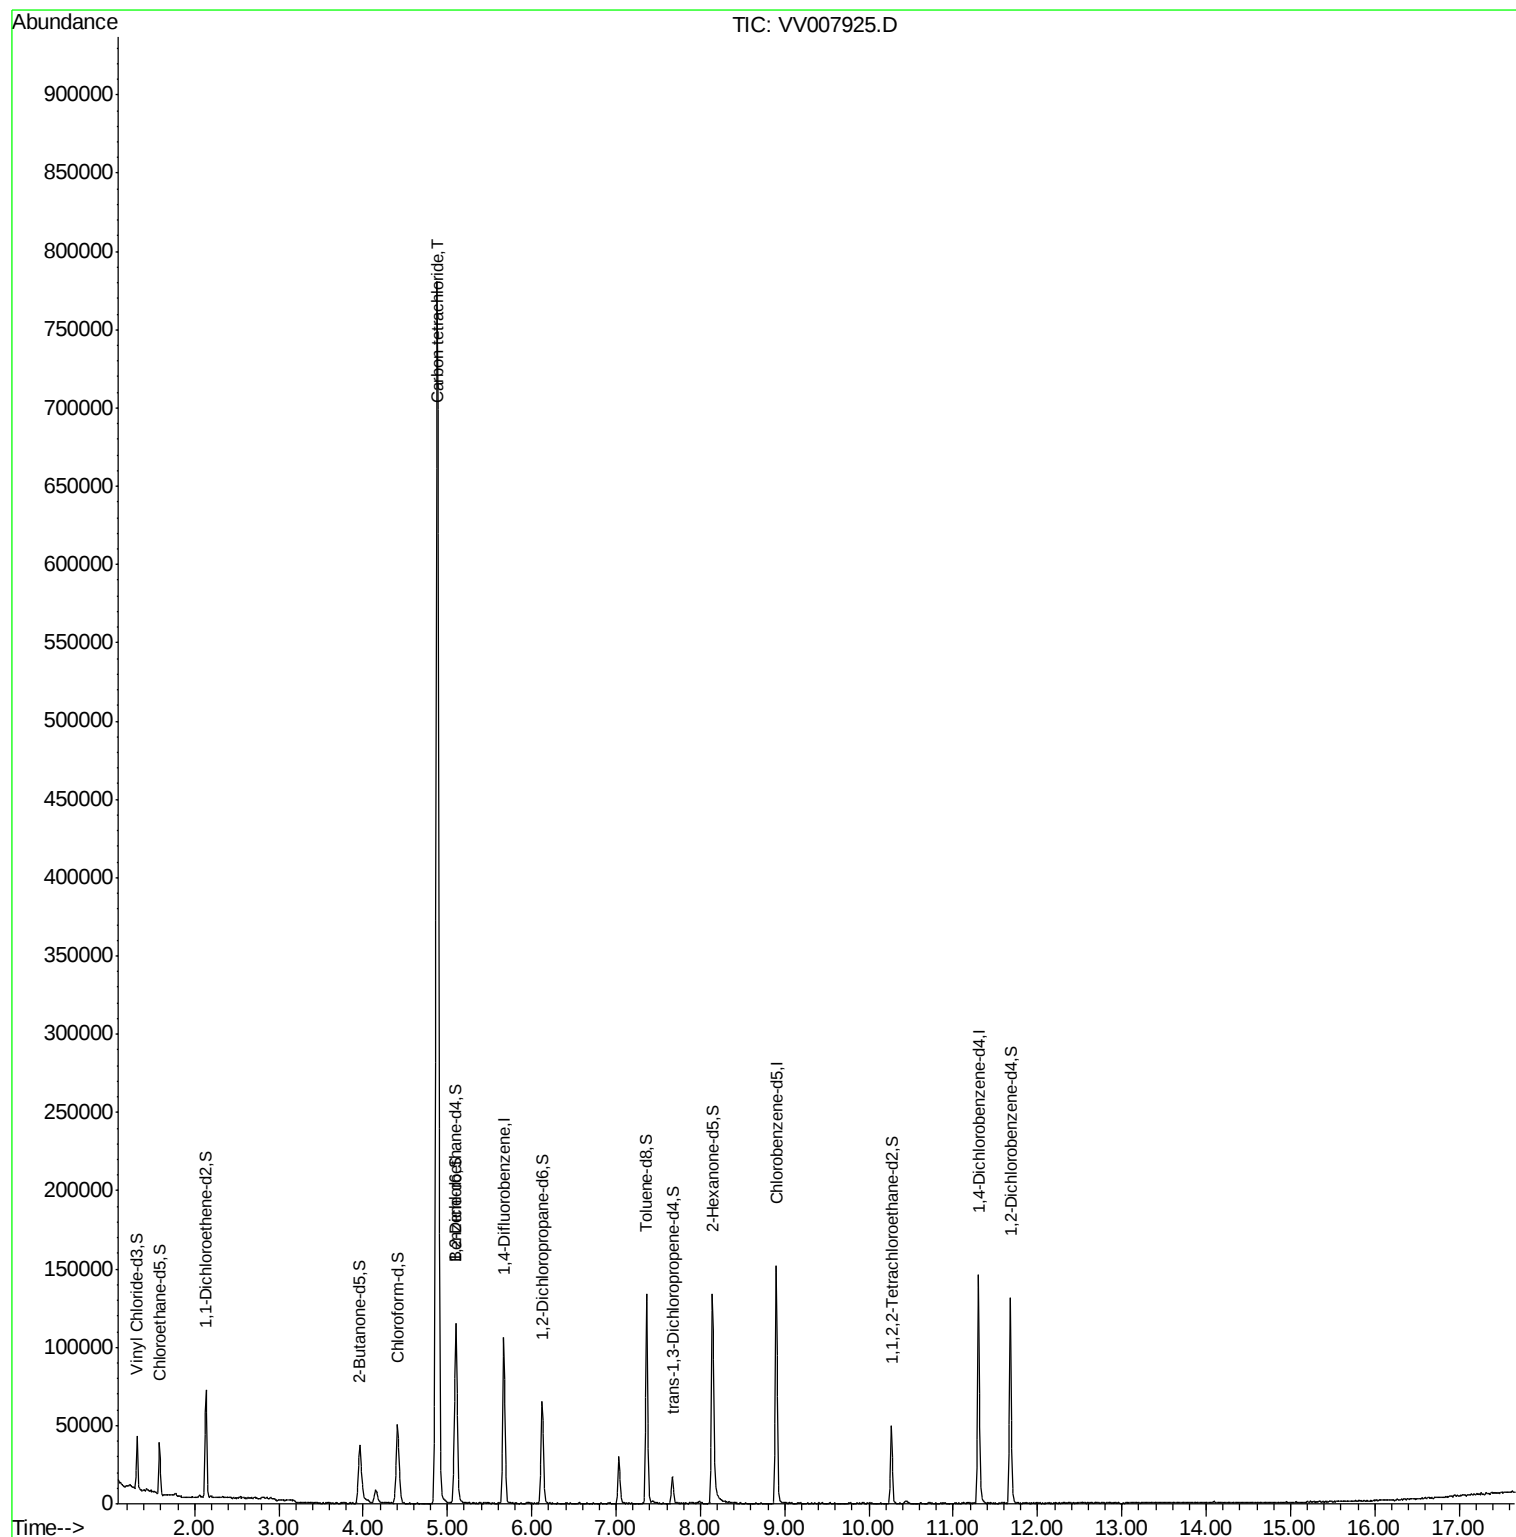

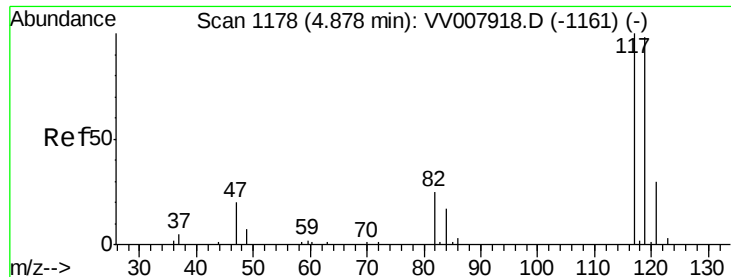

#31

Carbon tetrachloride

Concen: 64.400 ug/L

RT: 4.88 min Scan# 1179

Delta R.T. 0.00 min

Lab File: VV007925.D

Acq: 27 Sep 2018 23:29

Instrument :

MSVOA_V

ClientSampleId :

GAC33

Tot Ion:117 Resp: 570187

Ion Ratio Lower Upper

117 100

119 96.0 77.8 116.8

