

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092718\
 Data File : VV007929.D
 Acq On : 28 Sep 2018 01:18
 Operator : SY/MD
 Sample : J5063-16
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAC37

Quant Time: Sep 28 04:28:18 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 28 03:46:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	183105	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	173138	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	83746	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	20735	2.11	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	42.20%
7) Chloroethane-d5	1.59	69	19923	2.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	47.00%#
11) 1,1-Dichloroethene-d2	2.14	63	35153	1.59	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	31.80%#
20) 2-Butanone-d5	3.96	46	64652	21.90	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	43.80%
24) Chloroform-d	4.41	84	49580	2.22	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	44.40%#
26) 1,2-Dichloroethane-d4	5.09	65	26980	2.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	43.80%#
32) Benzene-d6	5.10	84	96344	2.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	46.60%#
36) 1,2-Dichloropropane-d6	6.13	67	30038	2.29	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	45.80%#
41) Toluene-d8	7.36	98	90178	2.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	42.80%#
43) trans-1,3-Dichloropropene-	7.67	79	9817	1.95	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	39.00%#
46) 2-Hexanone-d5	8.14	63	46334	20.80	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	41.60%#
57) 1,1,2,2-Tetrachloroethane-	10.27	84	22359	2.21	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	44.20%#
64) 1,2-Dichlorobenzene-d4	11.68	152	37973	2.34	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	46.80%#


Target Compounds					Ovalue
31) Carbon tetrachloride	4.88	117	261052	14.223 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092718\
Data File : VV007929.D
Acq On : 28 Sep 2018 01:18
Operator : SY/MD
Sample : J5063-16
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAC37

Quant Time: Sep 28 04:28:18 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 28 03:46:50 2018
Response via : Initial Calibration

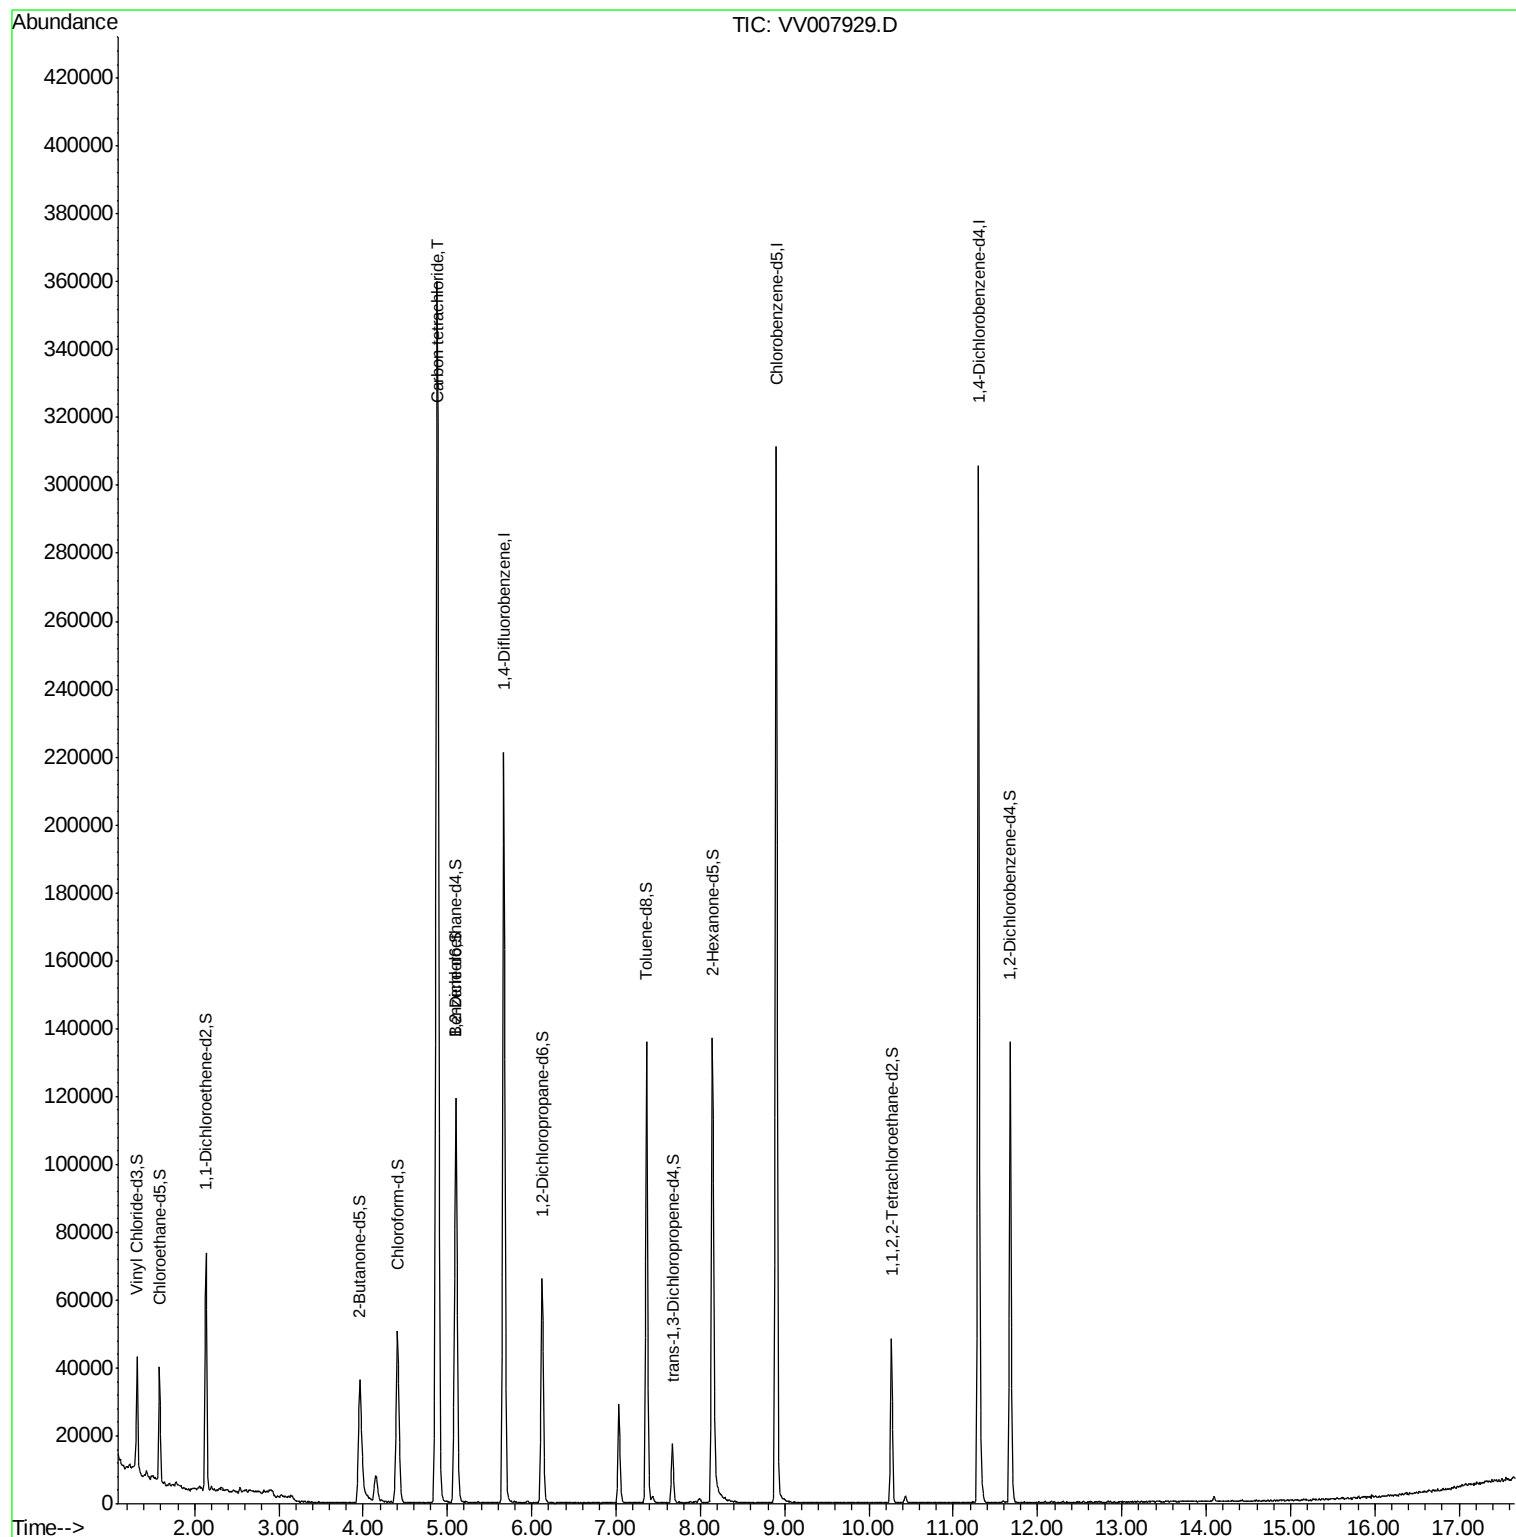

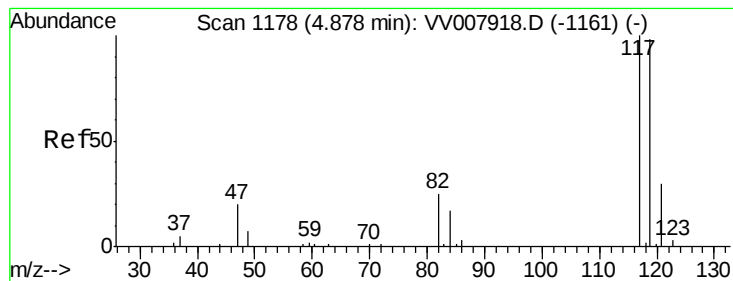

#31

Carbon tetrachloride

Concen: 14.223 ug/L

RT: 4.88 min Scan# 1179

Delta R.T. 0.00 min

Lab File: VV007929.D

Acq: 28 Sep 2018 01:18

Instrument :

MSVOA_V

ClientSampleId :

GAC37

Tot Ion:117 Resp: 261052

Ion Ratio Lower Upper

117 100

119 97.2 77.8 116.8

