

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092718\
 Data File : VV007936.D
 Acq On : 28 Sep 2018 04:30
 Operator : SY/MD
 Sample : J5062-06
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAC06

Quant Time: Sep 28 05:08:42 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 28 03:46:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	85730	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	84307	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	44151	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	20903	4.55	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.00%
7) Chloroethane-d5	1.58	69	18764	4.73	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.60%
11) 1,1-Dichloroethene-d2	2.13	63	34345	3.31	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.20%
20) 2-Butanone-d5	3.99	46	58238	42.13	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	84.26%
24) Chloroform-d	4.41	84	49685	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.00%
26) 1,2-Dichloroethane-d4	5.09	65	27007	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.80%
32) Benzene-d6	5.10	84	94491	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.00%
36) 1,2-Dichloropropane-d6	6.12	67	29766	4.66	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.20%
41) Toluene-d8	7.36	98	91892	4.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.60%
43) trans-1,3-Dichloropropene-	7.67	79	10185	4.15	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.00%
46) 2-Hexanone-d5	8.14	63	56378	51.99	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.98%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	22718	4.61	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	41092	4.81	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.20%


Target Compounds				Ovalue
15) Methyl Acetate	2.48	43	4560	1.770 ug/L # 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092718\
Data File : VV007936.D
Acq On : 28 Sep 2018 04:30
Operator : SY/MD
Sample : J5062-06
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAC06

Quant Time: Sep 28 05:08:42 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 28 03:46:50 2018
Response via : Initial Calibration

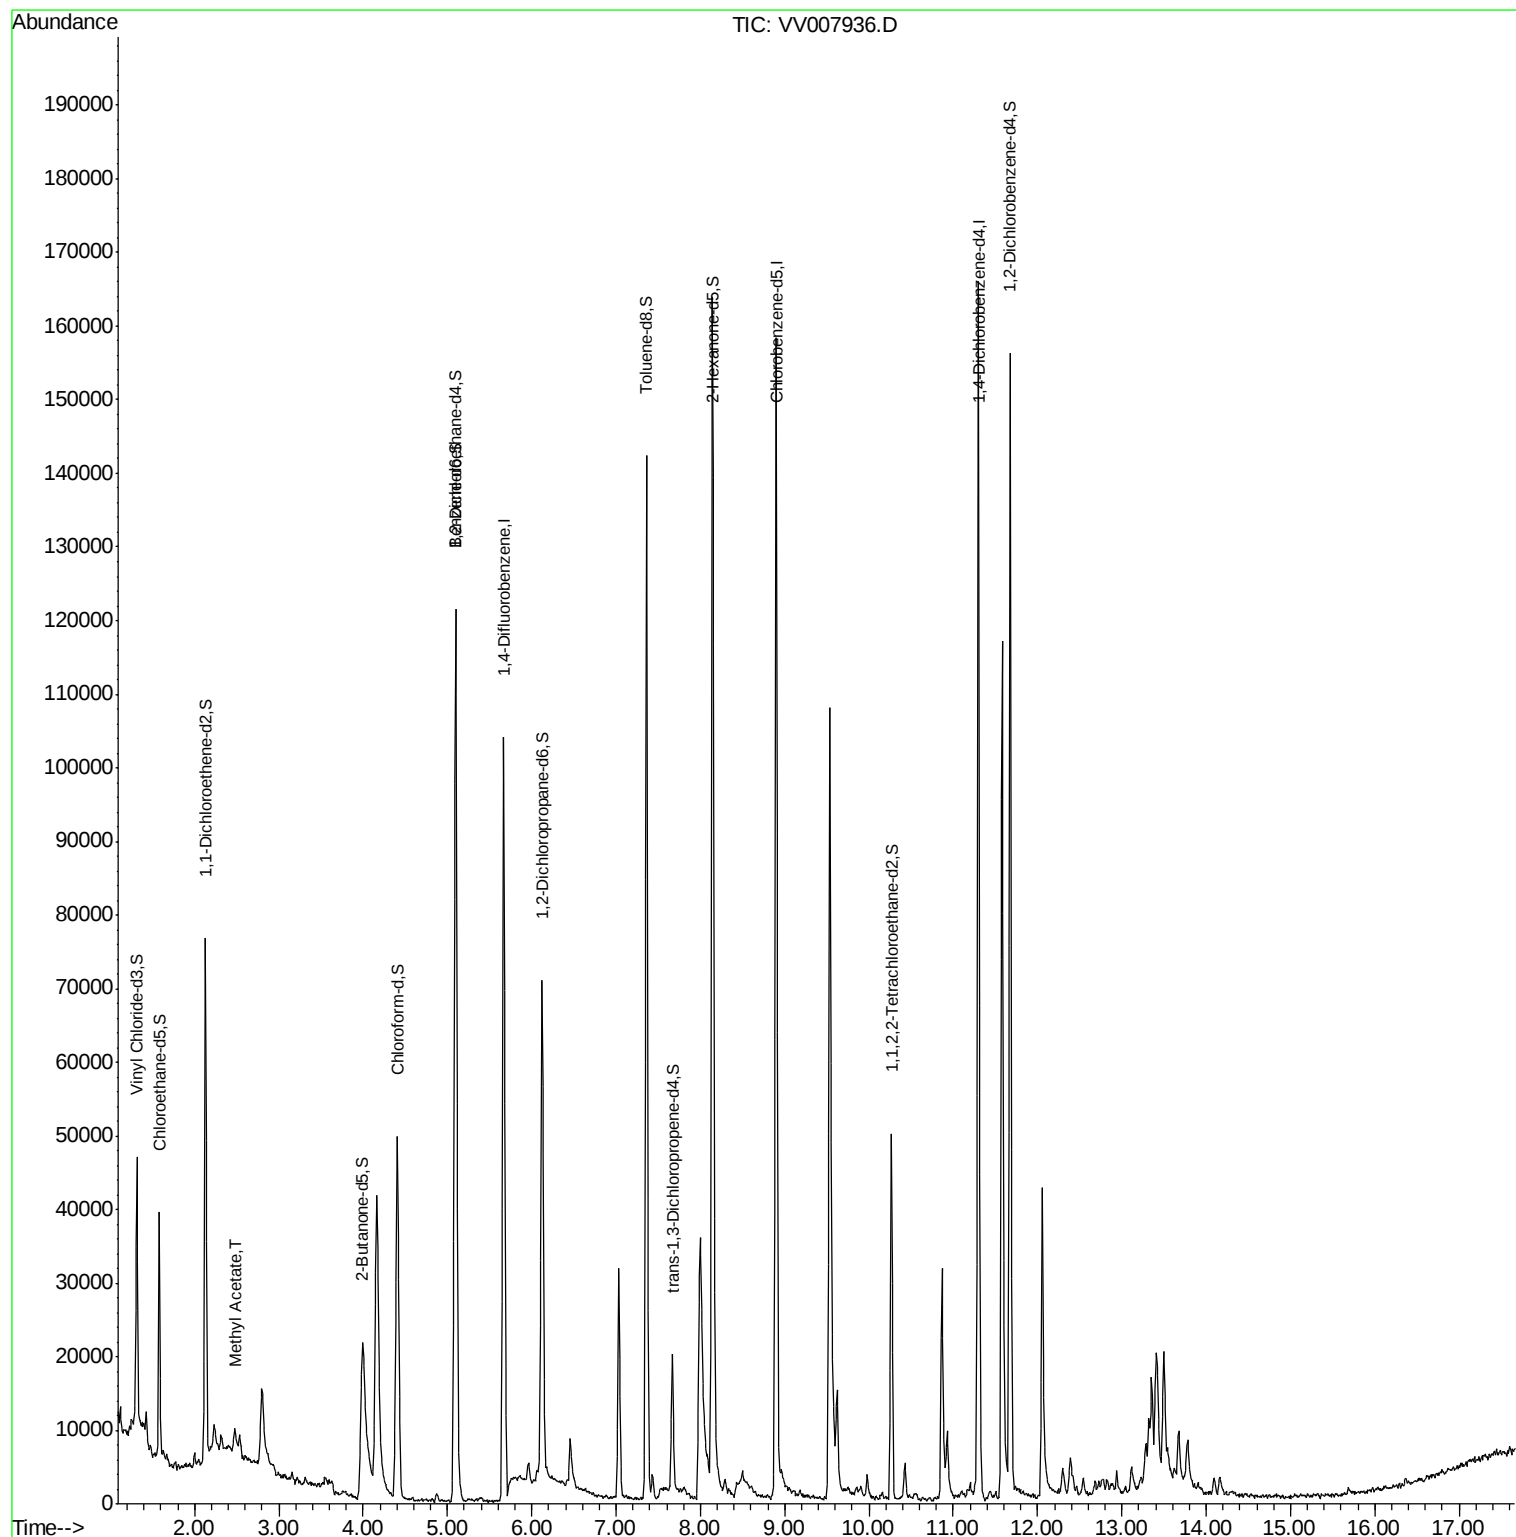

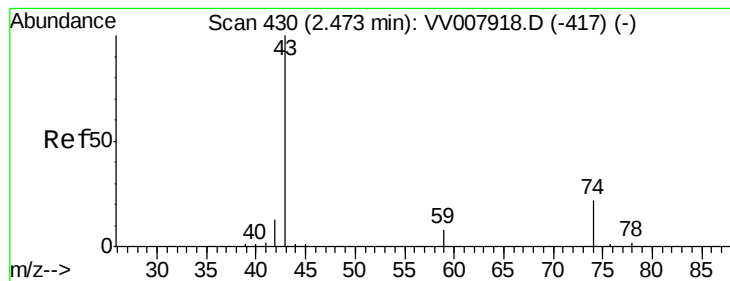

#15
Methyl Acetate
Concen: 1.770 ug/L
RT: 2.48 min Scan# 433
Delta R.T. 0.01 min
Lab File: VV007936.D
Acq: 28 Sep 2018 04:30

Instrument :
MSVOA_V
ClientSampleId :
GAC06

Tot Ion: 43 Resp: 4560
Ion Ratio Lower Upper
43 100
74 30.0 19.5 29.3#

