


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV092718\
Data File : VV007889.D
Acq On : 26 Sep 2018 17:46
Operator : SY/MD
Sample : BFB75
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB75

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Sep 28 03:46:50 2018

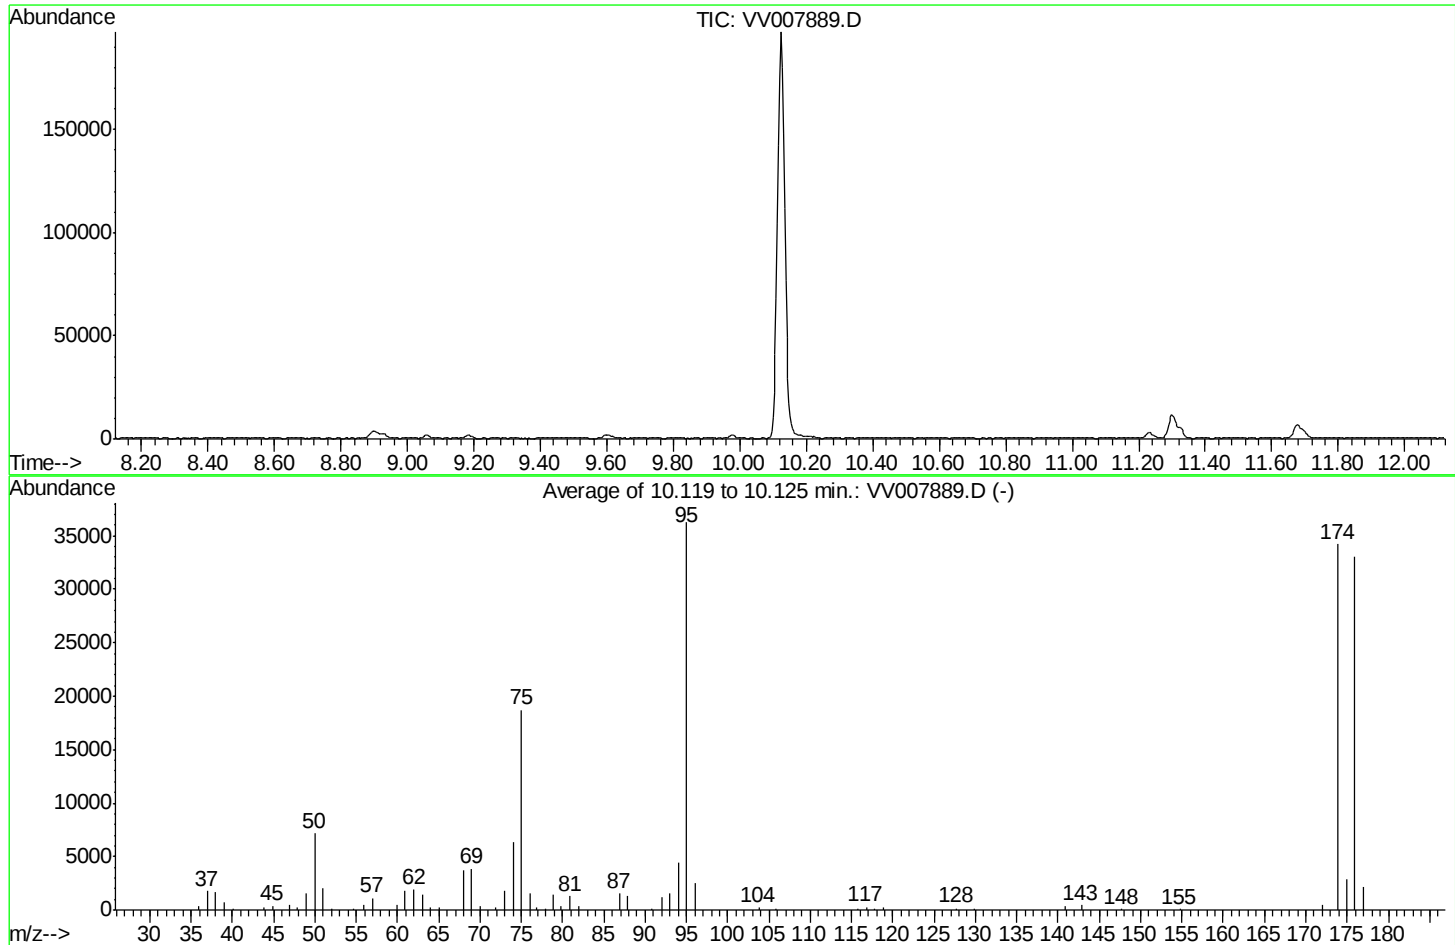

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	7142	PASS
75	95	30	80	51.7	18736	PASS
95	95	100	100	100.0	36266	PASS
96	95	5	9	6.9	2514	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	94.3	34210	PASS
175	174	5	9	8.3	2827	PASS
176	174	95	101	96.5	33000	PASS
177	176	5	9	6.5	2133	PASS

m/z	Abundance
43.90	316.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
35.90	419.0
37.00	1655.0
38.00	1635.0
39.00	655.0
40.00	162.0
43.90	510.0
44.90	323.0
46.90	477.0
47.80	266.0
49.00	1432.0
50.00	6716.0
51.00	1947.0
54.70	107.0
55.90	501.0
56.90	1107.0
60.00	381.0
61.00	1637.0
62.00	1702.0
63.00	1446.0
63.90	186.0
65.10	259.0
68.00	3352.0
69.00	3766.0
70.00	336.0
71.90	268.0
72.90	1609.0
74.00	5761.0
75.00	17488.0
76.00	1441.0
76.90	189.0
77.90	103.0
78.90	1399.0
79.80	309.0
80.90	1246.0
81.90	334.0
86.90	1337.0
87.90	1350.0
90.80	170.0
92.00	1029.0
93.00	1498.0
94.00	4139.0
95.00	34272.0
96.00	2414.0
103.80	201.0
105.90	150.0
115.80	143.0
116.80	291.0
117.70	139.0
118.80	204.0
127.70	135.0
140.80	349.0
142.80	471.0
147.70	105.0
171.90	378.0
173.90	30808.0
174.90	2627.0
175.90	29904.0
176.90	1960.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
35.90	416.0
37.00	1843.0
38.00	1686.0
39.00	769.0
40.00	145.0
43.90	509.0
44.90	404.0
46.80	442.0
47.80	283.0
49.00	1585.0
50.00	7410.0
51.00	2132.0
52.10	107.0
54.70	118.0
55.90	505.0
57.00	1166.0
60.00	443.0
60.90	1926.0
62.00	1994.0
63.00	1527.0
63.90	216.0
65.00	277.0
68.00	3877.0
69.00	3987.0
69.90	330.0
71.90	294.0
72.90	1803.0
74.00	6578.0
75.00	19320.0
76.00	1594.0
76.90	217.0
77.80	124.0
78.90	1532.0
79.90	354.0
80.90	1333.0
81.90	369.0
86.90	1554.0
87.90	1422.0
90.80	171.0
92.00	1221.0
93.00	1628.0
94.00	4548.0
95.00	37552.0
96.00	2587.0
103.80	187.0
105.90	150.0
115.80	169.0
116.80	311.0
117.80	164.0
118.80	238.0
127.70	155.0
129.80	117.0
140.90	375.0
142.90	475.0
147.80	116.0
154.80	110.0
171.90	450.0
173.90	35280.0
174.90	2935.0
175.90	34104.0
176.90	2202.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
35.90	393.0
37.00	1799.0
38.00	1571.0
39.00	791.0
40.10	142.0
43.90	515.0
44.90	452.0
46.80	383.0
47.80	258.0
49.00	1652.0
50.00	7301.0
51.00	2046.0
52.10	101.0
54.70	127.0
55.90	499.0
57.00	1101.0
60.00	469.0
60.90	1985.0
62.00	1984.0
63.00	1440.0
64.00	216.0
65.00	262.0
68.00	4035.0
69.00	3862.0
69.90	297.0
71.90	271.0
72.90	1873.0
74.00	6785.0
75.00	19400.0
76.00	1610.0
76.90	236.0
77.80	134.0
78.90	1452.0
79.90	359.0
80.90	1339.0
81.90	380.0
86.90	1631.0
87.90	1365.0
90.80	161.0
92.00	1253.0
92.90	1613.0
94.00	4602.0
95.00	36976.0
96.00	2541.0
103.80	175.0
105.80	143.0
115.80	185.0
116.80	297.0
117.80	171.0
118.80	255.0
127.70	149.0
129.80	124.0
140.90	401.0
142.90	456.0
147.80	106.0
154.80	108.0
172.00	456.0
173.90	36544.0
174.90	2919.0
175.90	34992.0
176.90	2238.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75