

Data File : VV013005.D
Acq On : 27 Sep 2019 11:25
Operator : SY/MD
Sample : K4988-13
Misc : 5.10G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Sep 27 22:53:46 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 27 22:50:49 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	786164	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	773349	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	376704	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	256357	21.02	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.08%
7) Chloroethane-d5	1.58	69	223414	22.65	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.60%
10) 1,1-Dichloroethene-d2	2.13	63	342226	16.87	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.48%
20) 2-Butanone-d5	3.95	46	157760	37.46	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.92%
24) Chloroform-d	4.40	84	473578	21.93	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.72%
26) 1,2-Dichloroethane-d4	5.08	65	271922	21.66	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.64%
29) Benzene-d6	5.10	84	985264	22.82	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.28%
33) 1,2-Dichloropropane-d6	6.12	67	311103	22.99	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.96%
37) Toluene-d8	7.36	98	888027	22.66	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.64%
38) trans-1,3-Dichloropropene-	7.66	79	118464	20.67	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.68%
39) 2-Hexanone-d5	8.14	63	106014	38.93	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.86%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	254031	19.76	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	79.04%
61) 1,2-Dichlorobenzene-d4	11.67	152	349302	23.87	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.48%


Target Compounds					Qvalue
13) Acetone	2.21	43	5779	1.291 ug/L	85
16) Methylene chloride	2.54	84	18995	1.616 ug/L	96
59) 1,2,3-Trichloropropane	11.29	75	44230	4.558 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV013005.D
Acq On : 27 Sep 2019 11:25
Operator : SY/MD
Sample : K4988-13
Misc : 5.10G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Sep 27 22:53:46 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 27 22:50:49 2019
Response via : Initial Calibration

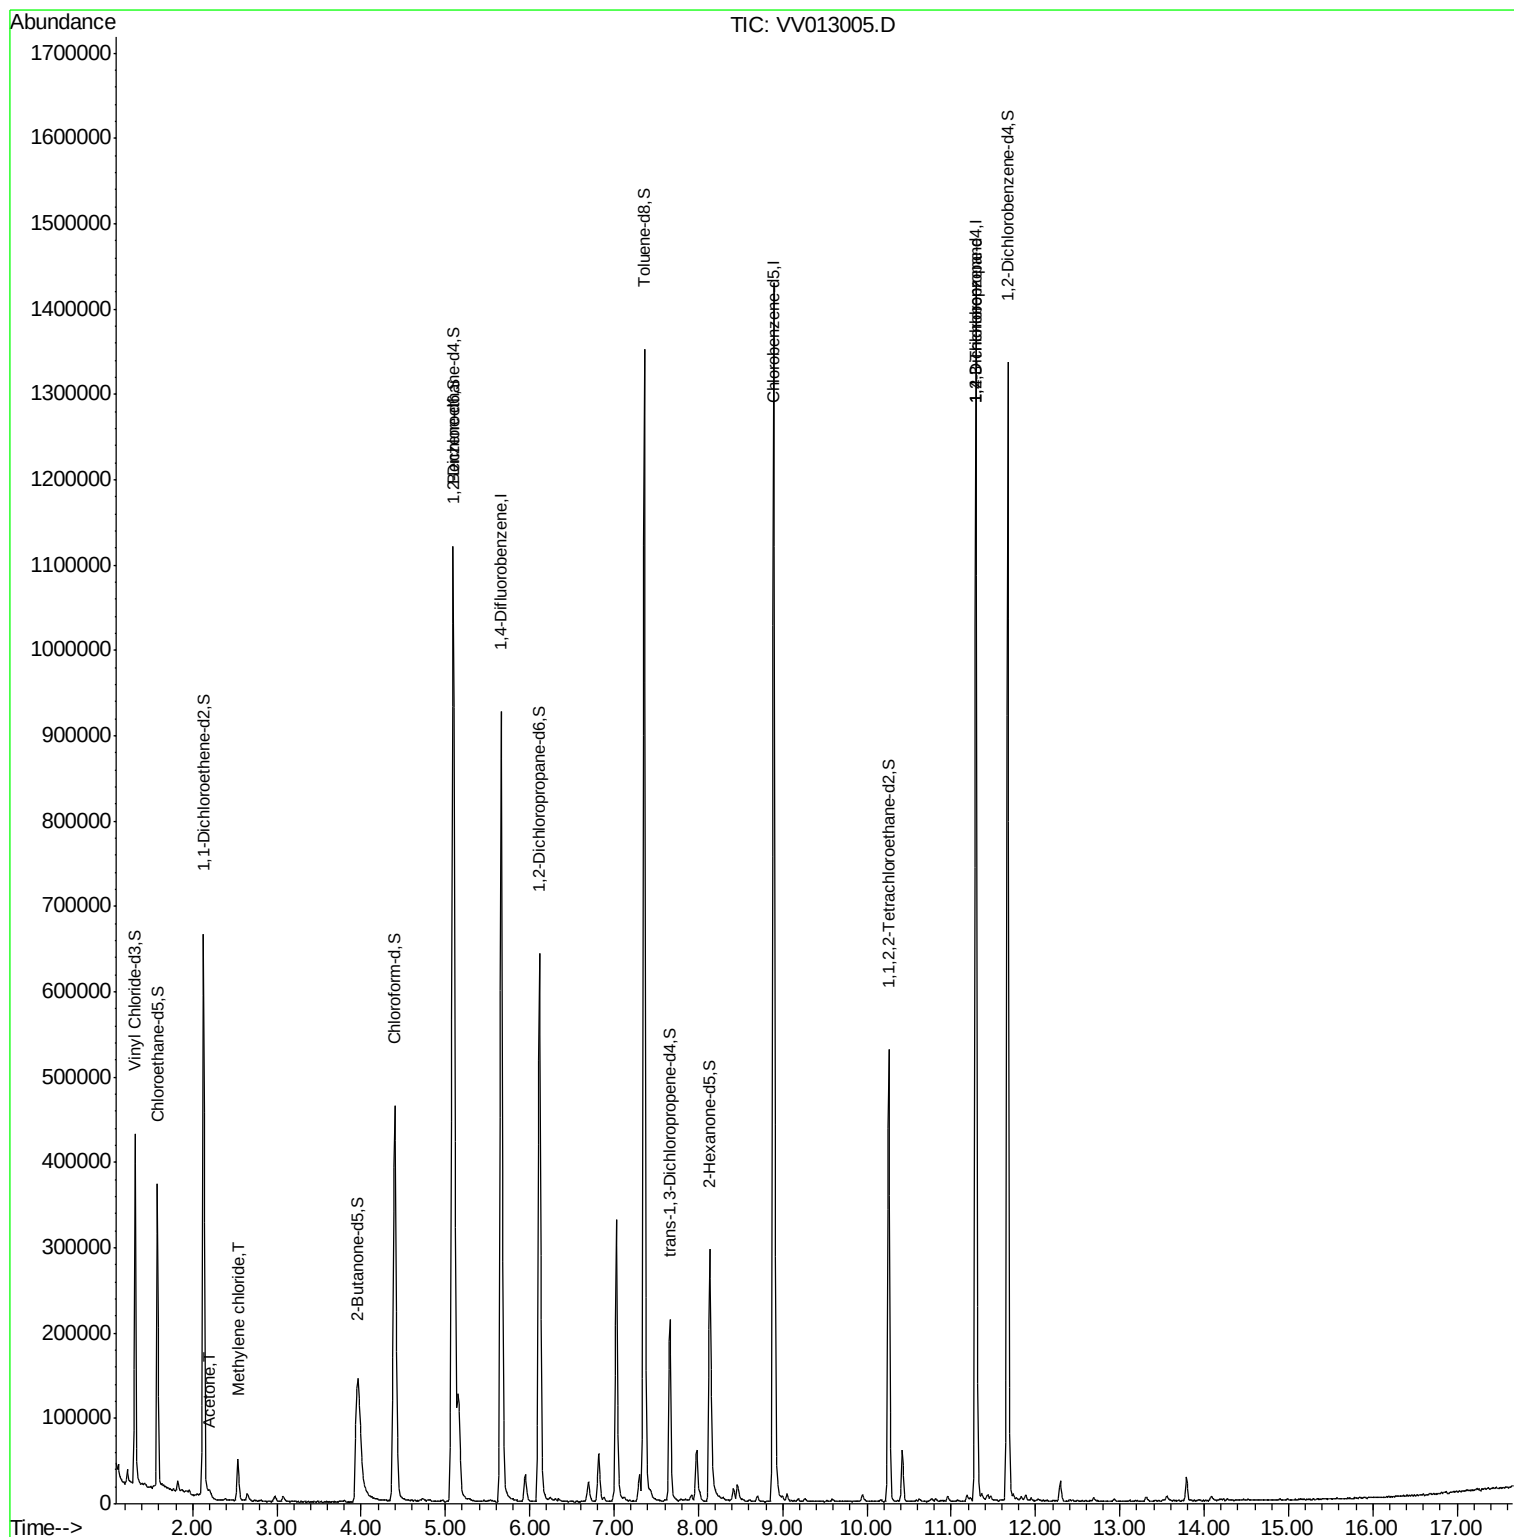

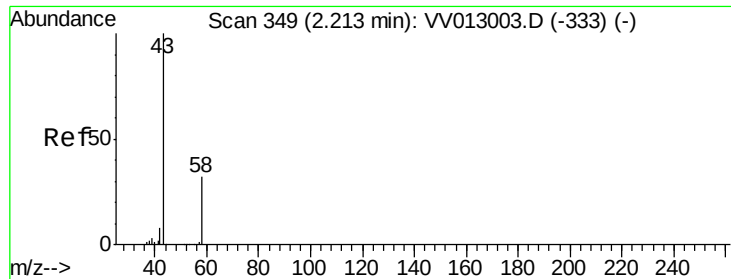

#13

Acetone

Concen: 1.291 ug/L

RT: 2.21 min Scan# 347

Delta R.T. -0.01 min

Lab File: VV013005.D

Acq: 27 Sep 2019 11:25

Instrument :

MSVOA_V

ClientSampleId :





VHBLK01

Tgt Ion: 43 Resp: 5779

Ion Ratio Lower Upper

43 100

58 40.9 0.0 65.0

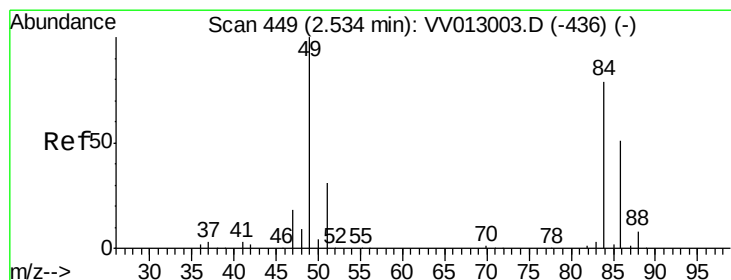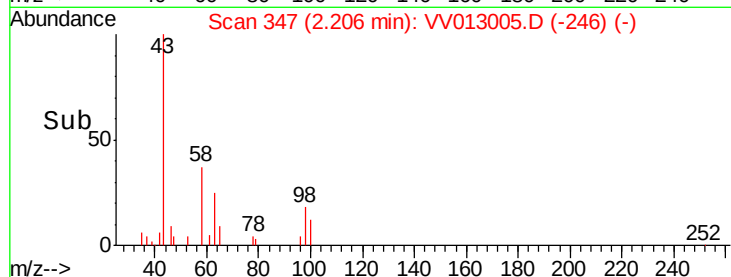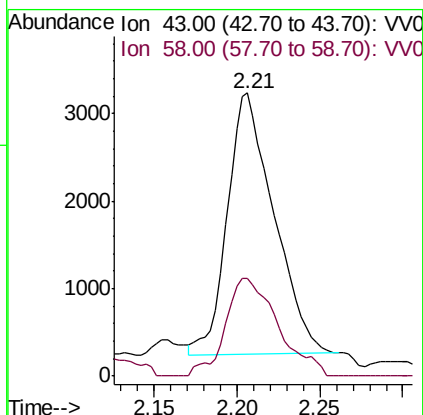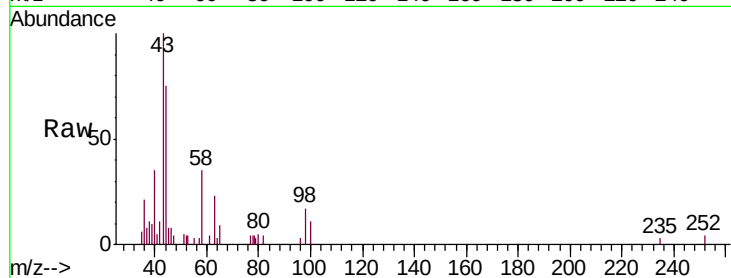

#16

Methylene chloride

Concen: 1.616 ug/L

RT: 2.54 min Scan# 450

Delta R.T. 0.00 min

Lab File: VV013005.D

Acq: 27 Sep 2019 11:25




Tgt Ion: 84 Resp: 18995


Ion Ratio Lower Upper

84 100

49 128.7 88.3 164.1

86 69.6 44.9 83.3

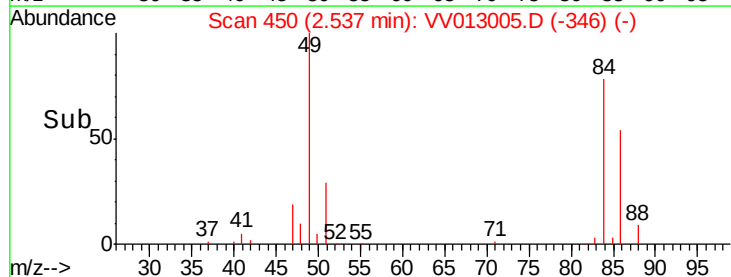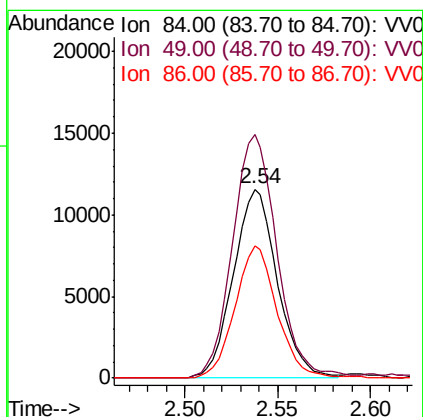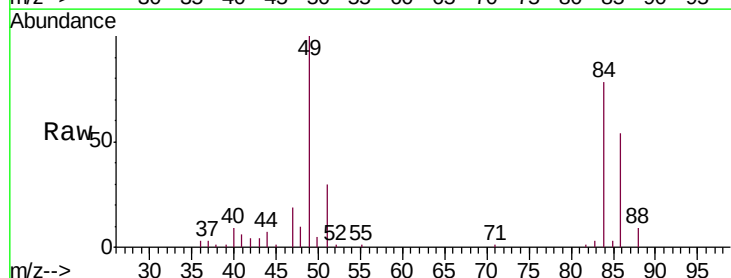

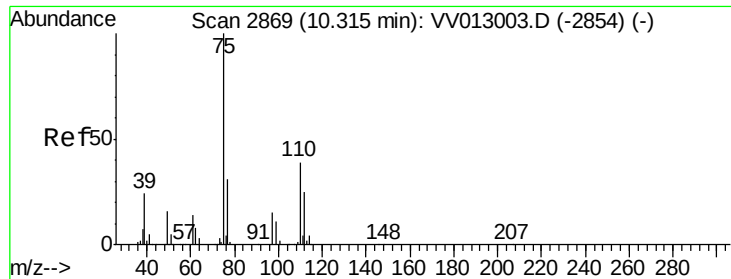

#59
 1,2,3-Trichloropropane
 Concen: 4.558 ug/L
 RT: 11.29 min Scan# 3172
 Delta R.T. 0.97 min
 Lab File: VV013005.D
 Acq: 27 Sep 2019 11:25

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Tgt Ion: 75 Resp: 44230
 Ion Ratio Lower Upper
 75 100
 77 35.7 25.4 38.0

