

Data File : VV013007.D
Acq On : 27 Sep 2019 12:20
Operator : SY/MD
Sample : K4984-12
Misc : 5.04G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Time: Sep 27 22:54:02 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 27 22:50:49 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	655974	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	665148	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	317745	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	216541	21.27	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.08%
7) Chloroethane-d5	1.58	69	186608	22.68	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.72%
10) 1,1-Dichloroethene-d2	2.13	63	292778	17.30	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.20%
20) 2-Butanone-d5	3.94	46	167840	47.76	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.52%
24) Chloroform-d	4.40	84	419669	23.29	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.16%
26) 1,2-Dichloroethane-d4	5.08	65	251682	24.03	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.12%
29) Benzene-d6	5.10	84	860599	23.17	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.68%
33) 1,2-Dichloropropane-d6	6.12	67	279318	24.00	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.00%
37) Toluene-d8	7.36	98	762154	22.61	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.44%
38) trans-1,3-Dichloropropene-	7.66	79	109041	22.12	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.48%
39) 2-Hexanone-d5	8.13	63	106348	45.40	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.80%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	244862	22.15	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.60%
61) 1,2-Dichlorobenzene-d4	11.67	152	316424	25.63	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.52%


Target Compounds					Qvalue
13) Acetone	2.21	43	5714	1.530 ug/L	95
16) Methylene chloride	2.54	84	20662	2.107 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV013007.D
Acq On : 27 Sep 2019 12:20
Operator : SY/MD
Sample : K4984-12
Misc : 5.04G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Time: Sep 27 22:54:02 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 27 22:50:49 2019
Response via : Initial Calibration

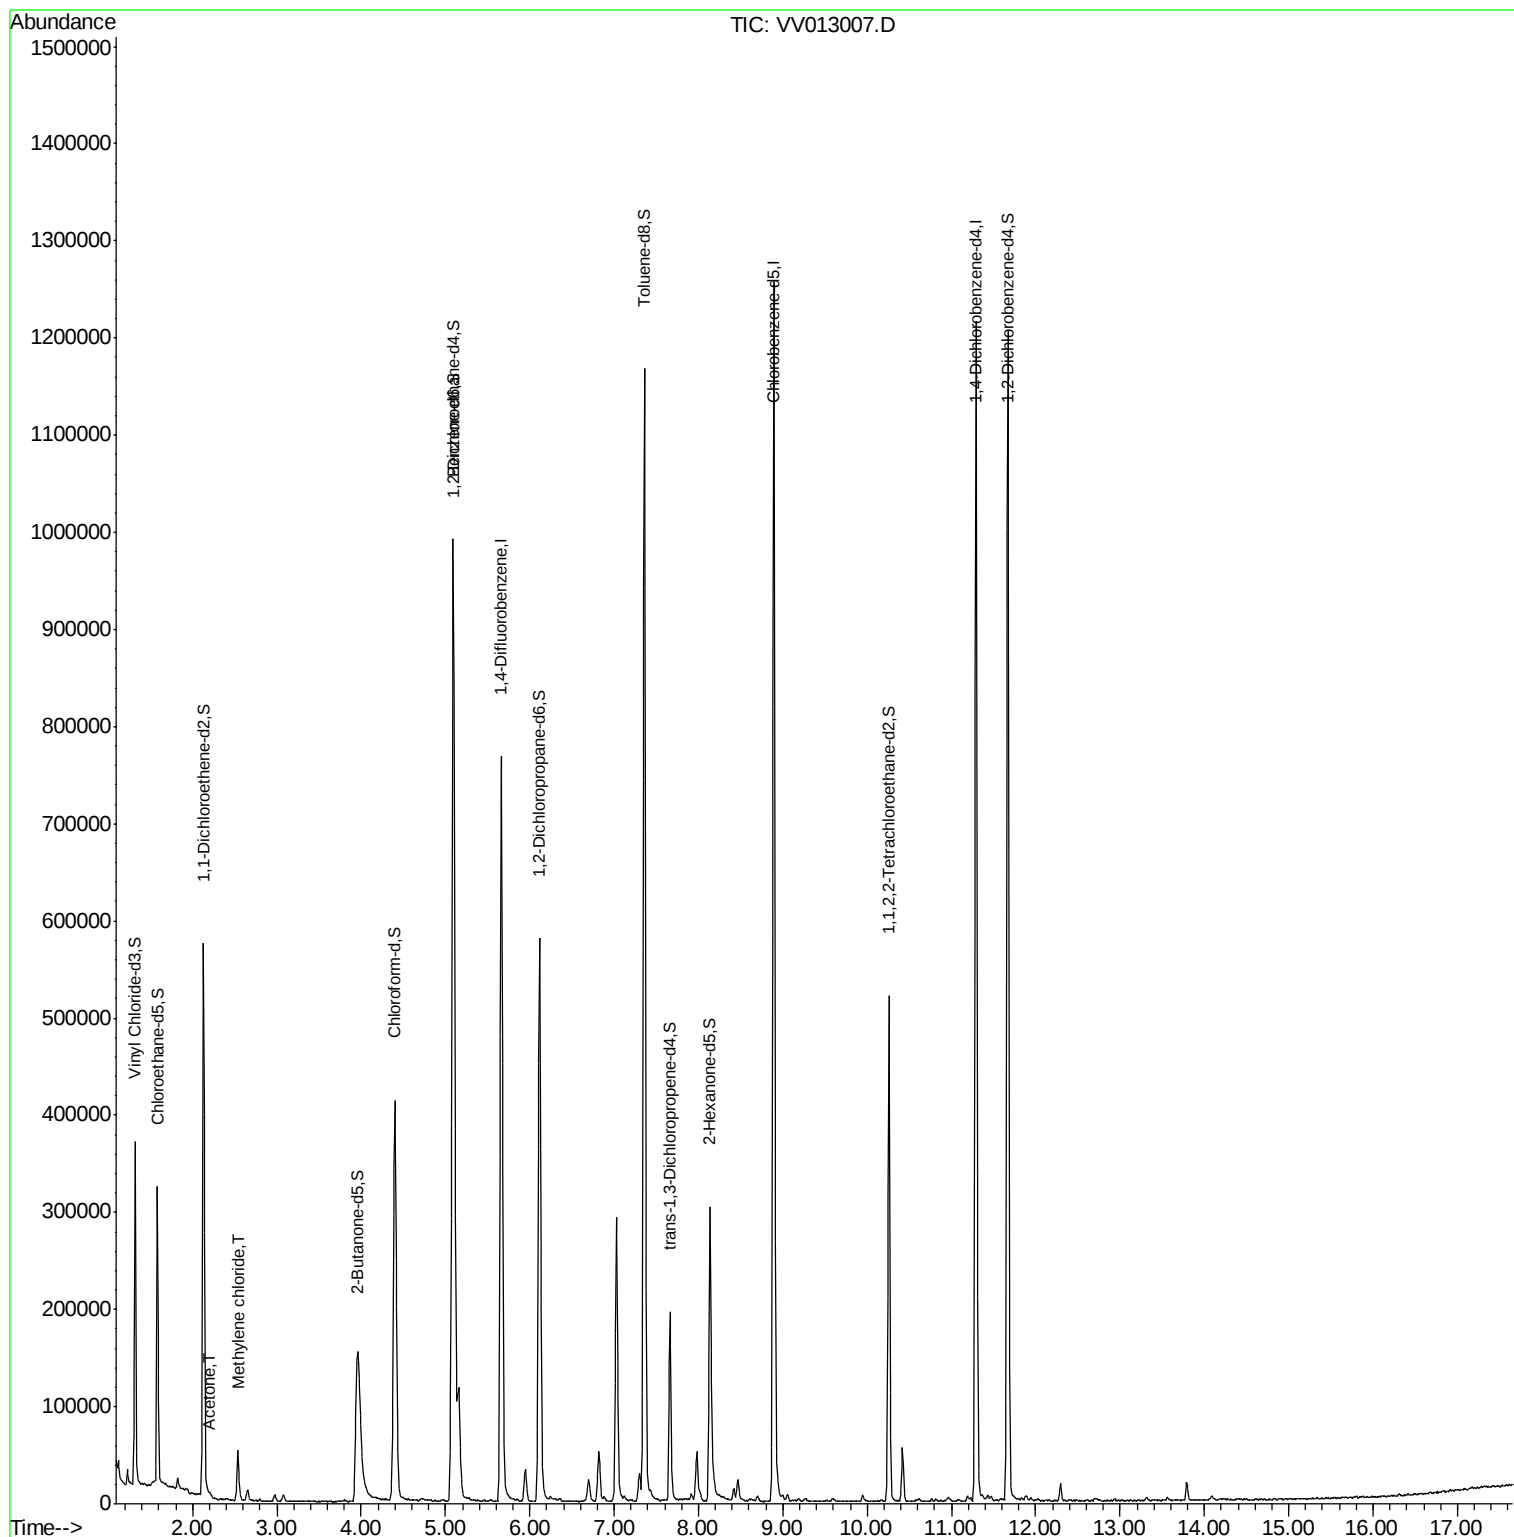

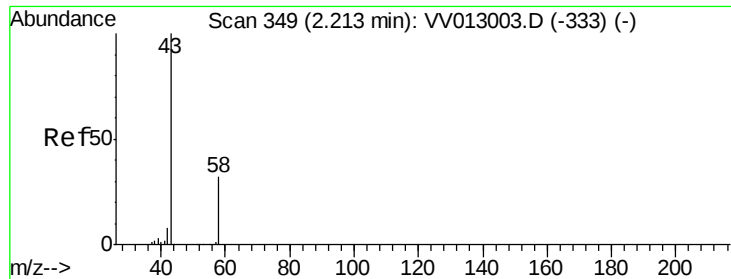

#13

Acetone

Concen: 1.530 ug/L

RT: 2.21 min Scan# 347

Delta R.T. -0.01 min

Lab File: VV013007.D

Acq: 27 Sep 2019 12:20

Instrument :

MSVOA_V

ClientSampleId :


VHBLK02

Tgt Ion: 43 Resp: 5714

Ion Ratio Lower Upper




43 100

58 29.6 0.0 65.0

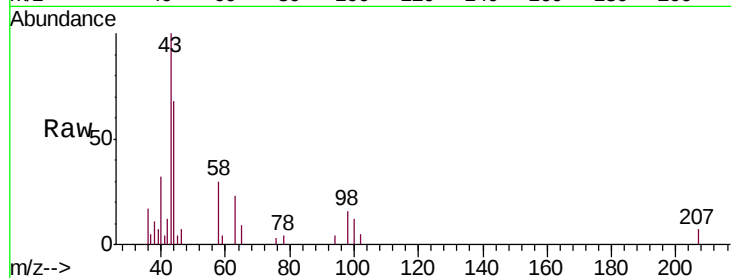

Abundance Ion 43.00 (42.70 to 43.70): VV0

Ion 58.00 (57.70 to 58.70): VV0

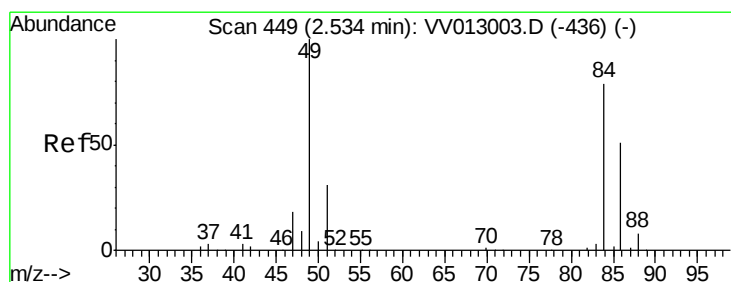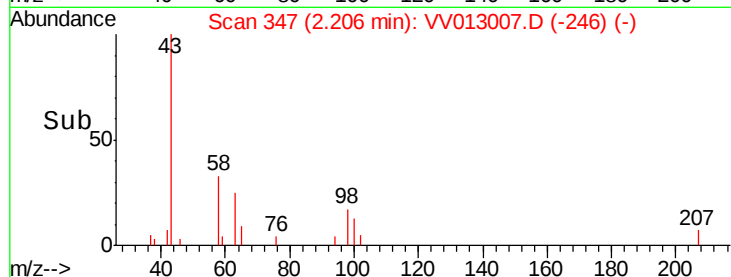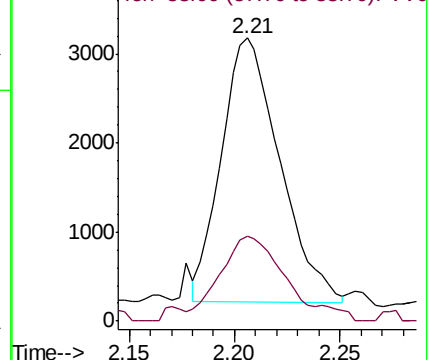

#16

Methylene chloride

Concen: 2.107 ug/L

RT: 2.54 min Scan# 451

Delta R.T. 0.01 min

Lab File: VV013007.D

Acq: 27 Sep 2019 12:20


Tgt Ion: 84 Resp: 20662

Ion Ratio Lower Upper

84 100

49 127.9 88.3 164.1

86 59.2 44.9 83.3

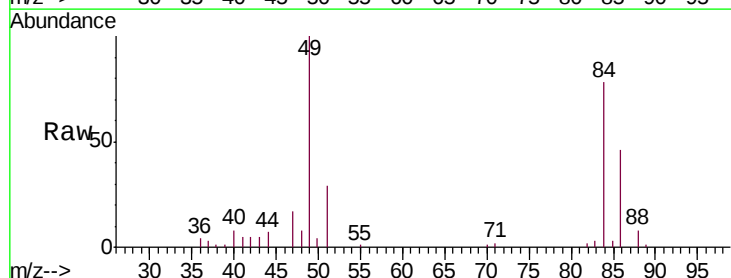

Abundance Ion 84.00 (83.70 to 84.70): VV0

Ion 49.00 (48.70 to 49.70): VV0

Ion 86.00 (85.70 to 86.70): VV0

