

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV092721\  
 Data File : VV022328.D  
 Acq On : 27 Sep 2021 10:45  
 Operator : SY/MD  
 Sample : VV0927WBL01  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 VBLK212

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR092321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022328.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.301       | 75            | 81          | 91           | rVB      | 38595          | 39923         | 7.81%           | 1.119%        |
| 2         | 1.564       | 155           | 163         | 176          | rBV      | 50919          | 62217         | 12.16%          | 1.745%        |
| 3         | 2.105       | 320           | 331         | 344          | rBV      | 89174          | 127707        | 24.97%          | 3.581%        |
| 4         | 2.503       | 446           | 455         | 469          | rVB      | 5347           | 9531          | 1.86%           | 0.267%        |
| 5         | 3.915       | 883           | 894         | 952          | rBV2     | 38880          | 205577        | 40.19%          | 5.764%        |
| 6         | 4.349       | 1013          | 1029        | 1051         | rBV      | 76169          | 190499        | 37.24%          | 5.342%        |
| 7         | 5.050       | 1231          | 1247        | 1276         | rBV2     | 167763         | 423849        | 82.87%          | 11.885%       |
| 8         | 5.619       | 1408          | 1424        | 1456         | rBV      | 131024         | 275586        | 53.88%          | 7.727%        |
| 9         | 5.908       | 1506          | 1514        | 1525         | rBV8     | 3407           | 6820          | 1.33%           | 0.191%        |
| 10        | 6.072       | 1552          | 1565        | 1598         | rBV2     | 101516         | 210294        | 41.11%          | 5.897%        |
| 11        | 6.992       | 1841          | 1851        | 1870         | rBV      | 35447          | 68882         | 13.47%          | 1.931%        |
| 12        | 7.317       | 1940          | 1952        | 1970         | rBV      | 174424         | 315046        | 61.59%          | 8.834%        |
| 13        | 7.628       | 2037          | 2049        | 2062         | rBV2     | 21350          | 39423         | 7.71%           | 1.105%        |
| 14        | 8.095       | 2183          | 2194        | 2225         | rBV      | 257684         | 511491        | 100.00%         | 14.342%       |
| 15        | 8.853       | 2419          | 2430        | 2451         | rBV      | 205179         | 340888        | 66.65%          | 9.558%        |
| 16        | 10.220      | 2844          | 2855        | 2874         | rVB2     | 83001          | 134007        | 26.20%          | 3.757%        |
| 17        | 11.252      | 3163          | 3176        | 3195         | rBV      | 196872         | 310512        | 60.71%          | 8.707%        |
| 18        | 11.625      | 3279          | 3292        | 3311         | rBV      | 185061         | 294141        | 57.51%          | 8.248%        |




Sum of corrected areas: 3566393

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV092721\  
Data File : VV022328.D  
Acq On : 27 Sep 2021 10:45  
Operator : SY/MD  
Sample : VV0927WBL01  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
VBLK212

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR092321WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

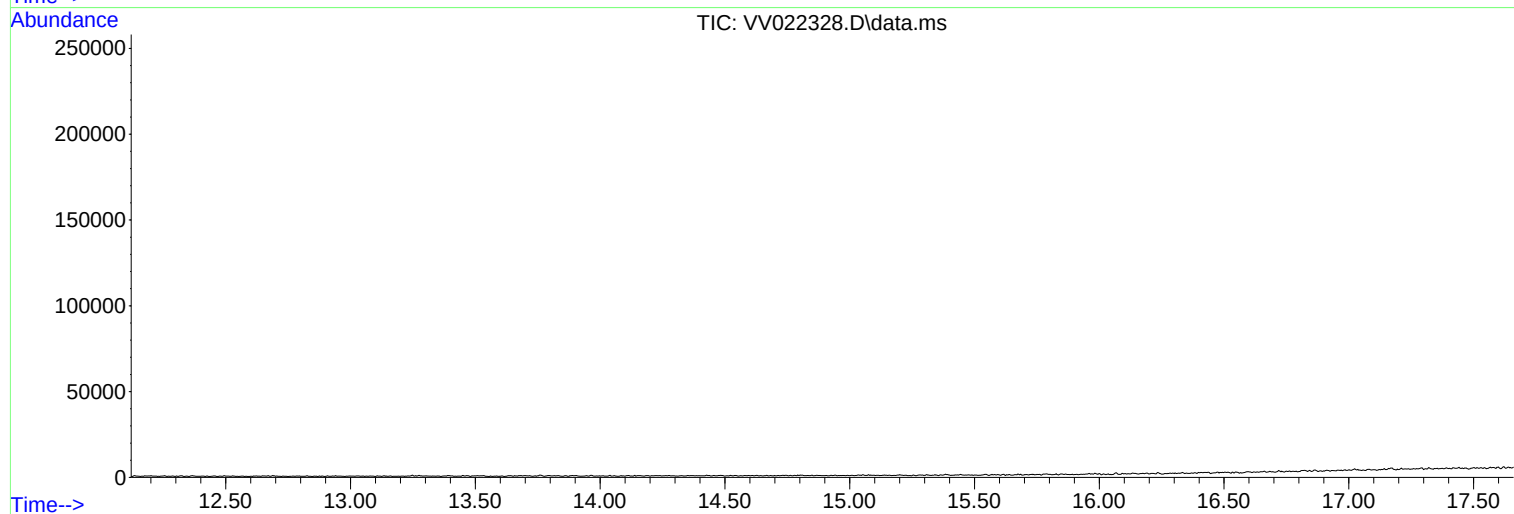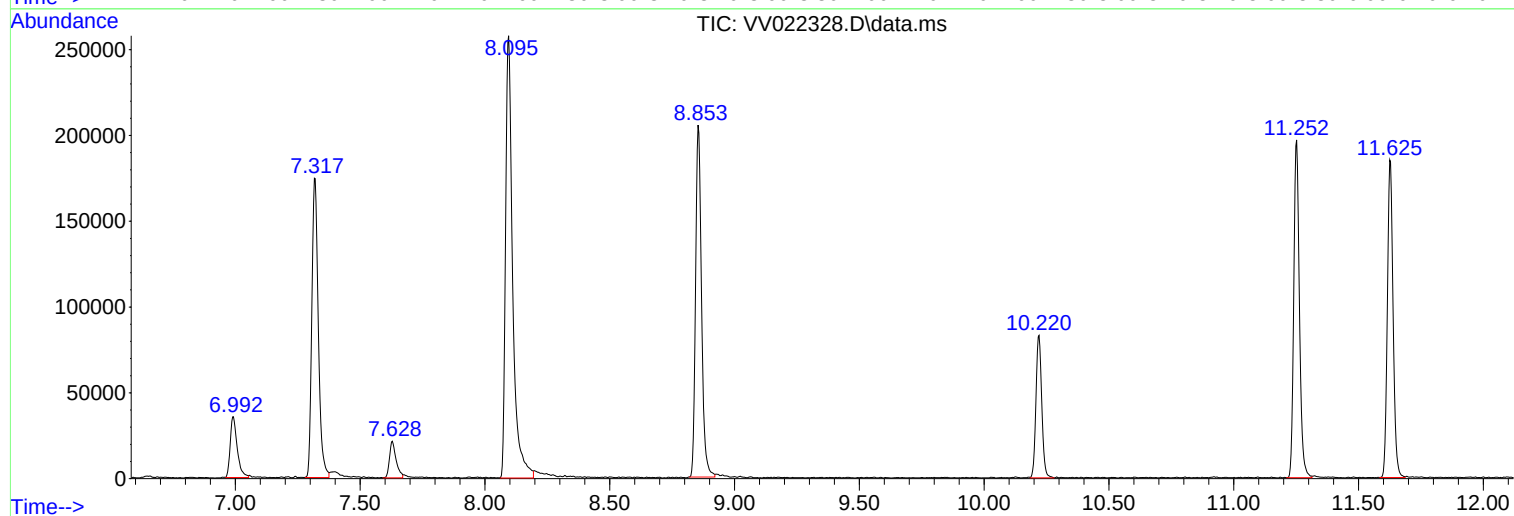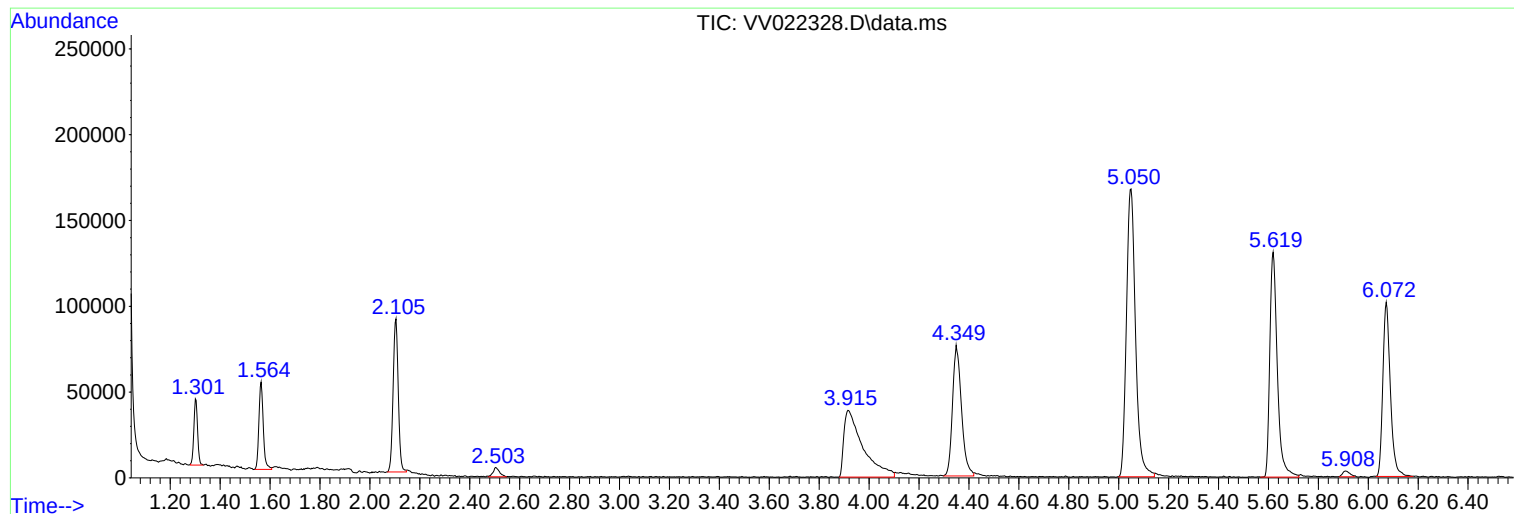

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV092721\  
Data File : VV022328.D  
Acq On : 27 Sep 2021 10:45  
Operator : SY/MD  
Sample : VV0927WBL01  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
VBLK212

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR092321WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV092721\  
Data File : VV022328.D  
Acq On : 27 Sep 2021 10:45  
Operator : SY/MD  
Sample : VV0927WBL01  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
VBLK212

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR092321WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----