

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092721\
 Data File : VV022330.D
 Acq On : 27 Sep 2021 11:55
 Operator : SY/MD
 Sample : M3834-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW415

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022330.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	92	rVB	41167	42040	9.46%	1.136%
2	1.564	156	163	172	rBV	53048	63373	14.27%	1.712%
3	2.108	320	332	343	rBV	87506	129196	29.09%	3.490%
4	2.294	380	390	400	rBV	13700	21980	4.95%	0.594%
5	3.883	873	884	915	rBV2	63204	182089	41.00%	4.919%
6	4.352	1015	1030	1053	rBV2	80893	204944	46.14%	5.537%
7	5.050	1231	1247	1277	rBV2	173179	435794	98.11%	11.774%
8	5.619	1411	1424	1451	rBV	146477	310034	69.80%	8.376%
9	5.908	1504	1514	1516	rBV3	5038	6584	1.48%	0.178%
10	6.072	1551	1565	1593	rBV	107078	222414	50.07%	6.009%
11	6.992	1840	1851	1873	rBV2	35555	71346	16.06%	1.928%
12	7.320	1941	1953	1969	rBV	183926	332239	74.80%	8.976%
13	7.397	1972	1977	1993	rVB	6731	12777	2.88%	0.345%
14	7.629	2038	2049	2063	rBV2	21621	40947	9.22%	1.106%
15	8.092	2182	2193	2227	rBV	231858	444170	100.00%	12.000%
16	8.854	2419	2430	2456	rBV	231216	387227	87.18%	10.462%
17	10.217	2844	2854	2874	rBV	73196	118657	26.71%	3.206%
18	10.384	2896	2906	2917	rVB6	2632	4825	1.09%	0.130%
19	10.921	3064	3073	3084	rBV4	4441	6660	1.50%	0.180%
20	11.252	3164	3176	3197	rBV	224872	355487	80.03%	9.604%
21	11.625	3281	3292	3309	rBV	189080	308663	69.49%	8.339%




Sum of corrected areas: 3701446

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092721\
Data File : VV022330.D
Acq On : 27 Sep 2021 11:55
Operator : SY/MD
Sample : M3834-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
EW415

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

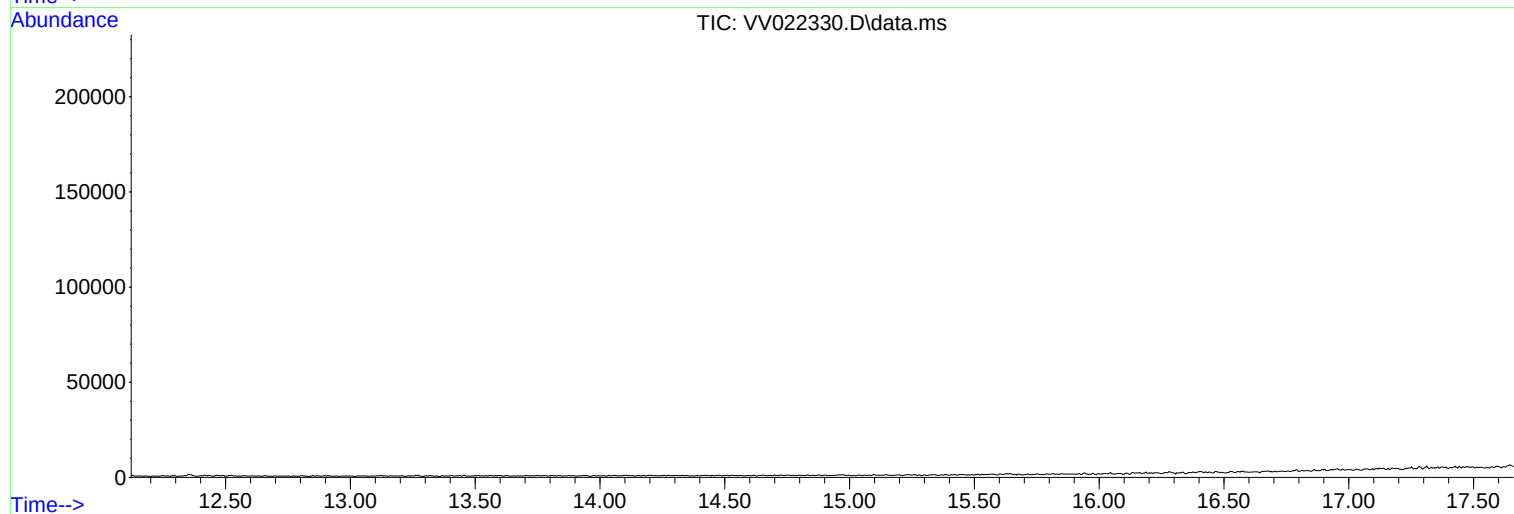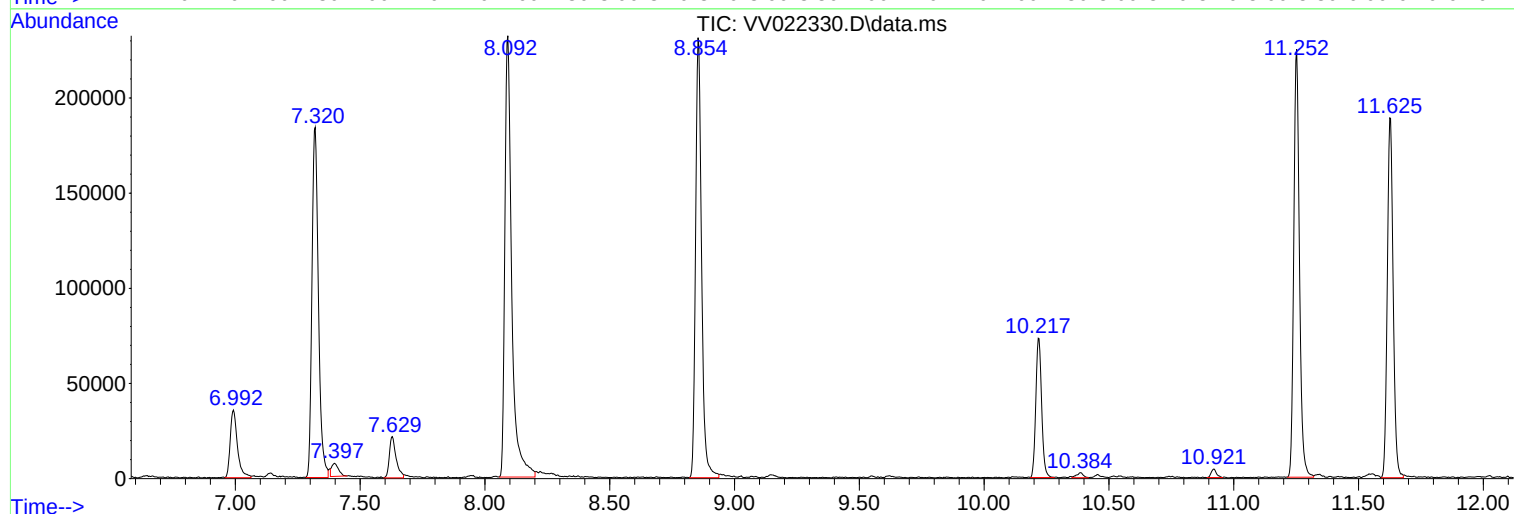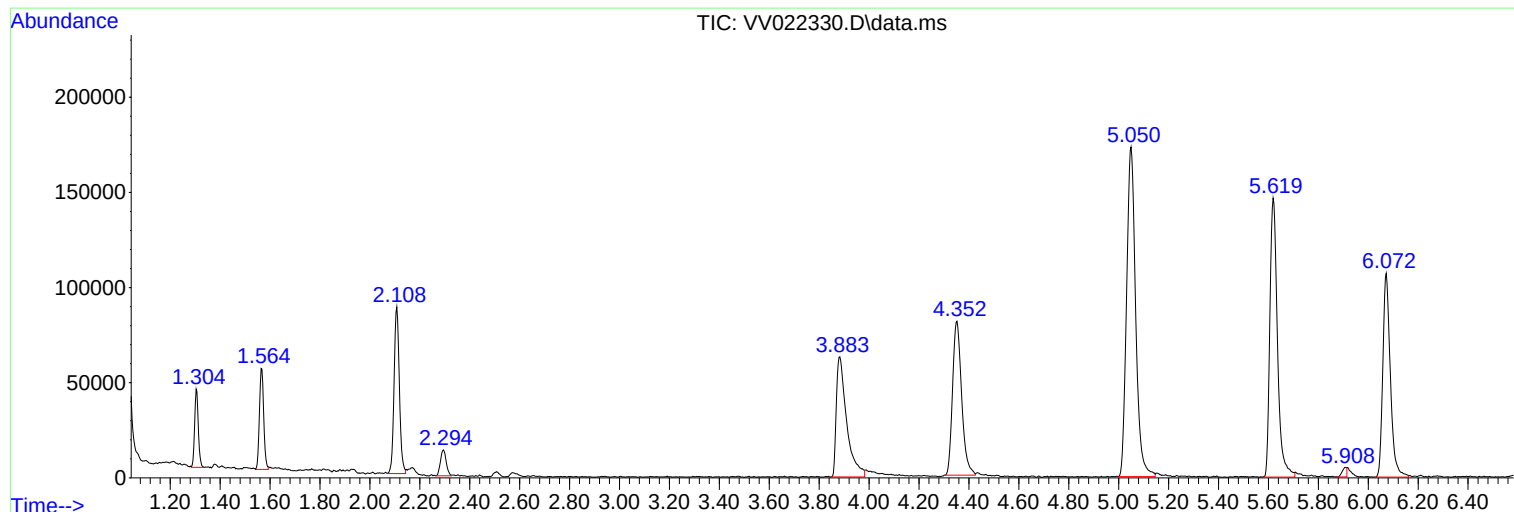

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092721\
Data File : VV022330.D
Acq On : 27 Sep 2021 11:55
Operator : SY/MD
Sample : M3834-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW415

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092721\
Data File : VV022330.D
Acq On : 27 Sep 2021 11:55
Operator : SY/MD
Sample : M3834-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW415

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
