
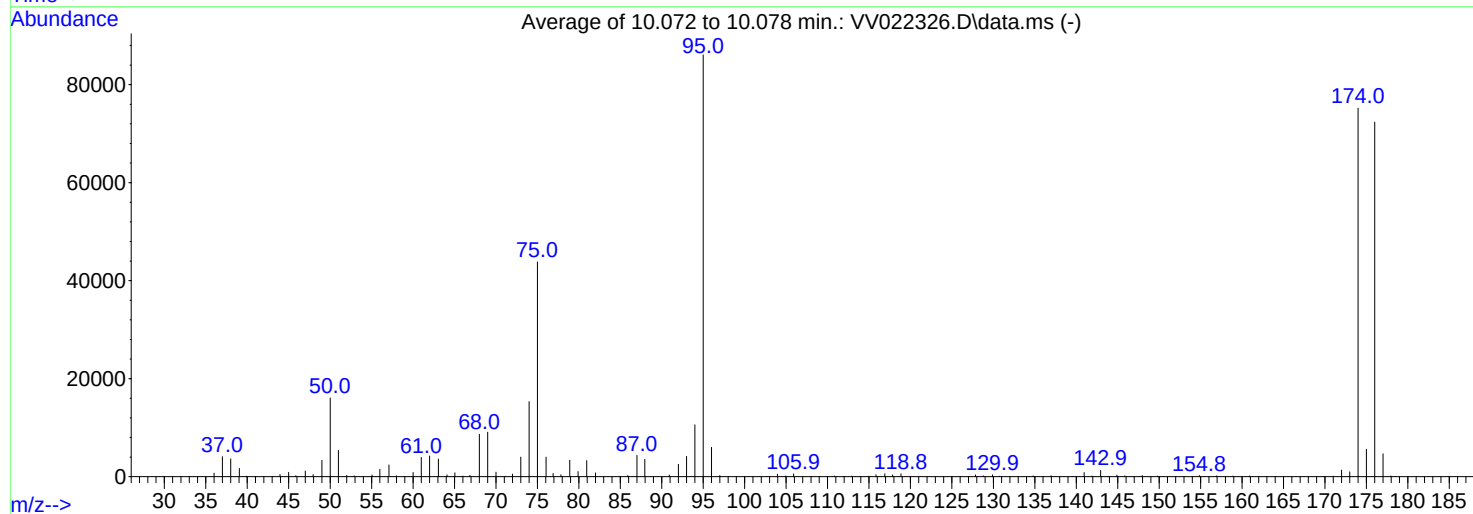


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092721\
 Data File : VV022326.D
 Acq On : 27 Sep 2021 09:06
 Operator : SY/MD
 Sample : BFB207
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB207

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Sep 28 01:24:48 2021

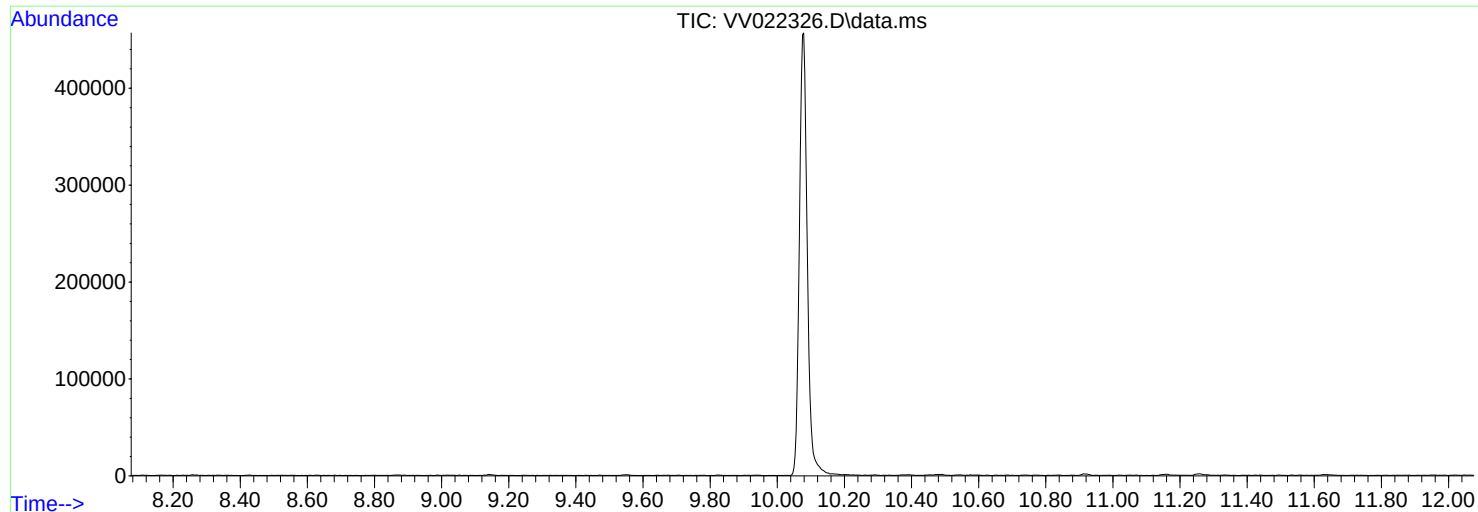

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	16077	PASS
75	95	30	80	50.9	43819	PASS
95	95	100	100	100.0	86085	PASS
96	95	5	9	7.0	5983	PASS
173	174	0.00	2	1.3	995	PASS
174	95	50	120	87.4	75221	PASS
175	174	5	9	7.4	5598	PASS
176	174	95	105	96.2	72363	PASS
177	176	5	10	6.5	4684	PASS

m/z	Abundance
40.00	172.0
43.90	317.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

m/z	Abundance
36.00	644.0
37.00	3968.0
38.00	3402.0
39.00	1501.0
39.90	257.0
41.00	122.0
44.00	729.0
45.00	776.0
45.90	185.0
47.00	1042.0
48.00	317.0
49.00	3222.0
50.00	15198.0
51.00	5090.0
52.00	236.0
52.90	162.0
55.10	298.0
56.00	1446.0
57.10	2279.0
58.00	160.0
60.00	843.0
61.00	3806.0
62.00	4061.0
63.10	3355.0
64.10	319.0
65.00	846.0
65.80	115.0
66.90	279.0
68.00	7958.0
69.00	8598.0
70.00	825.0
71.20	140.0
72.00	498.0
73.00	3884.0
74.00	14080.0
75.00	41448.0
76.10	3826.0
76.90	650.0
77.80	334.0
78.90	3190.0
79.90	951.0
80.90	3201.0
82.00	676.0
85.90	246.0
87.00	3903.0
88.00	3416.0
90.90	319.0
92.00	2267.0
93.00	3802.0
94.00	10055.0
95.00	80952.0
96.00	5639.0
97.00	264.0
103.90	382.0
104.80	139.0
105.90	533.0
110.80	103.0
111.90	125.0
112.90	109.0
115.90	384.0
116.90	533.0
117.90	347.0
118.90	537.0
127.90	336.0
128.70	172.0
129.90	321.0
134.80	136.0
136.90	195.0
141.00	777.0
141.90	125.0
142.90	1205.0
144.90	328.0
145.80	144.0
148.00	178.0
149.80	133.0
155.00	205.0
156.90	167.0
158.90	114.0
160.90	113.0
169.90	106.0
172.00	1211.0
173.00	852.0
174.00	68264.0
175.00	5050.0
176.00	66224.0
177.00	4422.0
178.00	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

m/z	Abundance
36.00	733.0
37.00	4241.0
38.00	3732.0
39.10	1727.0
39.90	273.0
44.00	774.0
45.00	934.0
45.80	183.0
47.00	1222.0
48.00	421.0
49.00	3448.0
50.00	16640.0
51.00	5556.0
52.00	281.0
52.90	171.0
55.00	350.0
56.00	1557.0
57.10	2473.0
58.00	190.0
60.00	859.0
61.00	3983.0
62.00	4357.0
63.00	3795.0
64.10	352.0
65.10	814.0
66.00	134.0
66.90	257.0
68.00	8974.0
69.00	9432.0
70.00	980.0
71.20	123.0
72.00	552.0
73.00	4130.0
74.00	15909.0
75.00	45304.0
76.10	4134.0
76.90	677.0
77.80	376.0
78.90	3533.0
79.90	1078.0
80.90	3380.0
82.00	760.0
85.90	236.0
87.00	4521.0
87.90	3666.0
90.90	337.0
92.00	2574.0
93.00	4304.0
94.00	10885.0
95.00	88952.0
96.00	6231.0
97.00	253.0
103.90	499.0
104.90	130.0
105.90	577.0
110.80	121.0
112.90	112.0
114.90	118.0
115.90	394.0
116.90	575.0
117.80	374.0
118.80	604.0
127.90	372.0
128.80	180.0
129.90	399.0
130.70	125.0
134.80	151.0
136.90	210.0
140.90	838.0
141.90	133.0
142.90	1335.0
143.90	113.0
144.90	370.0
145.80	175.0
148.00	240.0
149.80	125.0
154.80	218.0
156.90	165.0
158.90	145.0
160.90	161.0
171.00	139.0
172.00	1402.0
173.00	1026.0
174.00	77688.0
175.00	5787.0
176.00	74672.0
177.00	4776.0
177.90	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

m/z	Abundance
36.00	774.0
37.00	4057.0
38.00	3781.0
39.10	1737.0
39.90	255.0
43.00	104.0
44.00	815.0
45.00	960.0
45.80	196.0
47.00	1175.0
47.90	542.0
49.00	3362.0
50.00	16392.0
51.00	5432.0
52.00	307.0
52.90	178.0
55.00	365.0
56.00	1477.0
57.10	2458.0
58.00	150.0
60.00	855.0
61.00	3955.0
62.00	4249.0
63.00	3676.0
64.10	375.0
65.10	732.0
66.00	163.0
66.80	252.0
68.00	8989.0
69.00	9213.0
70.00	985.0
72.00	545.0
73.00	3913.0
74.00	16012.0
75.00	44704.0
76.00	4042.0
76.90	683.0
77.90	433.0
78.90	3367.0
79.90	1150.0
81.00	3225.0
82.00	775.0
85.90	193.0
87.00	4573.0
87.90	3550.0
90.90	365.0
92.00	2687.0
93.00	4310.0
94.00	10775.0
95.00	88352.0
96.00	6080.0
97.00	218.0
102.70	104.0
104.00	562.0
105.00	137.0
105.90	519.0
108.10	106.0
109.90	101.0
110.90	130.0
112.90	121.0
114.90	140.0
115.80	408.0
116.90	624.0
117.80	361.0
118.80	618.0
127.80	374.0
128.90	172.0
129.90	403.0
130.80	144.0
134.80	166.0
137.00	186.0
139.60	110.0
140.90	911.0
141.90	152.0
143.00	1322.0
143.80	128.0
144.90	321.0
145.90	180.0
147.90	254.0
149.80	145.0
154.80	232.0
157.00	174.0
158.90	147.0
160.90	167.0
171.00	126.0
172.00	1398.0
173.00	1106.0
174.00	79712.0
175.00	5956.0
176.00	76192.0
177.00	4855.0
177.90	162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207