




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037613.D
Acq On : 27 Sep 2024 17:46
Operator : SY/MD
Sample : P4184-16DL 100X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY042DL

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/30/2024
Supervised By :Mahesh Dadoda 09/30/2024

Quant Time: Sep 28 06:16:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 28 00:49:19 2024
Response via : Initial Calibration

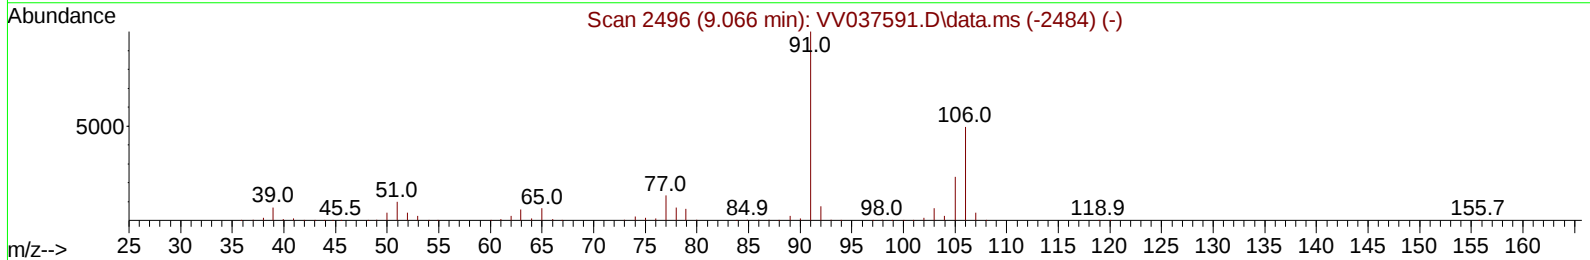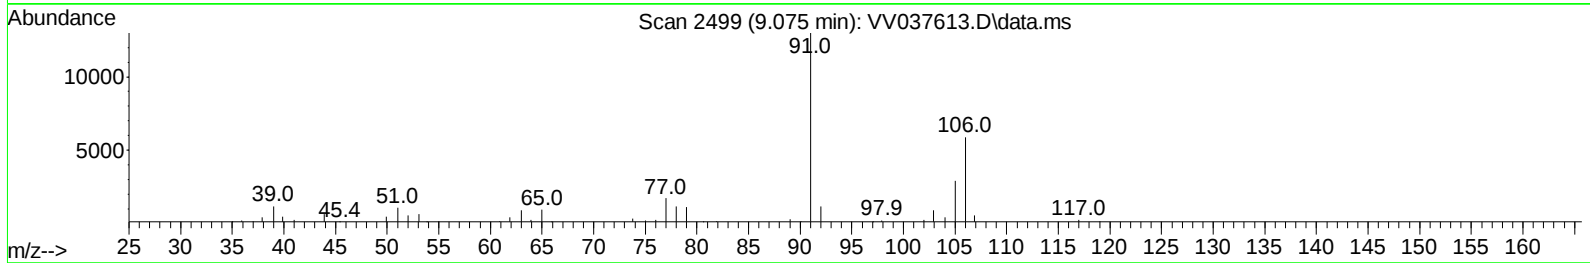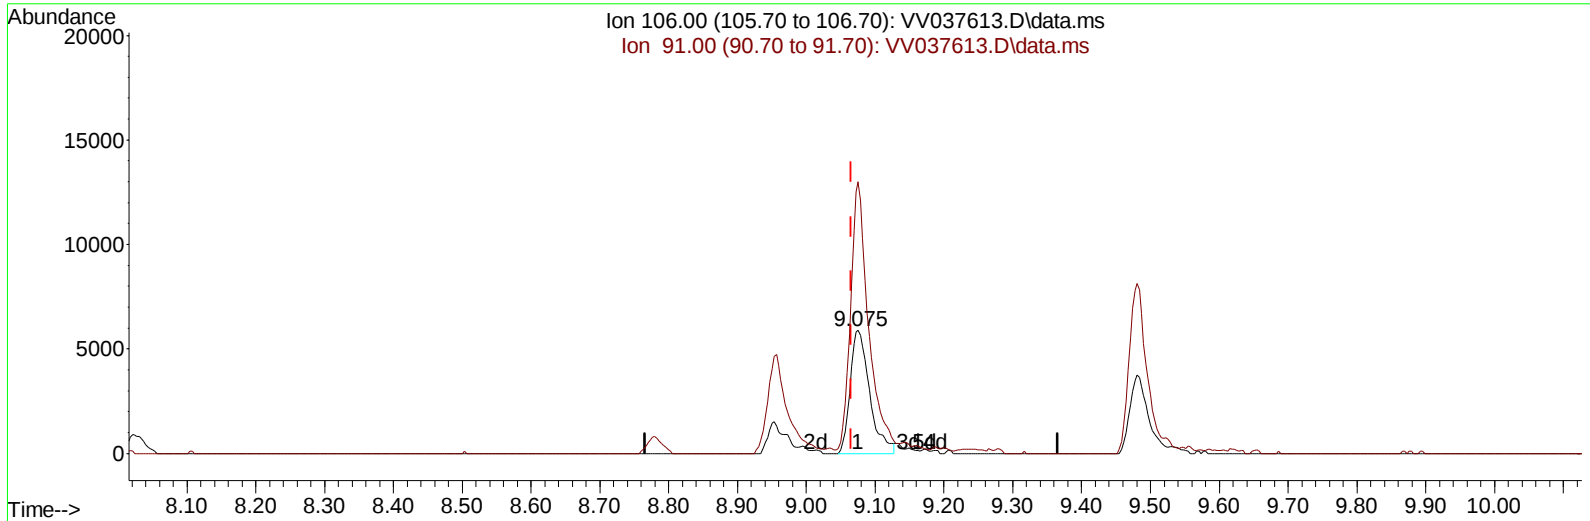

TIC: VV037613.D\data.ms

(53) m,p-Xylene (T)

9.075min (+ 0.010) 1.46 ug/L

response 11578

Ion	Exp%	Act%
106.00	100.00	100.00
91.00	202.80	220.50
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037613.D
Acq On : 27 Sep 2024 17:46
Operator : SY/MD
Sample : P4184-16DL 100X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY042DL

Manual IntegrationsAPPROVED

Quant Time: Sep 27 23:52:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 27 23:45:04 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/30/2024
Supervised By :Mahesh Dadoda 09/30/2024

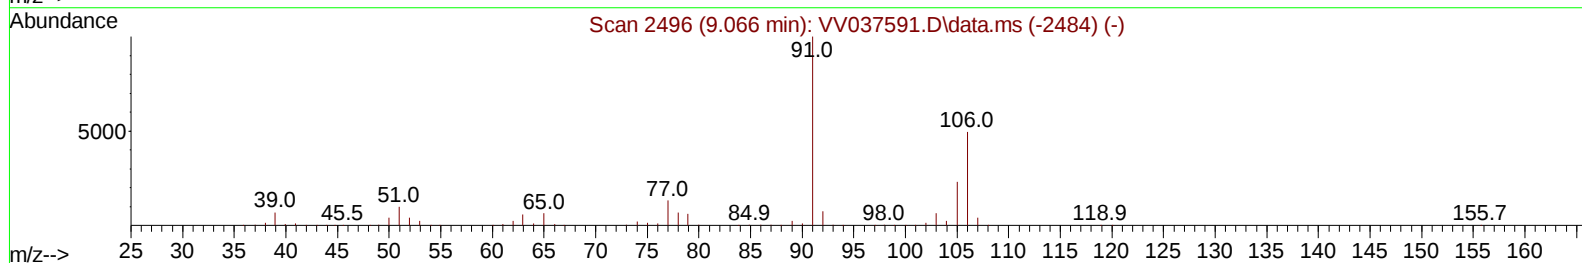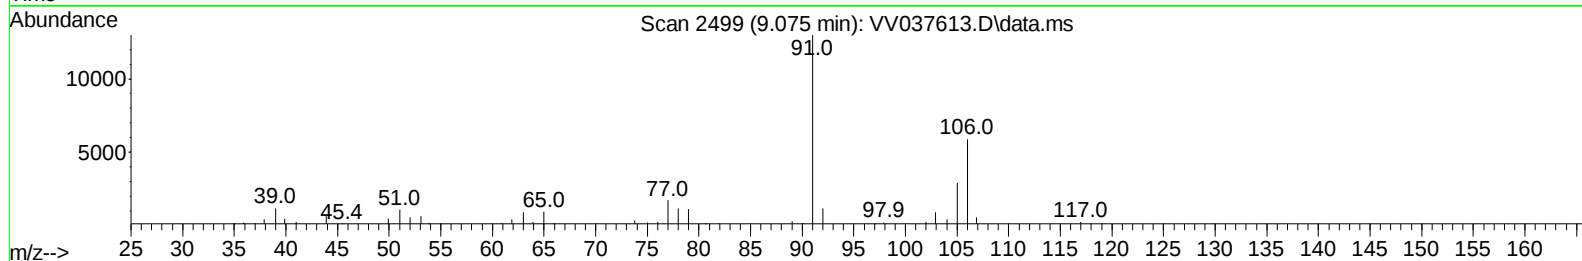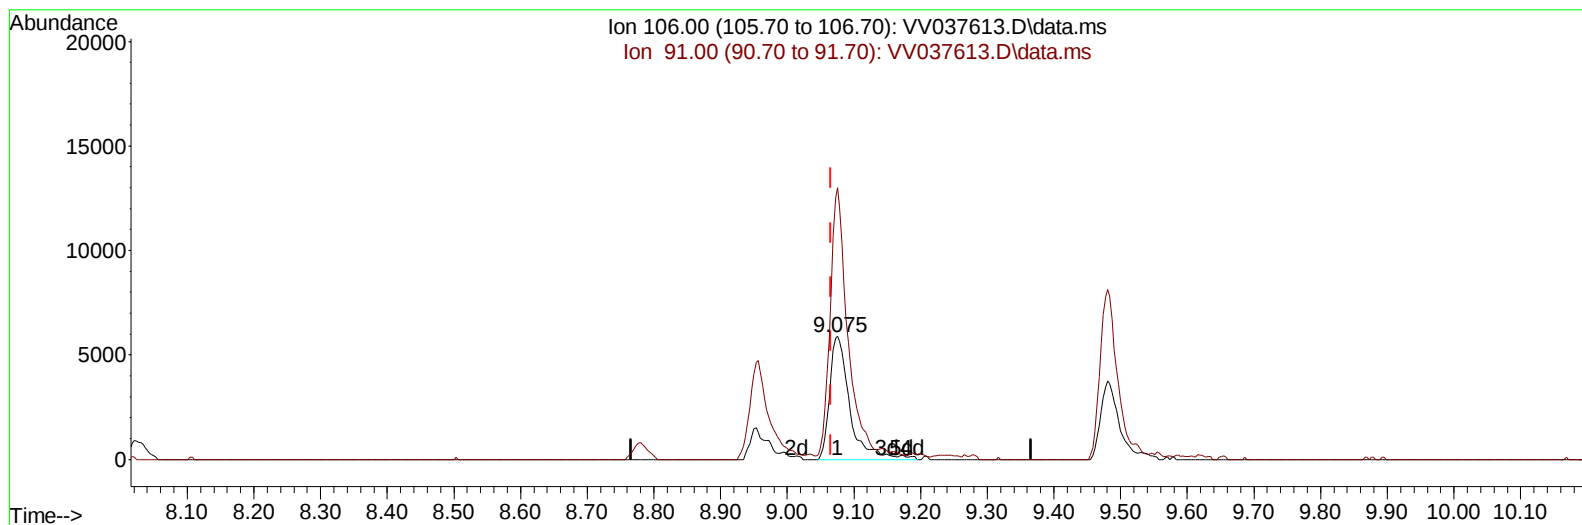

TIC: VV037613.D\data.ms

(53) m,p-Xylene (T)

9.075min (+ 0.010) 1.56 ug/L m

response 12391

Ion	Exp%	Act%
106.00	100.00	100.00
91.00	202.80	220.50
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037613.D
 Acq On : 27 Sep 2024 17:46
 Operator : SY/MD
 Sample : P4184-16DL 100X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY042DL

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/30/2024
 Supervised By :Mahesh Dadoda 09/30/2024

Quant Time: Sep 27 23:52:05 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 27 23:45:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	627831	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	605540	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	290881	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	217404	39.447	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	78.900%	
7) Chloroethane-d5	1.532	69	181966	42.536	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	85.080%	
11) 1,1-Dichloroethene-d2	2.060	65	98977	42.985	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	85.980%	
21) 2-Butanone-d5	3.793	46	182498	92.967	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	92.970%	
24) Chloroform-d	4.243	84	414829	42.306	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	84.620%	
26) 1,2-Dichloroethane-d4	4.937	65	251595	43.837	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	87.680%	
32) Benzene-d6	4.953	84	828760	43.737	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	87.480%	
36) 1,2-Dichloropropane-d6	5.982	67	266533	44.173	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	88.340%	
41) Toluene-d8	7.236	98	721590	41.997	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	84.000%	
43) trans-1,3-Dichloroprop...	7.551	79	110448	39.404	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	78.800%	
47) 2-Hexanone-d5	8.024	63	105233	82.595	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	82.590%	
56) 1,1,2,2-Tetrachloroeth...	10.146	84	301177	42.959	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	85.920%	
66) 1,2-Dichlorobenzene-d4	11.554	152	282822	46.142	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	92.280%	
Target Compounds						
						Qvalue
19) 1,1-Dichloroethane	3.105	63	171846	20.284	ug/L	99
20) cis-1,2-Dichloroethene	3.809	96	371425	75.062	ug/L	99
30) 1,1,1-Trichloroethane	4.503	97	467151	62.637	ug/L	99
42) Toluene	7.323	91	25714	1.358	ug/L	99
53) m,p-Xylene	9.075	106	12391m	1.562	ug/L	
63) 1,2,4-Trimethylbenzene	10.850	105	41207	2.770	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037613.D
Acq On : 27 Sep 2024 17:46
Operator : SY/MD
Sample : P4184-16DL 100X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY042DL

Manual IntegrationsAPPROVED

Quant Time: Sep 27 23:52:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 27 23:45:04 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/30/2024
Supervised By :Mahesh Dadoda 09/30/2024

