

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037593.D
 Acq On : 27 Sep 2024 10:06
 Operator : SY/MD
 Sample : VV0927WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK217

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037593.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	35	42	51	rBV	7295	14008	0.52%	0.072%
2	1.278	68	74	91	rVB	320307	345584	12.80%	1.770%
3	1.532	146	153	168	rVB	284413	337146	12.49%	1.727%
4	2.060	308	317	339	rVB	597890	862002	31.94%	4.415%
5	3.333	708	713	717	rBV6	818	784	0.03%	0.004%
6	3.529	772	774	776	rBV2	581	297	0.01%	0.002%
7	3.561	780	784	786	rBV2	700	516	0.02%	0.003%
8	3.619	795	802	803	rBV3	667	743	0.03%	0.004%
9	3.757	843	845	848	rBV3	481	356	0.01%	0.002%
10	3.793	848	856	892	rBV2	126046	379724	14.07%	1.945%
11	4.243	978	996	1022	rBV	439893	1131767	41.93%	5.797%
12	4.635	1116	1118	1120	rBV2	362	180	0.01%	0.001%
13	4.658	1120	1125	1126	rBV3	579	502	0.02%	0.003%
14	4.764	1157	1158	1161	rBV2	702	384	0.01%	0.002%
15	4.786	1162	1165	1169	rVV3	829	733	0.03%	0.004%
16	4.806	1169	1171	1178	rVB4	586	519	0.02%	0.003%
17	4.841	1178	1182	1184	rBV3	644	416	0.02%	0.002%
18	4.886	1190	1196	1197	rBV5	601	512	0.02%	0.003%
19	4.950	1200	1216	1249	rBV2	1059173	2699202	100.00%	13.825%
20	5.529	1385	1396	1434	rBV	746741	1539200	57.02%	7.883%
21	5.828	1480	1489	1501	rBV5	10437	22866	0.85%	0.117%
22	5.982	1525	1537	1568	rBV	609637	1260035	46.68%	6.454%
23	6.285	1625	1631	1639	rVB8	1549	2150	0.08%	0.011%
24	6.323	1639	1643	1645	rBV3	758	668	0.02%	0.003%
25	6.375	1656	1659	1663	rBV2	573	456	0.02%	0.002%
26	6.426	1672	1675	1677	rBV4	404	288	0.01%	0.001%
27	6.442	1677	1680	1683	rVV3	621	351	0.01%	0.002%
28	6.516	1701	1703	1706	rVB4	1064	469	0.02%	0.002%
29	6.539	1706	1710	1713	rBV3	990	758	0.03%	0.004%
30	6.584	1720	1724	1726	rBV3	1183	805	0.03%	0.004%
31	6.635	1738	1740	1743	rBV3	536	349	0.01%	0.002%
32	6.667	1745	1750	1755	rBV5	604	561	0.02%	0.003%
33	6.690	1755	1757	1760	rBV3	458	231	0.01%	0.001%
34	6.725	1766	1768	1774	rVB4	882	561	0.02%	0.003%
35	6.748	1774	1775	1777	rBV2	288	137	0.01%	0.001%
36	6.767	1777	1781	1784	rVV3	496	364	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037593.D
 Acq On : 27 Sep 2024 10:06
 Operator : SY/MD
 Sample : VV0927WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK217

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.783	1784	1786	1792	rVV4	709	533	0.02%	0.003%
38	6.860	1806	1810	1813	rVB4	455	304	0.01%	0.002%
39	6.908	1813	1825	1854	rBV	320692	617316	22.87%	3.162%
40	7.236	1916	1927	1962	rBV	1213981	2155471	79.86%	11.040%
41	7.548	2015	2024	2050	rBV	222922	407383	15.09%	2.087%
42	8.024	2163	2172	2213	rBV2	367304	795898	29.49%	4.076%
43	8.539	2329	2332	2333	rBV3	1225	771	0.03%	0.004%
44	8.780	2395	2407	2431	rBV	1152327	1902658	70.49%	9.745%
45	9.194	2532	2536	2540	rBV3	972	895	0.03%	0.005%
46	9.323	2573	2576	2579	rBV2	1060	712	0.03%	0.004%
47	9.432	2607	2610	2612	rBV3	1186	887	0.03%	0.005%
48	9.487	2624	2627	2631	rVB5	1027	759	0.03%	0.004%
49	9.510	2631	2634	2635	rBV2	572	339	0.01%	0.002%
50	9.551	2643	2647	2650	rBV4	983	812	0.03%	0.004%
51	9.616	2662	2667	2669	rBV3	912	760	0.03%	0.004%
52	9.677	2682	2686	2689	rBV4	898	588	0.02%	0.003%
53	9.699	2691	2693	2696	rVB3	773	352	0.01%	0.002%
54	9.722	2696	2700	2703	rBV3	640	554	0.02%	0.003%
55	9.754	2709	2710	2713	rBV	360	192	0.01%	0.001%
56	9.789	2717	2721	2724	rBV3	677	589	0.02%	0.003%
57	9.805	2724	2726	2727	rBV3	240	79	0.00%	0.000%
58	9.844	2736	2738	2741	rVB3	423	228	0.01%	0.001%
59	9.866	2741	2745	2747	rBV4	1146	984	0.04%	0.005%
60	9.928	2762	2764	2768	rBV3	418	277	0.01%	0.001%
61	9.998	2784	2786	2789	rBV3	629	379	0.01%	0.002%
62	10.030	2791	2796	2798	rVV3	553	484	0.02%	0.002%
63	10.059	2802	2805	2807	rVB3	612	365	0.01%	0.002%
64	10.095	2814	2816	2819	rVB2	577	287	0.01%	0.001%
65	10.146	2820	2832	2857	rBV	727117	1169597	43.33%	5.990%
66	10.567	2961	2963	2965	rBV2	769	378	0.01%	0.002%
67	10.580	2965	2967	2970	rVV3	712	358	0.01%	0.002%
68	10.641	2984	2986	2988	rVB2	415	185	0.01%	0.001%
69	10.657	2988	2991	2992	rBV	403	167	0.01%	0.001%
70	10.767	3023	3025	3027	rBV2	346	148	0.01%	0.001%
71	10.783	3028	3030	3037	rVB5	1164	962	0.04%	0.005%
72	10.828	3040	3044	3046	rBV3	673	541	0.02%	0.003%
73	10.969	3086	3088	3090	rBV	288	150	0.01%	0.001%
74	11.014	3093	3102	3104	rBV4	940	1144	0.04%	0.006%
75	11.046	3109	3112	3114	rBV2	523	350	0.01%	0.002%
76	11.101	3125	3129	3132	rBV4	720	584	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037593.D
 Acq On : 27 Sep 2024 10:06
 Operator : SY/MD
 Sample : VV0927WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK217

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	11.178	3142	3153	3174	rBV	1147353	1781507	66.00%	9.124%
78	11.554	3258	3270	3306	rBV	1279215	2059016	76.28%	10.546%
79	12.072	3429	3431	3433	rBV2	717	351	0.01%	0.002%
80	12.153	3454	3456	3459	rBV3	601	369	0.01%	0.002%
81	12.178	3459	3464	3468	rVB6	1378	1390	0.05%	0.007%
82	12.233	3474	3481	3484	rBV3	1442	1435	0.05%	0.007%
83	12.291	3495	3499	3500	rBV2	688	492	0.02%	0.003%
84	12.326	3508	3510	3515	rVB3	573	356	0.01%	0.002%
85	12.352	3515	3518	3519	rBV	377	210	0.01%	0.001%
86	12.371	3523	3524	3526	rBV	414	210	0.01%	0.001%
87	12.403	3532	3534	3536	rBV	379	127	0.00%	0.001%
88	12.429	3536	3542	3546	rBV6	965	1167	0.04%	0.006%
89	12.667	3613	3616	3620	rBV4	857	718	0.03%	0.004%
90	12.763	3642	3646	3650	rBV6	921	819	0.03%	0.004%
91	13.034	3728	3730	3732	rBV3	577	333	0.01%	0.002%
92	13.120	3754	3757	3760	rBV4	721	550	0.02%	0.003%
93	13.689	3929	3934	3942	rVB7	2237	2873	0.11%	0.015%
94	13.757	3951	3955	3960	rBV6	1021	1207	0.04%	0.006%
95	13.853	3983	3985	3988	rBV3	914	459	0.02%	0.002%




Sum of corrected areas: 19524633

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037593.D
Acq On : 27 Sep 2024 10:06
Operator : SY/MD
Sample : VV0927WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK217

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

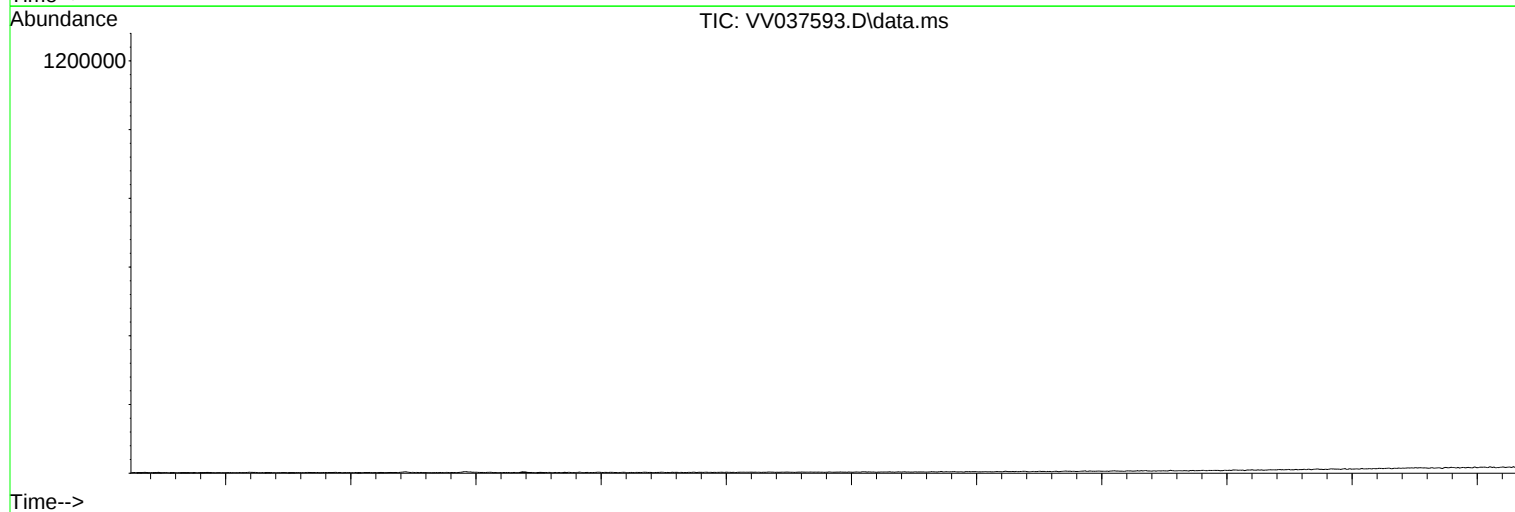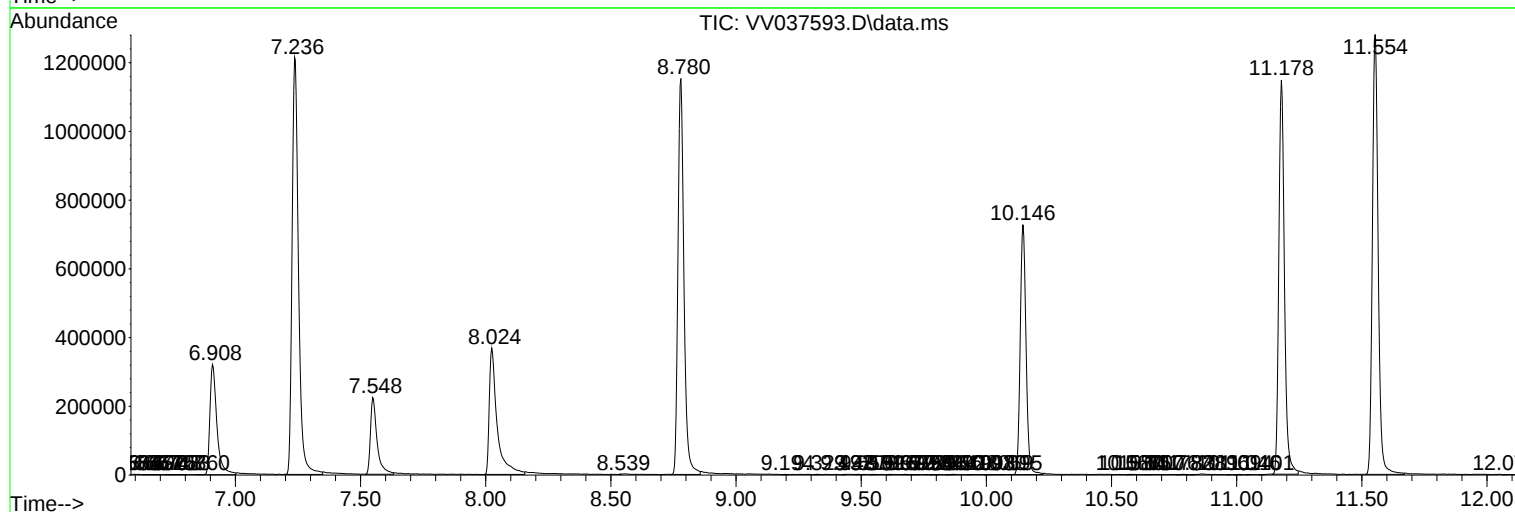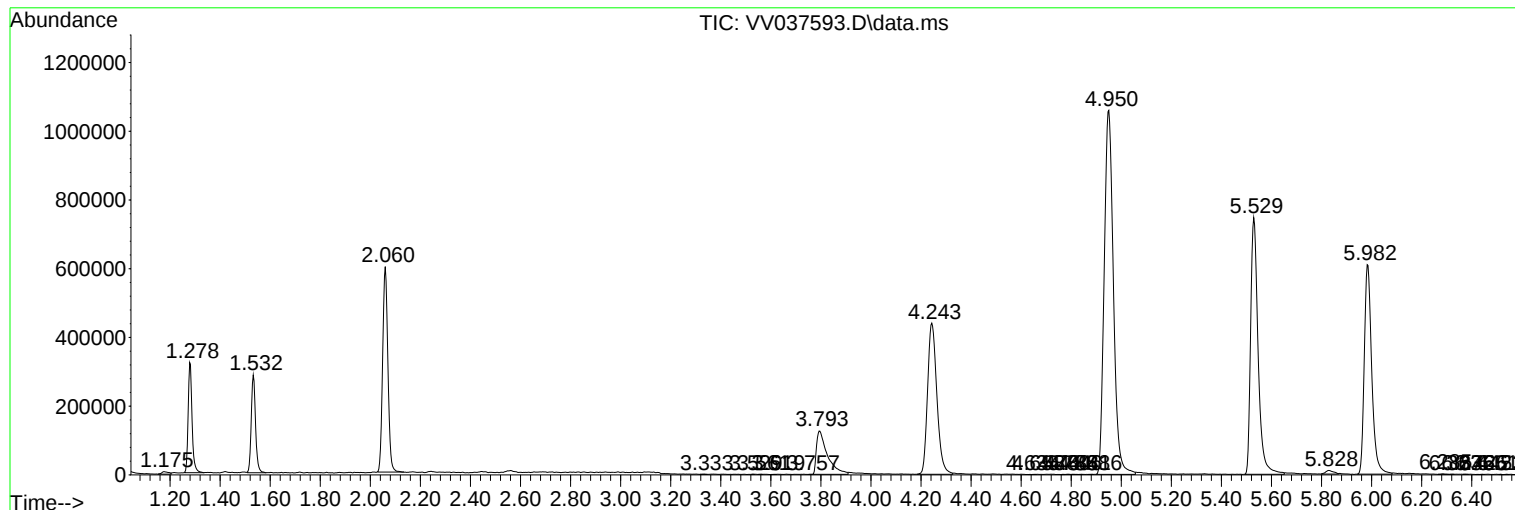

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037593.D
Acq On : 27 Sep 2024 10:06
Operator : SY/MD
Sample : VV0927WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK217

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037593.D
Acq On : 27 Sep 2024 10:06
Operator : SY/MD
Sample : VV0927WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK217

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc