

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037601.D
 Acq On : 27 Sep 2024 13:28
 Operator : SY/MD
 Sample : P4184-08
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY036

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037601.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	49	rBV	9313	13907	0.57%	0.072%
2	1.278	67	74	92	rBV	327708	354123	14.59%	1.827%
3	1.416	112	117	121	rBV7	3117	3896	0.16%	0.020%
4	1.532	145	153	174	rVB	276495	327166	13.48%	1.687%
5	1.992	293	296	299	rBV3	2526	2038	0.08%	0.011%
6	2.060	306	317	339	rBV2	605451	912020	37.58%	4.704%
7	3.105	630	642	663	rVB	321622	669972	27.61%	3.456%
8	3.378	722	727	729	rBV3	834	781	0.03%	0.004%
9	3.539	773	777	779	rBV2	838	587	0.02%	0.003%
10	3.590	790	793	799	rVB2	985	735	0.03%	0.004%
11	3.616	799	801	805	rBV3	786	641	0.03%	0.003%
12	3.699	823	827	829	rBV2	651	463	0.02%	0.002%
13	3.799	848	858	890	rBV2	136829	405791	16.72%	2.093%
14	4.056	936	938	945	rVB4	811	669	0.03%	0.003%
15	4.243	980	996	1022	rBV	391462	1006550	41.48%	5.192%
16	4.506	1057	1078	1109	rBV2	279633	718126	29.59%	3.704%
17	4.699	1133	1138	1141	rBV4	784	855	0.04%	0.004%
18	4.818	1171	1175	1179	rVB2	517	489	0.02%	0.003%
19	4.892	1195	1198	1200	rBV	774	587	0.02%	0.003%
20	4.950	1200	1216	1261	rBV2	949917	2426647	100.00%	12.516%
21	5.211	1292	1297	1300	rBV5	1296	1340	0.06%	0.007%
22	5.333	1333	1335	1342	rVB5	1574	1076	0.04%	0.006%
23	5.397	1353	1355	1359	rBV3	666	516	0.02%	0.003%
24	5.468	1374	1377	1382	rVB5	846	678	0.03%	0.003%
25	5.529	1385	1396	1430	rBV	711489	1472798	60.69%	7.596%
26	5.838	1479	1492	1510	rBV8	27500	70519	2.91%	0.364%
27	5.985	1525	1538	1571	rBV	526312	1095733	45.15%	5.652%
28	6.249	1616	1620	1624	rBV5	922	942	0.04%	0.005%
29	6.294	1632	1634	1636	rBV2	1007	643	0.03%	0.003%
30	6.394	1662	1665	1667	rBV3	1059	574	0.02%	0.003%
31	6.420	1671	1673	1676	rVB3	920	492	0.02%	0.003%
32	6.439	1676	1679	1681	rBV3	659	503	0.02%	0.003%
33	6.580	1719	1723	1727	rVB4	1328	1153	0.05%	0.006%
34	6.603	1727	1730	1732	rBV2	924	618	0.03%	0.003%
35	6.696	1757	1759	1762	rBV2	790	563	0.02%	0.003%
36	6.821	1792	1798	1800	rBV3	522	528	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037601.D
 Acq On : 27 Sep 2024 13:28
 Operator : SY/MD
 Sample : P4184-08
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY036

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.908	1814	1825	1859	rBV	273969	537015	22.13%	2.770%
38	7.239	1916	1928	1960	rBV	1082274	1924507	79.31%	9.926%
39	7.551	2016	2025	2050	rBV	184996	350112	14.43%	1.806%
40	7.902	2124	2134	2154	rBV3	53803	98348	4.05%	0.507%
41	8.027	2164	2173	2208	rBV2	310833	682552	28.13%	3.520%
42	8.545	2331	2334	2338	rBV7	1552	1215	0.05%	0.006%
43	8.609	2351	2354	2357	rVB5	850	561	0.02%	0.003%
44	8.641	2361	2364	2369	rBV4	745	777	0.03%	0.004%
45	8.706	2379	2384	2385	rBV3	718	614	0.03%	0.003%
46	8.780	2396	2407	2442	rBV	1091954	1823691	75.15%	9.406%
47	9.207	2535	2540	2541	rBV3	685	477	0.02%	0.002%
48	9.333	2576	2579	2584	rVB3	1234	660	0.03%	0.003%
49	9.487	2623	2627	2628	rBV3	744	464	0.02%	0.002%
50	9.599	2659	2662	2664	rBV3	983	507	0.02%	0.003%
51	9.693	2688	2691	2695	rVB4	508	472	0.02%	0.002%
52	9.744	2705	2707	2711	rVB4	704	542	0.02%	0.003%
53	9.931	2759	2765	2768	rVB5	690	707	0.03%	0.004%
54	9.985	2777	2782	2785	rBV4	962	699	0.03%	0.004%
55	10.001	2785	2787	2790	rVB2	899	485	0.02%	0.003%
56	10.146	2818	2832	2856	rBV	616029	993330	40.93%	5.123%
57	10.413	2913	2915	2919	rVB3	759	491	0.02%	0.003%
58	10.542	2952	2955	2960	rVV4	609	575	0.02%	0.003%
59	10.622	2976	2980	2984	rVB4	893	653	0.03%	0.003%
60	10.734	3009	3015	3018	rBV4	579	613	0.03%	0.003%
61	10.754	3018	3021	3026	rVV5	828	900	0.04%	0.005%
62	10.789	3026	3032	3039	rVB8	1551	2157	0.09%	0.011%
63	10.866	3047	3056	3068	rBV6	1950	4202	0.17%	0.022%
64	10.911	3068	3070	3077	rVB4	606	512	0.02%	0.003%
65	10.998	3093	3097	3102	rVB5	967	882	0.04%	0.005%
66	11.123	3132	3136	3137	rBV4	1065	592	0.02%	0.003%
67	11.133	3137	3139	3143	rVV3	1900	1273	0.05%	0.007%
68	11.178	3143	3153	3189	rVV	1080318	1708658	70.41%	8.813%
69	11.554	3257	3270	3299	rBV	1064709	1725563	71.11%	8.900%
70	11.931	3385	3387	3390	rBV	894	665	0.03%	0.003%
71	12.143	3449	3453	3456	rBV5	709	628	0.03%	0.003%
72	12.213	3470	3475	3479	rVB4	842	837	0.03%	0.004%
73	12.242	3479	3484	3486	rBV2	1082	981	0.04%	0.005%
74	12.304	3497	3503	3507	rBV4	876	971	0.04%	0.005%
75	12.361	3519	3521	3525	rVB2	981	719	0.03%	0.004%
76	12.590	3588	3592	3594	rBV2	1156	863	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037601.D
 Acq On : 27 Sep 2024 13:28
 Operator : SY/MD
 Sample : P4184-08
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY036

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.693	3622	3624	3627	rVB3	895	510	0.02%	0.003%
78	12.760	3638	3645	3650	rVB7	942	1094	0.05%	0.006%
79	12.789	3652	3654	3658	rVB4	811	551	0.02%	0.003%
80	12.815	3658	3662	3664	rBV2	1026	854	0.04%	0.004%
81	12.879	3679	3682	3688	rVB4	906	841	0.03%	0.004%
82	12.930	3694	3698	3703	rBV3	1044	908	0.04%	0.005%
83	12.959	3703	3707	3710	rBV3	678	502	0.02%	0.003%
84	13.004	3717	3721	3722	rBV4	669	480	0.02%	0.002%
85	13.213	3780	3786	3795	rBV6	2475	3530	0.15%	0.018%
86	13.271	3802	3804	3808	rVB3	755	480	0.02%	0.002%
87	13.294	3808	3811	3815	rVB5	904	640	0.03%	0.003%
88	13.320	3815	3819	3824	rBV7	1292	1279	0.05%	0.007%
89	13.464	3856	3864	3869	rBV8	2052	3300	0.14%	0.017%
90	13.686	3931	3933	3938	rVV4	1159	639	0.03%	0.003%
91	13.725	3942	3945	3947	rBV2	914	543	0.02%	0.003%
92	13.824	3971	3976	3978	rBV5	1173	1148	0.05%	0.006%
93	13.940	4010	4012	4016	rBV4	922	711	0.03%	0.004%
94	13.969	4017	4021	4023	rBV5	809	737	0.03%	0.004%
95	14.352	4136	4140	4144	rBV4	1085	778	0.03%	0.004%
96	14.397	4151	4154	4156	rBV2	869	616	0.03%	0.003%
97	14.596	4213	4216	4219	rBV3	817	686	0.03%	0.004%
98	14.676	4239	4241	4245	rBV4	776	497	0.02%	0.003%
99	14.924	4314	4318	4322	rBV4	862	862	0.04%	0.004%
100	15.004	4340	4343	4346	rBV3	879	583	0.02%	0.003%

Sum of corrected areas: 19387958




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037601.D
Acq On : 27 Sep 2024 13:28
Operator : SY/MD
Sample : P4184-08
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY036

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

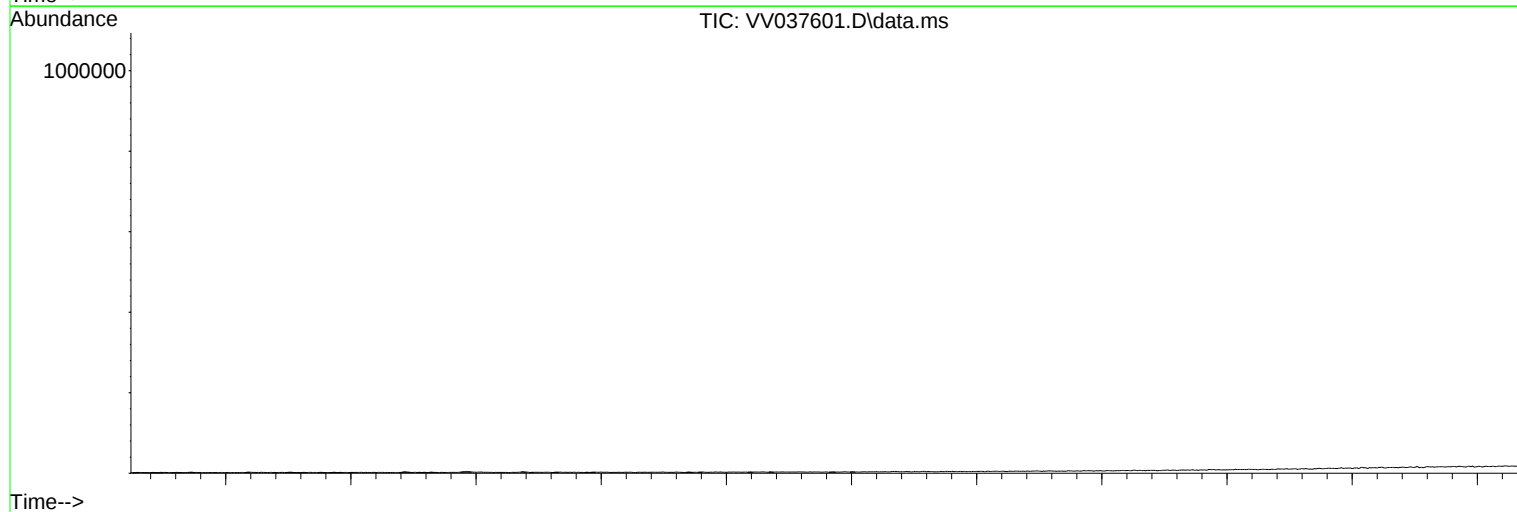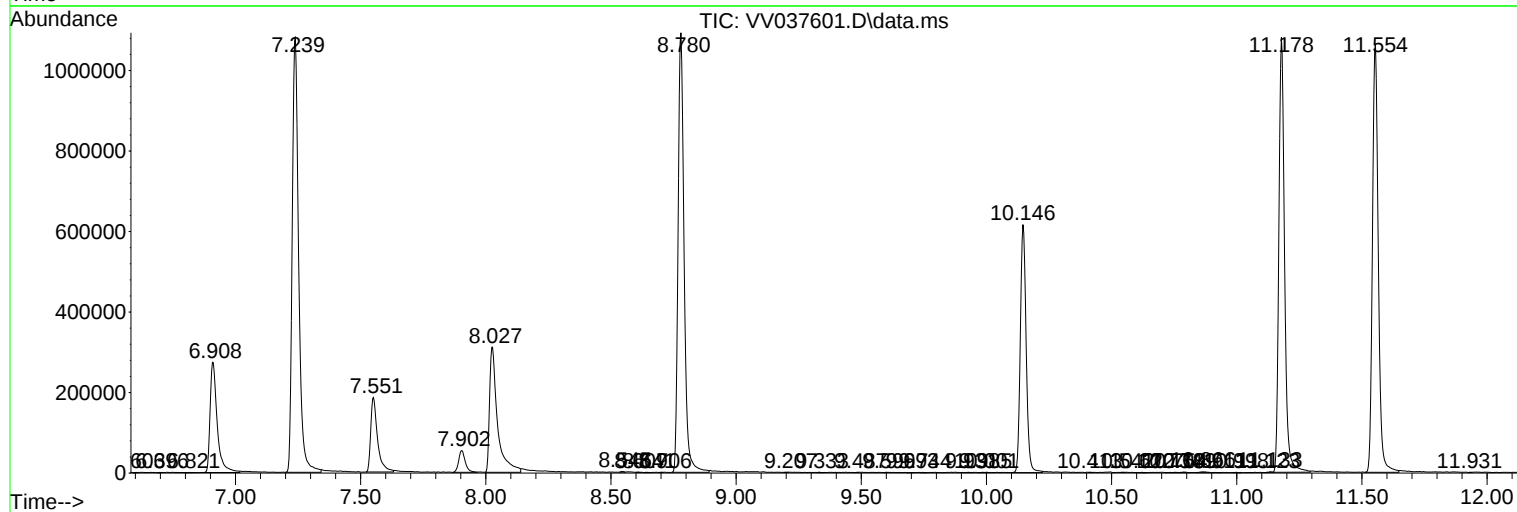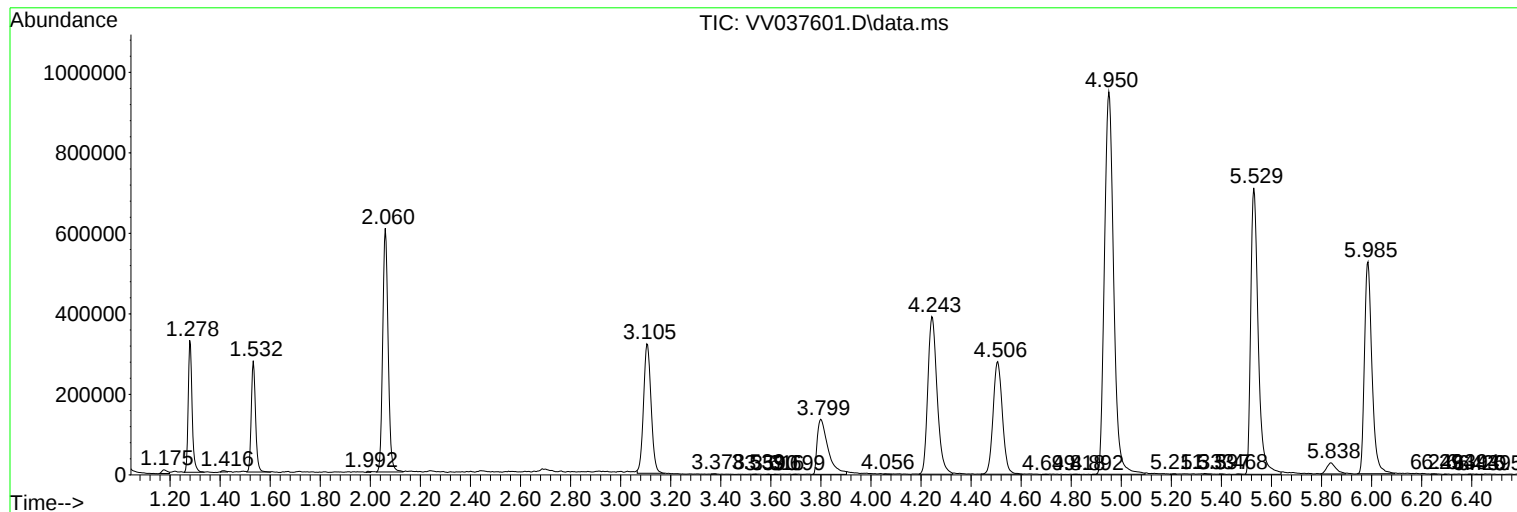

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037601.D
Acq On : 27 Sep 2024 13:28
Operator : SY/MD
Sample : P4184-08
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY036

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037601.D
Acq On : 27 Sep 2024 13:28
Operator : SY/MD
Sample : P4184-08
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY036

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
