

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037605.D
 Acq On : 27 Sep 2024 14:54
 Operator : SY/MD
 Sample : VIBLK391
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK391

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037605.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	95	rVB	306851	336188	12.87%	1.782%
2	1.532	146	153	169	rVB	277065	327716	12.55%	1.737%
3	2.059	307	317	338	rVB	573821	830011	31.78%	4.399%
4	3.429	739	743	745	rBV2	808	686	0.03%	0.004%
5	3.567	784	786	789	rVB3	482	176	0.01%	0.001%
6	3.641	807	809	813	rBV2	519	302	0.01%	0.002%
7	3.661	813	815	817	rVB3	614	242	0.01%	0.001%
8	3.731	834	837	841	rVB3	556	336	0.01%	0.002%
9	3.748	841	842	844	rVB2	158	38	0.00%	0.000%
10	3.796	847	857	898	rBV2	128865	405585	15.53%	2.150%
11	4.140	961	964	970	rBV5	1327	1115	0.04%	0.006%
12	4.243	981	996	1035	rVB	426170	1091294	41.78%	5.784%
13	4.571	1095	1098	1100	rBV2	671	335	0.01%	0.002%
14	4.606	1107	1109	1113	rBV3	719	422	0.02%	0.002%
15	4.654	1122	1124	1125	rBV	360	162	0.01%	0.001%
16	4.770	1155	1160	1164	rBV4	971	1029	0.04%	0.005%
17	4.841	1180	1182	1184	rBV	599	276	0.01%	0.001%
18	4.866	1188	1190	1193	rVB3	1094	605	0.02%	0.003%
19	4.883	1193	1195	1200	rVB3	546	447	0.02%	0.002%
20	4.950	1200	1216	1247	rBV2	1027828	2612111	100.00%	13.846%
21	5.529	1385	1396	1430	rBV	705787	1470087	56.28%	7.792%
22	5.985	1524	1538	1567	rBV	586372	1221374	46.76%	6.474%
23	6.281	1627	1630	1632	rBV3	1339	898	0.03%	0.005%
24	6.384	1660	1662	1664	rBV3	798	482	0.02%	0.003%
25	6.538	1706	1710	1713	rBV4	569	507	0.02%	0.003%
26	6.564	1716	1718	1721	rBV3	695	356	0.01%	0.002%
27	6.599	1725	1729	1731	rBV2	590	362	0.01%	0.002%
28	6.641	1740	1742	1749	rBV5	787	910	0.03%	0.005%
29	6.673	1749	1752	1753	rBV2	510	278	0.01%	0.001%
30	6.709	1759	1763	1769	rBV6	1163	1247	0.05%	0.007%
31	6.735	1769	1771	1777	rBV4	661	597	0.02%	0.003%
32	6.783	1783	1786	1788	rBV3	564	283	0.01%	0.002%
33	6.812	1793	1795	1797	rBV3	470	255	0.01%	0.001%
34	6.841	1803	1804	1807	rBV	333	204	0.01%	0.001%
35	6.908	1815	1825	1859	rBV	311141	594211	22.75%	3.150%
36	7.239	1917	1928	1954	rBV	1173571	2070599	79.27%	10.975%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037605.D
 Acq On : 27 Sep 2024 14:54
 Operator : SY/MD
 Sample : VIBLK391
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK391

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.548	2016	2024	2058	rBV	206186	395382	15.14%	2.096%
38	8.024	2163	2172	2212	rBV2	370106	798914	30.58%	4.235%
39	8.779	2396	2407	2433	rBV	1107378	1833694	70.20%	9.720%
40	9.336	2578	2580	2583	rBV2	469	236	0.01%	0.001%
41	9.419	2605	2606	2607	rBV2	472	124	0.00%	0.001%
42	9.429	2607	2609	2612	rVV2	515	251	0.01%	0.001%
43	9.445	2612	2614	2616	rVB	399	197	0.01%	0.001%
44	9.551	2644	2647	2649	rVB3	946	497	0.02%	0.003%
45	9.567	2649	2652	2655	rBV2	528	241	0.01%	0.001%
46	9.583	2655	2657	2658	rBV2	614	225	0.01%	0.001%
47	9.635	2671	2673	2676	rBV2	565	363	0.01%	0.002%
48	9.734	2702	2704	2705	rVB2	437	96	0.00%	0.001%
49	9.767	2712	2714	2716	rBV	441	195	0.01%	0.001%
50	9.783	2716	2719	2722	rVV3	701	405	0.02%	0.002%
51	9.805	2722	2726	2728	rVB2	365	280	0.01%	0.001%
52	9.837	2732	2736	2739	rBV3	1001	753	0.03%	0.004%
53	9.956	2770	2773	2774	rBV2	364	180	0.01%	0.001%
54	10.050	2799	2802	2806	rVB3	509	422	0.02%	0.002%
55	10.082	2809	2812	2813	rBV2	402	214	0.01%	0.001%
56	10.146	2820	2832	2856	rBV	737492	1154701	44.21%	6.121%
57	10.336	2889	2891	2893	rVB2	781	268	0.01%	0.001%
58	10.445	2923	2925	2926	rBV	581	195	0.01%	0.001%
59	10.564	2959	2962	2964	rBV2	595	329	0.01%	0.002%
60	10.606	2973	2975	2980	rBV4	593	481	0.02%	0.003%
61	10.680	2995	2998	3002	rBV4	804	604	0.02%	0.003%
62	10.718	3007	3010	3014	rVB3	630	444	0.02%	0.002%
63	10.750	3016	3020	3022	rBV3	748	576	0.02%	0.003%
64	10.808	3036	3038	3039	rBV	268	117	0.00%	0.001%
65	10.934	3074	3077	3081	rBV3	704	428	0.02%	0.002%
66	10.959	3083	3085	3089	rVB4	499	274	0.01%	0.001%
67	11.001	3095	3098	3099	rBV3	480	279	0.01%	0.001%
68	11.104	3128	3130	3132	rBV2	530	219	0.01%	0.001%
69	11.178	3143	3153	3182	rBV	1073742	1709280	65.44%	9.060%
70	11.554	3259	3270	3305	rBV	1238660	1983699	75.94%	10.515%
71	12.123	3443	3447	3449	rBV4	1049	896	0.03%	0.005%
72	12.316	3505	3507	3510	rBV2	772	397	0.02%	0.002%
73	12.365	3519	3522	3526	rBV5	850	881	0.03%	0.005%
74	12.567	3583	3585	3589	rBV3	507	290	0.01%	0.002%
75	12.593	3590	3593	3594	rBV2	733	415	0.02%	0.002%
76	12.635	3605	3606	3608	rBV2	671	229	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037605.D
 Acq On : 27 Sep 2024 14:54
 Operator : SY/MD
 Sample : VIBLK391
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK391

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.696	3621	3625	3626	rBV3	667	396	0.02%	0.002%
78	12.766	3644	3647	3649	rBV4	805	539	0.02%	0.003%
79	12.905	3686	3690	3694	rBV3	812	807	0.03%	0.004%
80	12.950	3702	3704	3707	rVB5	578	214	0.01%	0.001%
81	13.130	3758	3760	3765	rBV3	858	723	0.03%	0.004%
82	13.297	3809	3812	3816	rVB4	910	671	0.03%	0.004%
83	13.345	3826	3827	3829	rBV2	666	205	0.01%	0.001%
84	13.448	3856	3859	3861	rBV3	1206	993	0.04%	0.005%
85	13.561	3892	3894	3896	rBV2	892	486	0.02%	0.003%
86	13.721	3941	3944	3946	rBV4	871	554	0.02%	0.003%
87	13.834	3973	3979	3982	rBV4	1217	1130	0.04%	0.006%

Sum of corrected areas: 18866115




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037605.D
Acq On : 27 Sep 2024 14:54
Operator : SY/MD
Sample : VIBLK391
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK391

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

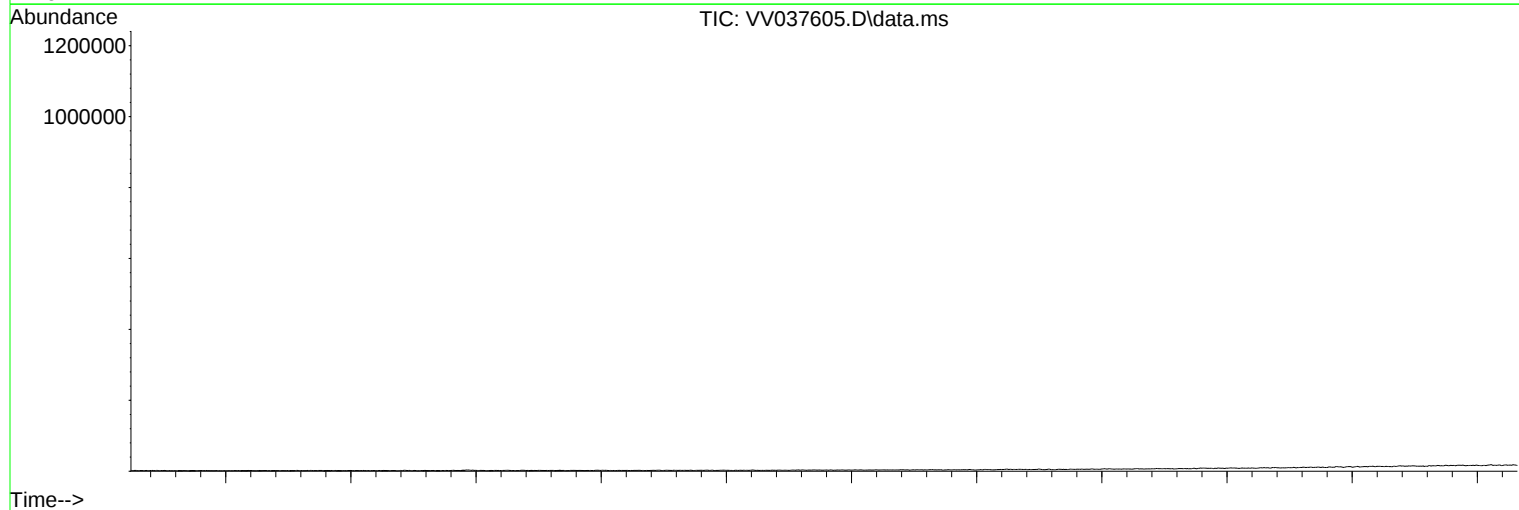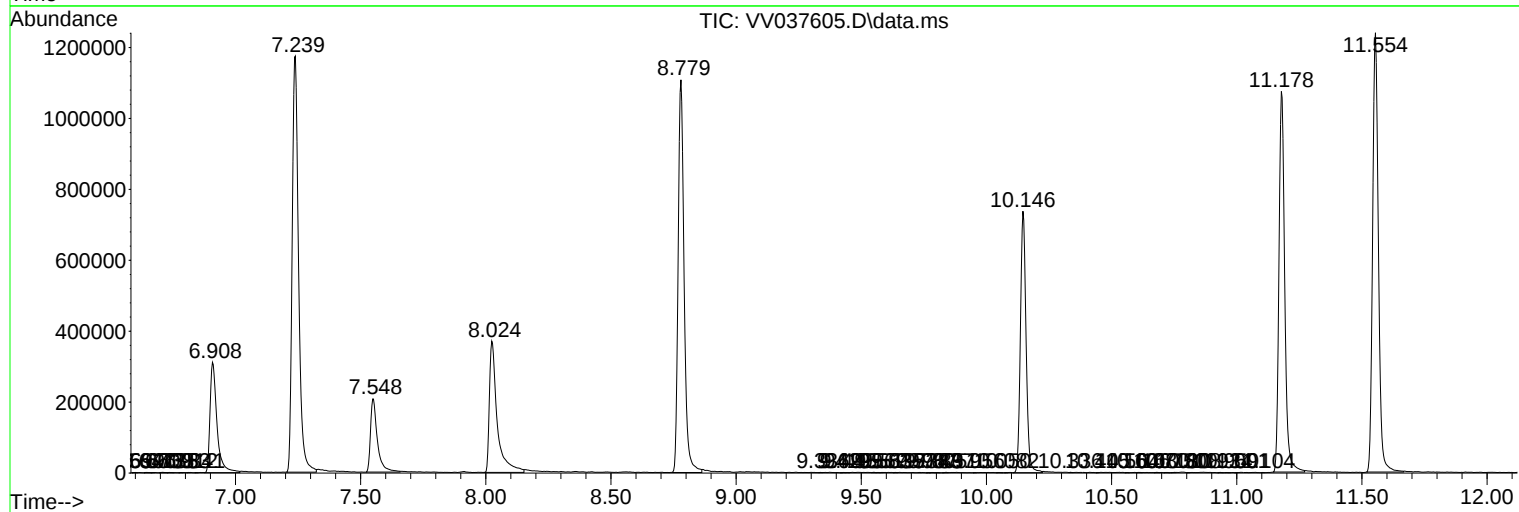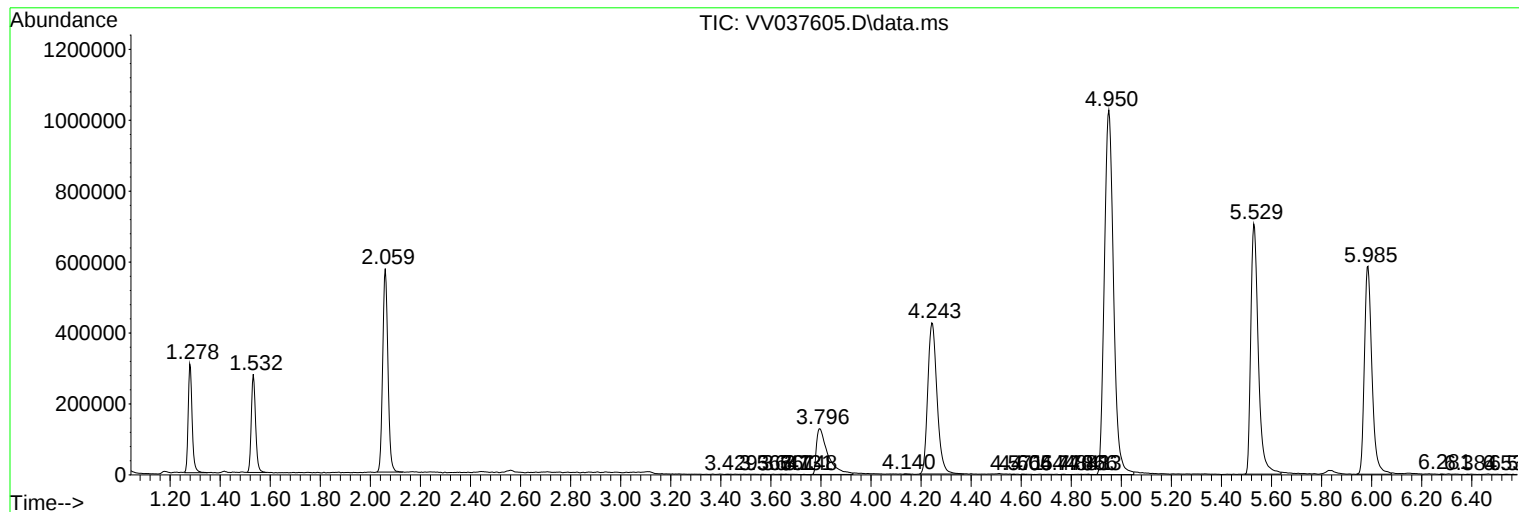

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037605.D
Acq On : 27 Sep 2024 14:54
Operator : SY/MD
Sample : VIBLK391
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK391

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037605.D
Acq On : 27 Sep 2024 14:54
Operator : SY/MD
Sample : VIBLK391
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK391

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc