

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037610.D
 Acq On : 27 Sep 2024 16:41
 Operator : SY/MD
 Sample : P4184-05DL 10X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY033DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037610.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	37	41	51	rBV2	5943	12357	0.53%	0.064%
2	1.278	67	74	93	rVB	337198	377510	16.07%	1.960%
3	1.519	142	149	166	rVB2	261733	391687	16.67%	2.034%
4	2.053	306	315	331	rVB	550781	802566	34.15%	4.168%
5	3.101	631	641	669	rVB	376513	784939	33.40%	4.076%
6	3.339	713	715	718	rBV2	690	283	0.01%	0.001%
7	3.378	723	727	731	rVB5	808	696	0.03%	0.004%
8	3.445	745	748	754	rBV6	1152	961	0.04%	0.005%
9	3.484	758	760	762	rBV2	469	215	0.01%	0.001%
10	3.539	775	777	779	rBV2	524	346	0.01%	0.002%
11	3.613	797	800	801	rBV	353	239	0.01%	0.001%
12	3.648	809	811	813	rBV2	591	272	0.01%	0.001%
13	3.690	820	824	827	rBV5	944	944	0.04%	0.005%
14	3.716	830	832	835	rVV2	453	275	0.01%	0.001%
15	3.748	840	842	846	rBV3	582	370	0.02%	0.002%
16	3.802	846	859	893	rBV2	453207	1201224	51.12%	6.238%
17	4.240	980	995	1029	rBV	379496	966708	41.14%	5.020%
18	4.503	1063	1077	1103	rVB2	246581	622711	26.50%	3.234%
19	4.670	1127	1129	1132	rBV2	676	489	0.02%	0.003%
20	4.732	1146	1148	1151	rBV3	523	241	0.01%	0.001%
21	4.789	1164	1166	1169	rVB	349	180	0.01%	0.001%
22	4.831	1177	1179	1180	rBV2	420	186	0.01%	0.001%
23	4.867	1187	1190	1193	rVB4	710	312	0.01%	0.002%
24	4.879	1193	1194	1196	rVB4	332	79	0.00%	0.000%
25	4.896	1196	1199	1200	rBV	894	463	0.02%	0.002%
26	4.947	1200	1215	1255	rBV2	920854	2349803	100.00%	12.203%
27	5.426	1360	1364	1365	rBV4	583	367	0.02%	0.002%
28	5.436	1365	1367	1368	rBV2	508	199	0.01%	0.001%
29	5.529	1385	1396	1435	rBV	656053	1367264	58.19%	7.100%
30	5.831	1479	1490	1504	rBV10	12548	30481	1.30%	0.158%
31	5.982	1525	1537	1573	rBV	518491	1069747	45.52%	5.555%
32	6.259	1620	1623	1627	rVB3	774	446	0.02%	0.002%
33	6.275	1627	1628	1632	rBV4	663	356	0.02%	0.002%
34	6.317	1639	1641	1643	rBV3	635	285	0.01%	0.001%
35	6.355	1651	1653	1655	rBV3	812	347	0.01%	0.002%
36	6.420	1672	1673	1676	rVB	446	186	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037610.D
 Acq On : 27 Sep 2024 16:41
 Operator : SY/MD
 Sample : P4184-05DL 10X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY033DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.436	1676	1678	1679	rBV3	341	117	0.00%	0.001%
38	6.455	1682	1684	1687	rBV3	662	350	0.01%	0.002%
39	6.468	1687	1688	1692	rBV3	796	433	0.02%	0.002%
40	6.577	1719	1722	1723	rVB2	394	139	0.01%	0.001%
41	6.613	1730	1733	1735	rBV2	747	397	0.02%	0.002%
42	6.641	1740	1742	1743	rBV2	515	251	0.01%	0.001%
43	6.680	1752	1754	1756	rBV2	388	170	0.01%	0.001%
44	6.693	1756	1758	1761	rVB3	756	281	0.01%	0.001%
45	6.722	1765	1767	1769	rBV2	736	430	0.02%	0.002%
46	6.844	1804	1805	1810	rVB3	683	355	0.02%	0.002%
47	6.867	1810	1812	1814	rBV2	729	363	0.02%	0.002%
48	6.908	1815	1825	1857	rBV	260025	506634	21.56%	2.631%
49	7.236	1916	1927	1955	rBV	1012676	1804140	76.78%	9.369%
50	7.551	2016	2025	2046	rBV	178642	329744	14.03%	1.712%
51	7.796	2098	2101	2103	rBV3	916	560	0.02%	0.003%
52	7.905	2126	2135	2147	rBV4	16205	30945	1.32%	0.161%
53	8.024	2164	2172	2207	rBV2	315644	668029	28.43%	3.469%
54	8.667	2369	2372	2374	rBV4	863	565	0.02%	0.003%
55	8.741	2393	2395	2396	rBV2	600	220	0.01%	0.001%
56	8.780	2396	2407	2432	rBV	1009744	1672466	71.17%	8.685%
57	9.281	2559	2563	2566	rBV3	734	664	0.03%	0.003%
58	9.329	2576	2578	2584	rVB4	953	815	0.03%	0.004%
59	9.355	2584	2586	2588	rBV	332	171	0.01%	0.001%
60	9.416	2600	2605	2607	rBV3	575	390	0.02%	0.002%
61	9.426	2607	2608	2609	rBV	189	50	0.00%	0.000%
62	9.436	2609	2611	2612	rBV	919	395	0.02%	0.002%
63	9.484	2620	2626	2637	rBV4	6099	10513	0.45%	0.055%
64	9.564	2648	2651	2652	rBV3	529	300	0.01%	0.002%
65	9.699	2687	2693	2696	rBV3	416	510	0.02%	0.003%
66	9.728	2697	2702	2704	rBV5	643	553	0.02%	0.003%
67	9.770	2713	2715	2716	rBV	471	171	0.01%	0.001%
68	9.809	2723	2727	2728	rBV3	590	457	0.02%	0.002%
69	9.818	2728	2730	2732	rVV2	521	294	0.01%	0.002%
70	9.870	2740	2746	2747	rBV5	1679	1353	0.06%	0.007%
71	9.934	2762	2766	2770	rBV4	711	595	0.03%	0.003%
72	9.969	2773	2777	2779	rVV3	475	273	0.01%	0.001%
73	9.995	2783	2785	2786	rBV	309	135	0.01%	0.001%
74	10.063	2802	2806	2810	rVB5	845	621	0.03%	0.003%
75	10.098	2816	2817	2819	rVB	403	123	0.01%	0.001%
76	10.146	2819	2832	2856	rBV	616801	978833	41.66%	5.083%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037610.D
 Acq On : 27 Sep 2024 16:41
 Operator : SY/MD
 Sample : P4184-05DL 10X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY033DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.554	2956	2959	2962	rBV4	516	386	0.02%	0.002%
78	10.677	2990	2997	3007	rBV3	6480	11048	0.47%	0.057%
79	10.760	3021	3023	3025	rBV	399	208	0.01%	0.001%
80	10.773	3025	3027	3028	rBV2	498	234	0.01%	0.001%
81	10.780	3028	3029	3032	rBV3	808	505	0.02%	0.003%
82	10.853	3043	3052	3064	rBV2	15537	26938	1.15%	0.140%
83	10.950	3077	3082	3085	rBV5	933	701	0.03%	0.004%
84	10.963	3085	3086	3087	rBV	320	110	0.00%	0.001%
85	11.069	3116	3119	3121	rBV	636	348	0.01%	0.002%
86	11.178	3142	3153	3176	rBV	985365	1556893	66.26%	8.085%
87	11.554	3259	3270	3304	rVB	1031606	1651588	70.29%	8.577%
88	12.149	3453	3455	3458	rBV3	520	185	0.01%	0.001%
89	12.345	3514	3516	3519	rBV3	850	516	0.02%	0.003%
90	12.500	3561	3564	3567	rBV3	696	643	0.03%	0.003%
91	12.728	3633	3635	3639	rBV3	762	632	0.03%	0.003%
92	12.776	3647	3650	3654	rBV2	1121	1110	0.05%	0.006%
93	13.394	3839	3842	3847	rVB5	902	986	0.04%	0.005%
94	13.429	3847	3853	3855	rBV4	1053	1023	0.04%	0.005%
95	13.564	3891	3895	3900	rBV3	976	765	0.03%	0.004%
96	13.747	3950	3952	3955	rBV3	693	279	0.01%	0.001%
97	14.111	4062	4065	4069	rBV4	1245	1073	0.05%	0.006%
98	14.185	4086	4088	4091	rBV3	1010	744	0.03%	0.004%

Sum of corrected areas: 19256454




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037610.D
Acq On : 27 Sep 2024 16:41
Operator : SY/MD
Sample : P4184-05DL 10X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY033DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

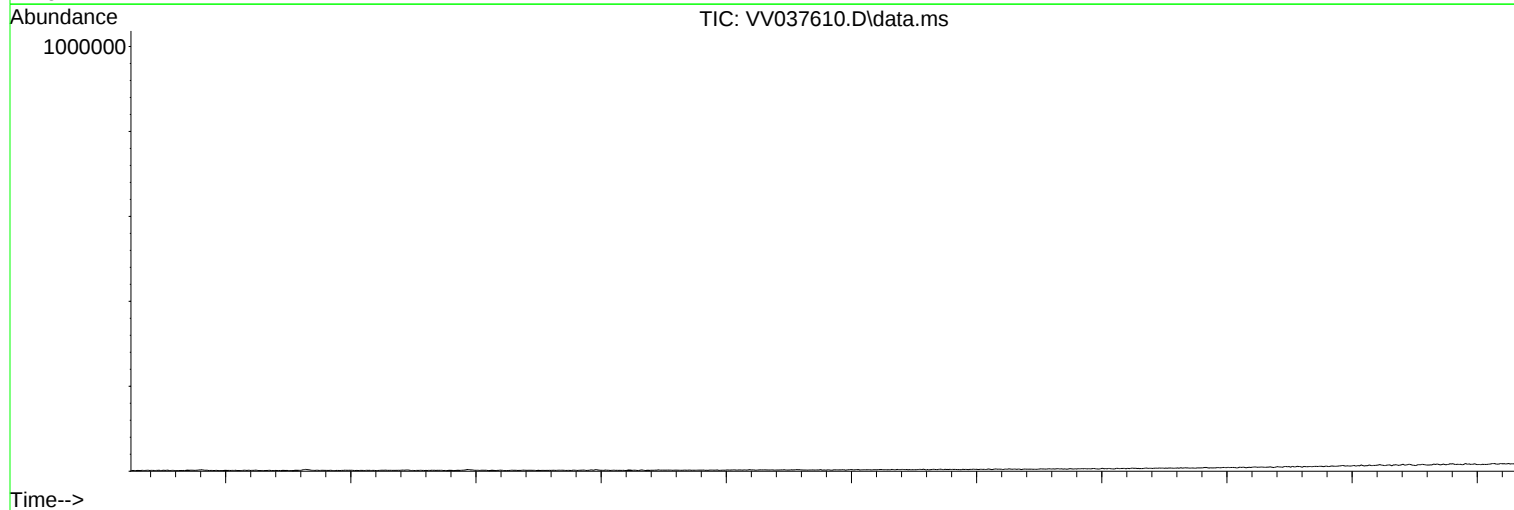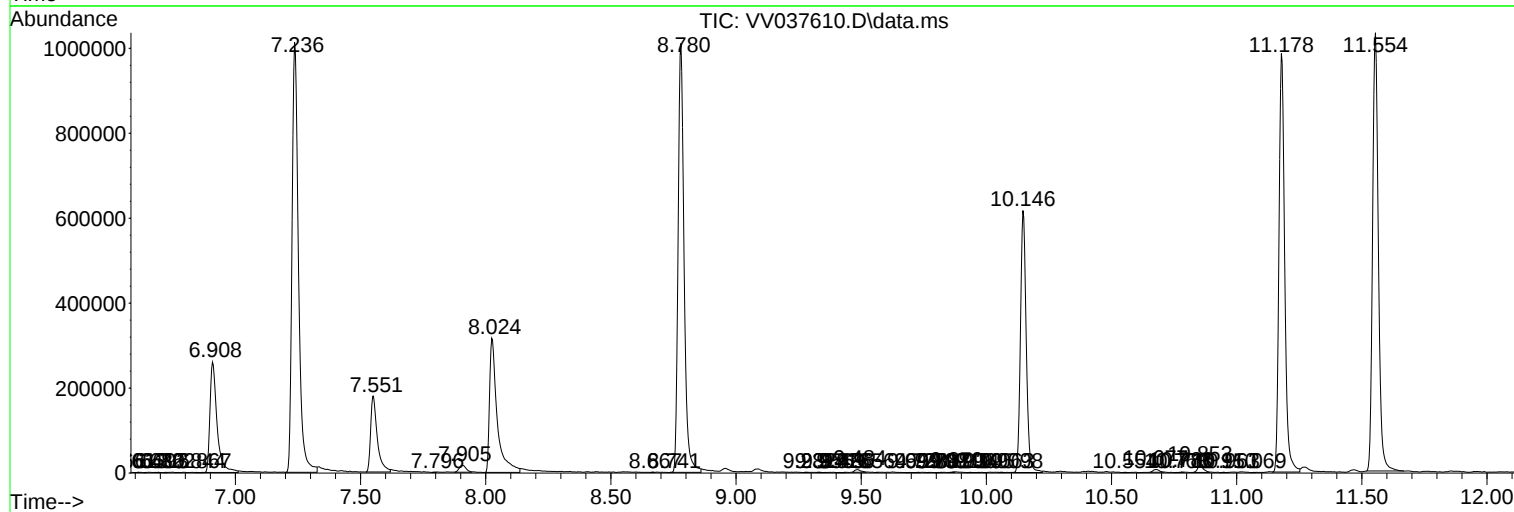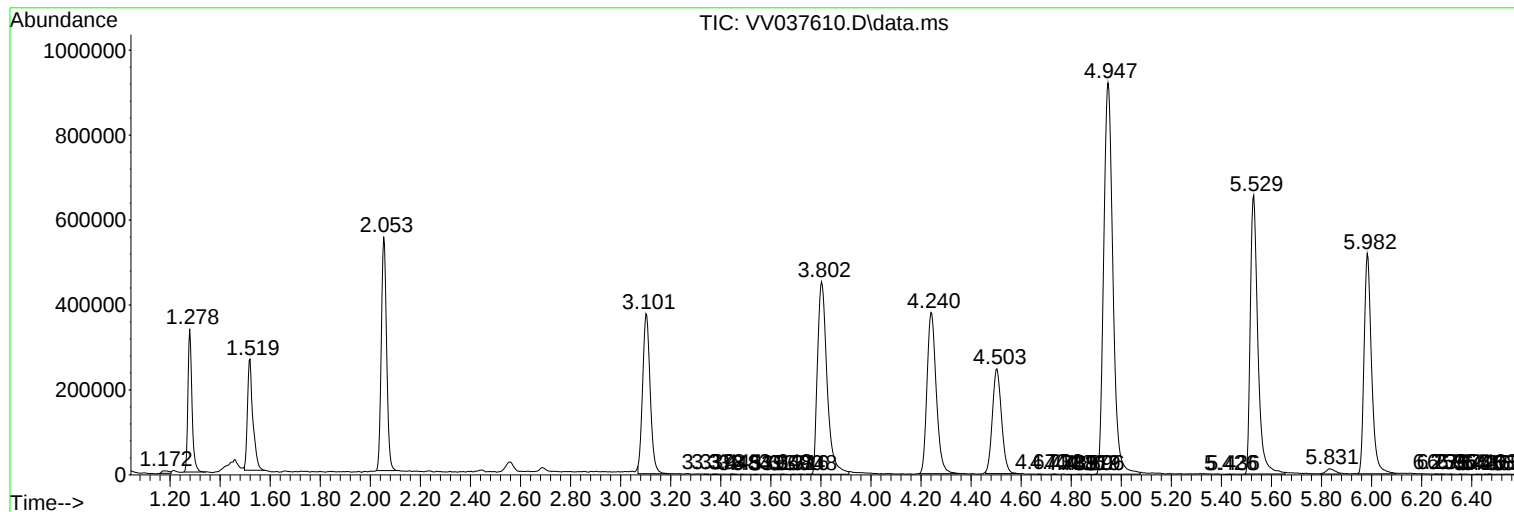

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037610.D
Acq On : 27 Sep 2024 16:41
Operator : SY/MD
Sample : P4184-05DL 10X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY033DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037610.D
Acq On : 27 Sep 2024 16:41
Operator : SY/MD
Sample : P4184-05DL 10X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY033DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------