

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037612.D
 Acq On : 27 Sep 2024 17:25
 Operator : SY/MD
 Sample : P4184-15DL 40X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY041DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037612.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rBV	324789	354719	15.29%	1.972%
2	1.519	142	149	166	rVB	256819	326026	14.05%	1.812%
3	2.053	306	315	333	rBV	557272	808475	34.84%	4.493%
4	3.397	731	733	736	rVB3	818	402	0.02%	0.002%
5	3.539	776	777	779	rBV2	594	294	0.01%	0.002%
6	3.712	826	831	834	rVB3	993	821	0.04%	0.005%
7	3.732	834	837	839	rBV2	724	489	0.02%	0.003%
8	3.802	846	859	904	rBV2	392494	1057026	45.56%	5.875%
9	4.240	979	995	1026	rBV	379481	964611	41.57%	5.361%
10	4.503	1060	1077	1100	rBV3	92185	235121	10.13%	1.307%
11	4.690	1133	1135	1140	rBV4	540	430	0.02%	0.002%
12	4.802	1168	1170	1173	rBV2	526	355	0.02%	0.002%
13	4.847	1182	1184	1186	rVB2	457	165	0.01%	0.001%
14	4.947	1199	1215	1243	rBV2	917062	2320276	100.00%	12.896%
15	5.166	1281	1283	1287	rVB3	1332	771	0.03%	0.004%
16	5.529	1385	1396	1429	rBV	681703	1415256	61.00%	7.866%
17	5.773	1469	1472	1476	rBV5	1568	1383	0.06%	0.008%
18	5.982	1526	1537	1569	rBV	506113	1043128	44.96%	5.798%
19	6.310	1637	1639	1640	rBV	665	218	0.01%	0.001%
20	6.342	1647	1649	1652	rBV4	908	507	0.02%	0.003%
21	6.375	1657	1659	1661	rBV3	638	278	0.01%	0.002%
22	6.416	1670	1672	1674	rBV3	885	504	0.02%	0.003%
23	6.458	1684	1685	1688	rVB2	439	187	0.01%	0.001%
24	6.516	1701	1703	1705	rBV3	572	253	0.01%	0.001%
25	6.580	1720	1723	1724	rVB2	960	424	0.02%	0.002%
26	6.590	1724	1726	1733	rVV6	755	696	0.03%	0.004%
27	6.619	1733	1735	1737	rVV3	536	296	0.01%	0.002%
28	6.645	1741	1743	1746	rBV3	280	139	0.01%	0.001%
29	6.677	1748	1753	1758	rVB4	1063	1139	0.05%	0.006%
30	6.719	1763	1766	1768	rBV3	667	355	0.02%	0.002%
31	6.728	1768	1769	1771	rBV3	407	164	0.01%	0.001%
32	6.738	1771	1772	1775	rVB	397	176	0.01%	0.001%
33	6.776	1781	1784	1788	rVB3	745	496	0.02%	0.003%
34	6.796	1788	1790	1794	rVB3	521	386	0.02%	0.002%
35	6.828	1799	1800	1805	rVB2	277	156	0.01%	0.001%
36	6.847	1805	1806	1807	rVB2	185	36	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037612.D
 Acq On : 27 Sep 2024 17:25
 Operator : SY/MD
 Sample : P4184-15DL 40X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY041DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.860	1807	1810	1813	rBV2	571	463	0.02%	0.003%
38	6.908	1815	1825	1852	rBV	261409	500302	21.56%	2.781%
39	7.236	1916	1927	1962	rBV	1019485	1834194	79.05%	10.194%
40	7.551	2015	2025	2047	rBV	170620	329920	14.22%	1.834%
41	7.854	2117	2119	2121	rBV3	1178	471	0.02%	0.003%
42	7.982	2151	2159	2162	rBV5	1083	1353	0.06%	0.008%
43	8.024	2164	2172	2210	rBV2	320152	682267	29.40%	3.792%
44	8.506	2320	2322	2324	rBV2	1072	397	0.02%	0.002%
45	8.632	2358	2361	2363	rBV3	658	299	0.01%	0.002%
46	8.725	2385	2390	2392	rBV5	751	769	0.03%	0.004%
47	8.780	2395	2407	2430	rBV	1079636	1763325	76.00%	9.801%
48	9.410	2601	2603	2606	rVB4	721	325	0.01%	0.002%
49	9.442	2610	2613	2615	rBV3	443	267	0.01%	0.001%
50	9.490	2624	2628	2635	rBV6	1565	1929	0.08%	0.011%
51	9.545	2642	2645	2648	rBV4	859	579	0.02%	0.003%
52	9.628	2669	2671	2672	rBV2	824	389	0.02%	0.002%
53	9.686	2686	2689	2690	rBV2	304	142	0.01%	0.001%
54	9.696	2690	2692	2694	rVV3	747	438	0.02%	0.002%
55	9.722	2697	2700	2705	rBV3	833	710	0.03%	0.004%
56	9.844	2735	2738	2740	rVB3	817	381	0.02%	0.002%
57	9.870	2740	2746	2747	rBV4	607	504	0.02%	0.003%
58	9.960	2772	2774	2777	rBV2	580	385	0.02%	0.002%
59	9.998	2783	2786	2790	rVB4	576	424	0.02%	0.002%
60	10.037	2796	2798	2799	rBV	560	226	0.01%	0.001%
61	10.056	2802	2804	2806	rVV3	631	267	0.01%	0.001%
62	10.146	2820	2832	2855	rBV	620820	986120	42.50%	5.481%
63	10.436	2920	2922	2923	rBV2	616	272	0.01%	0.002%
64	10.606	2971	2975	2979	rBV3	932	839	0.04%	0.005%
65	10.657	2988	2991	2994	rBV3	618	465	0.02%	0.003%
66	10.731	3012	3014	3017	rBV2	515	236	0.01%	0.001%
67	10.767	3021	3025	3027	rBV3	861	615	0.03%	0.003%
68	10.860	3048	3054	3055	rBV5	2255	1776	0.08%	0.010%
69	10.966	3085	3087	3089	rBV2	302	149	0.01%	0.001%
70	11.034	3105	3108	3109	rBV	620	293	0.01%	0.002%
71	11.082	3119	3123	3127	rBV3	999	653	0.03%	0.004%
72	11.104	3127	3130	3131	rBV2	442	183	0.01%	0.001%
73	11.133	3137	3139	3140	rBV	665	278	0.01%	0.002%
74	11.178	3143	3153	3179	rVV	1057004	1653355	71.26%	9.189%
75	11.554	3258	3270	3301	rBV	1050982	1684598	72.60%	9.363%
76	12.082	3428	3434	3435	rBV3	814	673	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037612.D
 Acq On : 27 Sep 2024 17:25
 Operator : SY/MD
 Sample : P4184-15DL 40X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY041DL

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.181	3461	3465	3467	rBV3	875	609	0.03%	0.003%
78	12.297	3498	3501	3504	rVB3	910	572	0.02%	0.003%
79	12.497	3559	3563	3565	rBV2	818	583	0.03%	0.003%
80	12.570	3584	3586	3590	rBV3	545	347	0.01%	0.002%
81	12.628	3602	3604	3606	rBV2	479	169	0.01%	0.001%
82	12.657	3612	3613	3615	rBV	322	137	0.01%	0.001%
83	12.828	3662	3666	3670	rBV4	1143	1238	0.05%	0.007%
84	13.693	3933	3935	3938	rBV2	806	504	0.02%	0.003%
85	14.554	4200	4203	4204	rBV2	1099	637	0.03%	0.004%




Sum of corrected areas: 17992185

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037612.D
Acq On : 27 Sep 2024 17:25
Operator : SY/MD
Sample : P4184-15DL 40X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY041DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

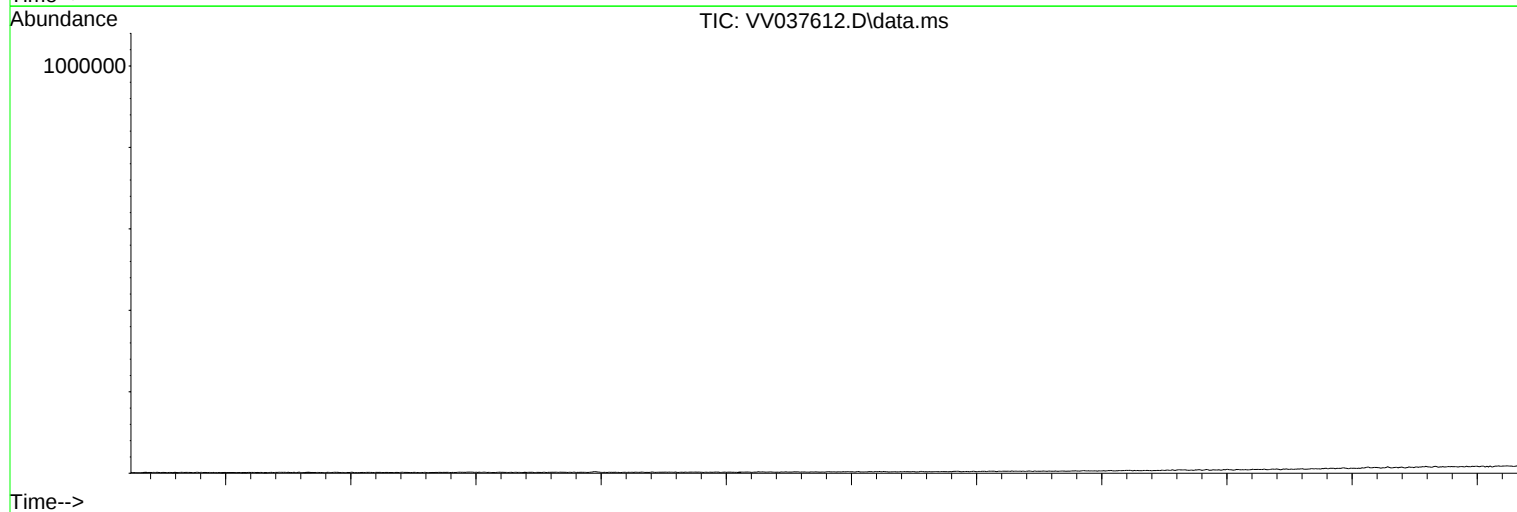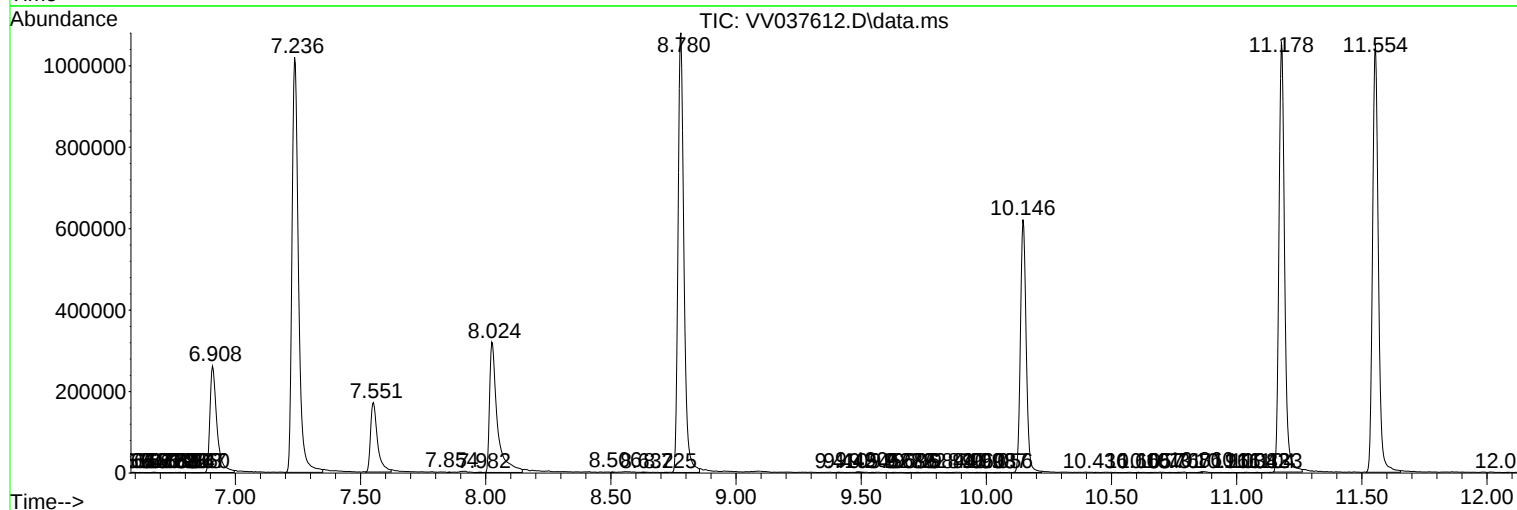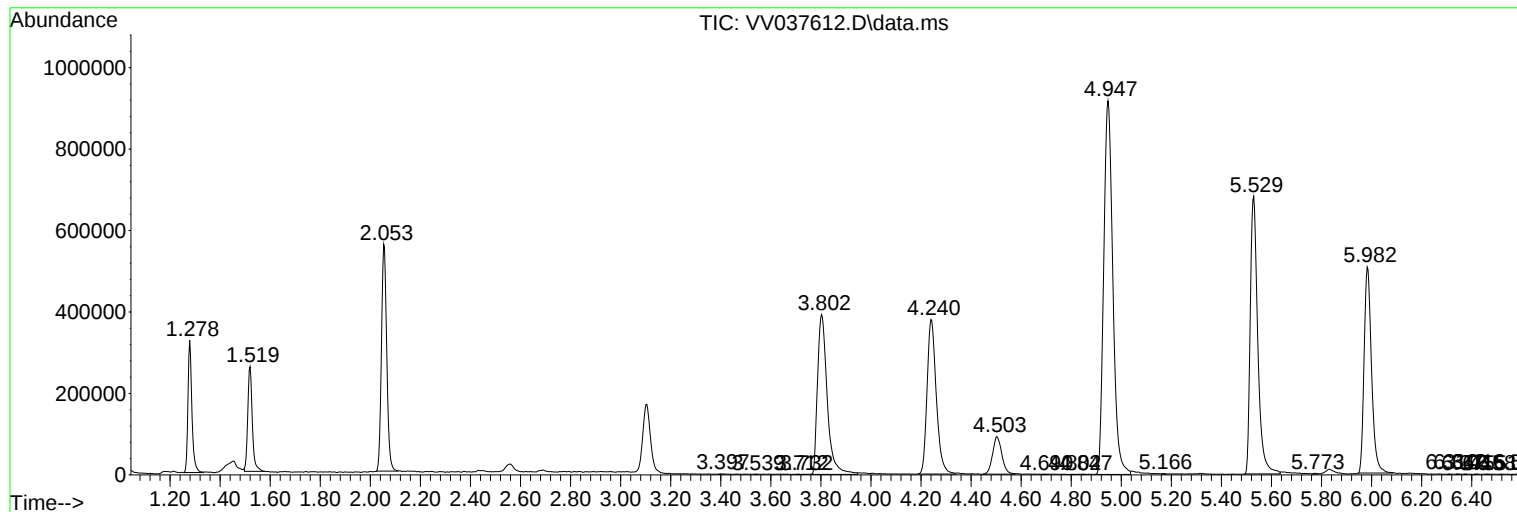

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037612.D
Acq On : 27 Sep 2024 17:25
Operator : SY/MD
Sample : P4184-15DL 40X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY041DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037612.D
Acq On : 27 Sep 2024 17:25
Operator : SY/MD
Sample : P4184-15DL 40X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY041DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc