

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037617.D
 Acq On : 27 Sep 2024 19:34
 Operator : SY/MD
 Sample : VV0927WBL02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK219

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037617.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	311713	336751	12.83%	1.785%
2	1.532	145	153	169	rVB	280275	330635	12.60%	1.752%
3	2.060	308	317	337	rVB	581532	835128	31.83%	4.426%
4	3.417	736	739	742	rVB3	1214	804	0.03%	0.004%
5	3.494	759	763	764	rBV	565	357	0.01%	0.002%
6	3.552	776	781	784	rBV3	967	836	0.03%	0.004%
7	3.638	805	808	811	rVB3	884	592	0.02%	0.003%
8	3.654	811	813	816	rBV2	551	393	0.01%	0.002%
9	3.690	822	824	827	rBV3	375	187	0.01%	0.001%
10	3.738	835	839	841	rBV4	959	763	0.03%	0.004%
11	3.793	848	856	892	rBV	122416	367456	14.00%	1.948%
12	4.243	980	996	1029	rBV	428024	1091150	41.59%	5.783%
13	4.494	1072	1074	1080	rBV6	1069	877	0.03%	0.005%
14	4.558	1091	1094	1099	rBV4	1111	1215	0.05%	0.006%
15	4.616	1107	1112	1114	rBV3	1049	1057	0.04%	0.006%
16	4.645	1119	1121	1125	rBV4	515	440	0.02%	0.002%
17	4.716	1138	1143	1144	rBV3	728	486	0.02%	0.003%
18	4.796	1163	1168	1170	rBV2	846	711	0.03%	0.004%
19	4.815	1173	1174	1179	rVV2	715	424	0.02%	0.002%
20	4.838	1179	1181	1183	rVV	469	204	0.01%	0.001%
21	4.857	1185	1187	1188	rVV2	386	105	0.00%	0.001%
22	4.950	1199	1216	1262	rBV2	1030599	2623869	100.00%	13.907%
23	5.452	1367	1372	1373	rBV3	877	696	0.03%	0.004%
24	5.474	1377	1379	1383	rBV3	557	382	0.01%	0.002%
25	5.529	1385	1396	1431	rBV	714963	1475497	56.23%	7.820%
26	5.982	1525	1537	1571	rBV	579793	1216798	46.37%	6.449%
27	6.269	1624	1626	1628	rBV2	880	468	0.02%	0.002%
28	6.301	1634	1636	1638	rBV2	807	504	0.02%	0.003%
29	6.330	1641	1645	1647	rBV3	1223	873	0.03%	0.005%
30	6.404	1664	1668	1672	rBV4	662	566	0.02%	0.003%
31	6.526	1703	1706	1707	rBV	572	358	0.01%	0.002%
32	6.625	1733	1737	1743	rBV6	643	675	0.03%	0.004%
33	6.677	1748	1753	1754	rBV2	820	512	0.02%	0.003%
34	6.719	1762	1766	1770	rBV2	737	553	0.02%	0.003%
35	6.744	1770	1774	1776	rVV3	780	475	0.02%	0.003%
36	6.770	1780	1782	1786	rBV3	661	456	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037617.D
 Acq On : 27 Sep 2024 19:34
 Operator : SY/MD
 Sample : VV0927WBL02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK219

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.793	1786	1789	1791	rVB2	859	401	0.02%	0.002%
38	6.822	1795	1798	1802	rVB3	1138	720	0.03%	0.004%
39	6.850	1802	1807	1809	rBV2	698	638	0.02%	0.003%
40	6.908	1815	1825	1855	rBV	301425	580962	22.14%	3.079%
41	7.127	1891	1893	1896	rBV3	824	453	0.02%	0.002%
42	7.236	1917	1927	1957	rBV	1169439	2069197	78.86%	10.967%
43	7.548	2015	2024	2057	rBV	208210	393644	15.00%	2.086%
44	7.960	2150	2152	2154	rBV2	879	581	0.02%	0.003%
45	8.024	2164	2172	2212	rBV2	355493	773900	29.49%	4.102%
46	8.645	2362	2365	2367	rBV3	909	667	0.03%	0.004%
47	8.780	2396	2407	2443	rBV	1111097	1854787	70.69%	9.830%
48	9.378	2592	2593	2594	rBV	449	136	0.01%	0.001%
49	9.432	2607	2610	2611	rBV	608	311	0.01%	0.002%
50	9.648	2673	2677	2678	rBV2	734	464	0.02%	0.002%
51	9.680	2684	2687	2691	rVB4	604	368	0.01%	0.002%
52	9.709	2694	2696	2698	rBV2	543	269	0.01%	0.001%
53	9.764	2709	2713	2716	rBV3	463	396	0.02%	0.002%
54	9.809	2723	2727	2728	rBV	664	430	0.02%	0.002%
55	9.825	2731	2732	2734	rVB	487	160	0.01%	0.001%
56	9.860	2739	2743	2744	rBV2	745	563	0.02%	0.003%
57	9.924	2759	2763	2764	rBV3	486	383	0.01%	0.002%
58	9.969	2775	2777	2782	rVB4	619	499	0.02%	0.003%
59	9.998	2782	2786	2788	rBV2	590	447	0.02%	0.002%
60	10.011	2788	2790	2791	rBV	234	98	0.00%	0.001%
61	10.034	2791	2797	2799	rBV5	639	602	0.02%	0.003%
62	10.092	2811	2815	2817	rBV2	703	488	0.02%	0.003%
63	10.146	2820	2832	2859	rBV	714717	1141238	43.49%	6.049%
64	10.535	2950	2953	2954	rBV3	607	322	0.01%	0.002%
65	10.580	2963	2967	2969	rBV4	823	545	0.02%	0.003%
66	10.625	2979	2981	2983	rVB3	438	147	0.01%	0.001%
67	10.645	2983	2987	2991	rBV5	714	590	0.02%	0.003%
68	10.664	2991	2993	2999	rBV5	641	644	0.02%	0.003%
69	10.722	3005	3011	3017	rBV5	657	895	0.03%	0.005%
70	10.764	3021	3024	3027	rVB3	803	459	0.02%	0.002%
71	10.780	3027	3029	3031	rBV3	733	433	0.02%	0.002%
72	10.837	3046	3047	3049	rBV	350	161	0.01%	0.001%
73	10.863	3049	3055	3056	rBV4	1921	1816	0.07%	0.010%
74	10.956	3082	3084	3087	rVB2	998	461	0.02%	0.002%
75	10.989	3087	3094	3096	rBV4	951	1090	0.04%	0.006%
76	11.079	3120	3122	3123	rBV	608	246	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037617.D
 Acq On : 27 Sep 2024 19:34
 Operator : SY/MD
 Sample : VV0927WBL02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK219

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	11.178	3143	3153	3186	rBV	1083413	1725533	65.76%	9.145%
78	11.554	3258	3270	3299	rBV	1238322	1978197	75.39%	10.485%
79	11.866	3365	3367	3369	rBV2	599	301	0.01%	0.002%
80	11.982	3402	3403	3405	rVB	781	217	0.01%	0.001%
81	12.011	3409	3412	3417	rBV3	709	721	0.03%	0.004%
82	12.108	3440	3442	3443	rBV	632	248	0.01%	0.001%
83	12.525	3568	3572	3574	rBV2	1353	891	0.03%	0.005%
84	12.648	3607	3610	3612	rBV4	932	473	0.02%	0.003%
85	12.706	3625	3628	3631	rBV4	522	323	0.01%	0.002%
86	12.786	3650	3653	3656	rVB3	1300	638	0.02%	0.003%
87	12.834	3664	3668	3670	rBV	705	476	0.02%	0.003%
88	12.850	3670	3673	3677	rVB4	536	390	0.01%	0.002%
89	12.873	3677	3680	3683	rBV4	1045	680	0.03%	0.004%
90	13.323	3818	3820	3822	rBV2	680	355	0.01%	0.002%
91	13.448	3851	3859	3870	rBV4	10615	20241	0.77%	0.107%
92	13.683	3924	3932	3947	rVB8	7044	13783	0.53%	0.073%
93	14.371	4144	4146	4149	rBV2	1000	400	0.02%	0.002%




Sum of corrected areas: 18867731

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037617.D
Acq On : 27 Sep 2024 19:34
Operator : SY/MD
Sample : VV0927WBL02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK219

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

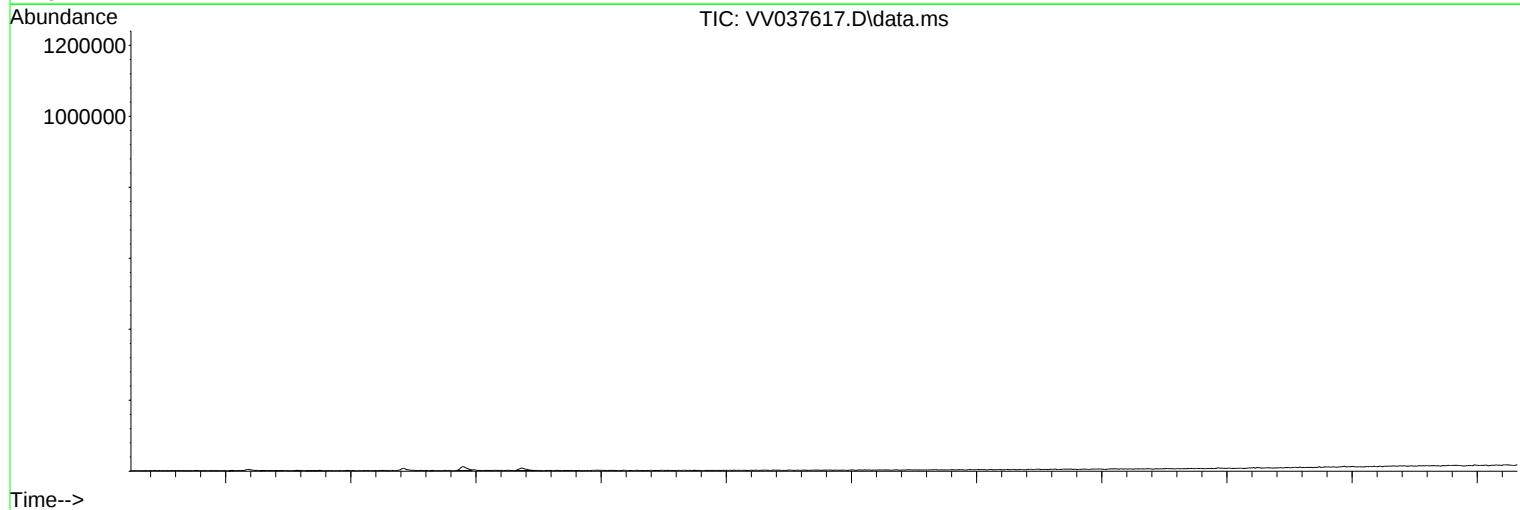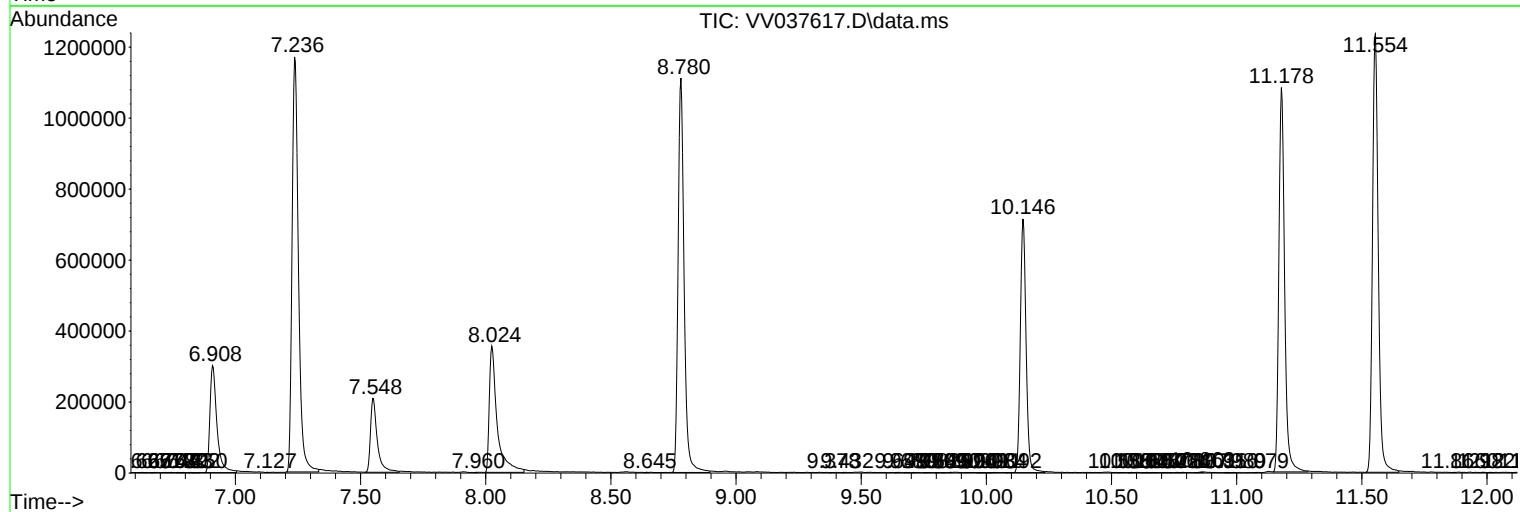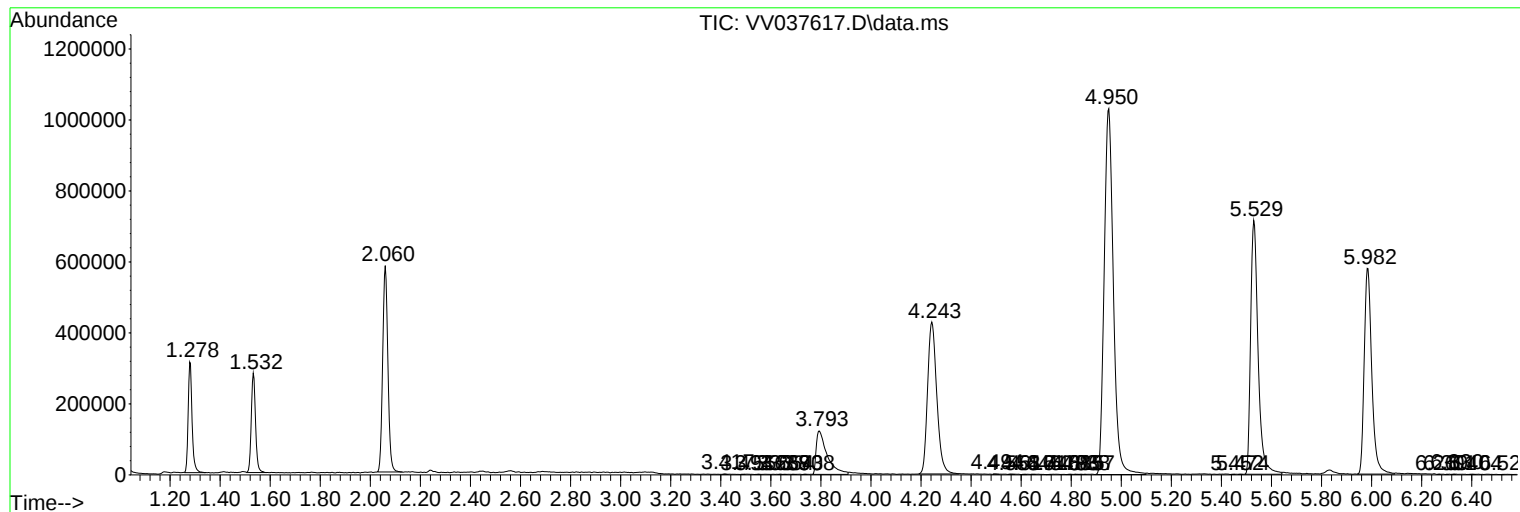

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037617.D
Acq On : 27 Sep 2024 19:34
Operator : SY/MD
Sample : VV0927WBL02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK219

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037617.D
Acq On : 27 Sep 2024 19:34
Operator : SY/MD
Sample : VV0927WBL02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK219

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc