

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037620.D
 Acq On : 27 Sep 2024 20:39
 Operator : SY/MD
 Sample : P4184-20DL 5X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY046DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037620.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	36	41	45	rBV2	8410	10299	0.44%	0.053%
2	1.278	67	74	91	rBV	299184	331922	14.29%	1.701%
3	1.516	141	148	165	rVB	255004	323354	13.92%	1.658%
4	2.057	306	316	336	rVB3	654421	1059515	45.62%	5.431%
5	3.102	632	641	661	rVB	174784	361500	15.56%	1.853%
6	3.481	754	759	760	rBV4	732	618	0.03%	0.003%
7	3.529	770	774	778	rBV5	867	750	0.03%	0.004%
8	3.593	792	794	796	rVB3	710	268	0.01%	0.001%
9	3.606	796	798	799	rBV	493	178	0.01%	0.001%
10	3.719	832	833	836	rBV2	377	184	0.01%	0.001%
11	3.799	847	858	890	rBV3	163927	490198	21.10%	2.513%
12	4.240	979	995	1023	rBV	376852	964610	41.53%	4.945%
13	4.503	1058	1077	1106	rBV	485936	1250286	53.83%	6.409%
14	4.809	1170	1172	1173	rBV3	840	368	0.02%	0.002%
15	4.831	1178	1179	1183	rBV4	470	311	0.01%	0.002%
16	4.947	1199	1215	1254	rBV2	911989	2322711	100.00%	11.906%
17	5.445	1365	1370	1374	rBV5	789	767	0.03%	0.004%
18	5.484	1378	1382	1384	rBV3	914	666	0.03%	0.003%
19	5.526	1384	1395	1430	rBV	666620	1405685	60.52%	7.206%
20	5.831	1479	1490	1516	rBV3	94492	216186	9.31%	1.108%
21	5.982	1526	1537	1568	rBV	509178	1040852	44.81%	5.335%
22	6.310	1637	1639	1641	rBV3	856	369	0.02%	0.002%
23	6.330	1642	1645	1650	rVB5	874	561	0.02%	0.003%
24	6.433	1676	1677	1680	rVB2	805	336	0.01%	0.002%
25	6.535	1703	1709	1716	rVB7	952	1306	0.06%	0.007%
26	6.564	1716	1718	1722	rBV3	491	449	0.02%	0.002%
27	6.590	1724	1726	1727	rBV	228	81	0.00%	0.000%
28	6.619	1731	1735	1737	rBV4	826	673	0.03%	0.003%
29	6.654	1745	1746	1750	rVB2	547	250	0.01%	0.001%
30	6.674	1750	1752	1753	rBV	351	161	0.01%	0.001%
31	6.738	1770	1772	1773	rBV	571	219	0.01%	0.001%
32	6.822	1796	1798	1801	rVB2	677	293	0.01%	0.002%
33	6.841	1801	1804	1809	rVB4	334	225	0.01%	0.001%
34	6.867	1809	1812	1815	rBV2	846	561	0.02%	0.003%
35	6.908	1815	1825	1853	rBV	257822	491971	21.18%	2.522%
36	7.236	1916	1927	1954	rBV	1018260	1814699	78.13%	9.302%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037620.D
 Acq On : 27 Sep 2024 20:39
 Operator : SY/MD
 Sample : P4184-20DL 5X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY046DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.548	2016	2024	2046	rBV	169548	318643	13.72%	1.633%
38	7.899	2122	2133	2162	rBV	209741	368755	15.88%	1.890%
39	8.024	2164	2172	2212	rBV	300110	636054	27.38%	3.260%
40	8.600	2349	2351	2356	rBV3	1038	681	0.03%	0.003%
41	8.696	2378	2381	2382	rBV2	707	407	0.02%	0.002%
42	8.780	2396	2407	2444	rBV	1044783	1748938	75.30%	8.965%
43	9.214	2540	2542	2543	rBV2	581	207	0.01%	0.001%
44	9.249	2552	2553	2555	rBV	403	150	0.01%	0.001%
45	9.336	2578	2580	2584	rBV3	812	665	0.03%	0.003%
46	9.436	2609	2611	2613	rVB3	557	223	0.01%	0.001%
47	9.455	2614	2617	2619	rVB2	854	491	0.02%	0.003%
48	9.593	2657	2660	2662	rBV2	1009	640	0.03%	0.003%
49	9.635	2669	2673	2675	rBV4	505	384	0.02%	0.002%
50	9.670	2682	2684	2686	rBV	502	224	0.01%	0.001%
51	9.680	2686	2687	2690	rVV2	298	186	0.01%	0.001%
52	9.696	2690	2692	2695	rVB3	558	318	0.01%	0.002%
53	9.712	2695	2697	2700	rBV2	321	213	0.01%	0.001%
54	9.760	2705	2712	2717	rBV5	977	1312	0.06%	0.007%
55	9.799	2722	2724	2725	rBV5	167	84	0.00%	0.000%
56	9.809	2725	2727	2729	rVB2	380	138	0.01%	0.001%
57	9.831	2729	2734	2736	rBV3	521	548	0.02%	0.003%
58	9.857	2738	2742	2744	rBV4	677	539	0.02%	0.003%
59	9.889	2750	2752	2755	rBV2	198	104	0.00%	0.001%
60	9.912	2755	2759	2764	rBV4	710	614	0.03%	0.003%
61	9.934	2764	2766	2768	rBV	476	267	0.01%	0.001%
62	9.989	2780	2783	2787	rBV5	833	615	0.03%	0.003%
63	10.024	2791	2794	2796	rVB4	431	249	0.01%	0.001%
64	10.050	2800	2802	2804	rVB2	496	225	0.01%	0.001%
65	10.063	2804	2806	2809	rBV3	639	327	0.01%	0.002%
66	10.079	2809	2811	2813	rBV2	389	219	0.01%	0.001%
67	10.146	2820	2832	2857	rBV	621312	970518	41.78%	4.975%
68	10.436	2920	2922	2925	rVB3	756	261	0.01%	0.001%
69	10.458	2925	2929	2931	rBV4	914	533	0.02%	0.003%
70	10.474	2932	2934	2937	rVV4	591	231	0.01%	0.001%
71	10.497	2940	2941	2943	rBV	501	240	0.01%	0.001%
72	10.555	2957	2959	2961	rVB	623	263	0.01%	0.001%
73	10.574	2962	2965	2967	rVB3	793	377	0.02%	0.002%
74	10.603	2973	2974	2978	rVB3	677	370	0.02%	0.002%
75	10.651	2987	2989	2990	rBV2	290	124	0.01%	0.001%
76	10.693	2996	3002	3006	rVB4	751	627	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037620.D
 Acq On : 27 Sep 2024 20:39
 Operator : SY/MD
 Sample : P4184-20DL 5X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY046DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.719	3006	3010	3015	rBV4	1005	907	0.04%	0.005%
78	10.754	3018	3021	3025	rVB2	938	569	0.02%	0.003%
79	10.780	3026	3029	3032	rBV4	829	610	0.03%	0.003%
80	10.818	3038	3041	3042	rBV2	1050	557	0.02%	0.003%
81	10.866	3053	3056	3061	rBV4	1107	1108	0.05%	0.006%
82	11.088	3124	3125	3127	rBV2	217	103	0.00%	0.001%
83	11.117	3128	3134	3136	rBV4	865	821	0.04%	0.004%
84	11.178	3142	3153	3185	rBV	1033305	1647177	70.92%	8.443%
85	11.555	3258	3270	3298	rBV	1060013	1700235	73.20%	8.715%
86	11.937	3387	3389	3392	rBV3	942	564	0.02%	0.003%
87	11.998	3405	3408	3413	rBV6	990	938	0.04%	0.005%
88	12.252	3485	3487	3489	rBV	362	198	0.01%	0.001%
89	12.265	3489	3491	3492	rBV	741	352	0.02%	0.002%
90	12.326	3508	3510	3512	rBV2	560	326	0.01%	0.002%
91	12.587	3589	3591	3593	rBV3	947	518	0.02%	0.003%
92	12.667	3613	3616	3617	rBV2	709	405	0.02%	0.002%
93	12.799	3655	3657	3660	rBV2	432	289	0.01%	0.001%
94	13.037	3728	3731	3735	rBV3	738	506	0.02%	0.003%
95	13.127	3757	3759	3762	rBV2	830	403	0.02%	0.002%
96	13.149	3762	3766	3767	rBV2	540	321	0.01%	0.002%
97	13.217	3784	3787	3788	rBV2	1513	904	0.04%	0.005%
98	13.390	3838	3841	3844	rBV3	755	544	0.02%	0.003%
99	14.230	4099	4102	4104	rBV4	1031	658	0.03%	0.003%

Sum of corrected areas: 19508359




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037620.D
Acq On : 27 Sep 2024 20:39
Operator : SY/MD
Sample : P4184-20DL 5X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY046DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

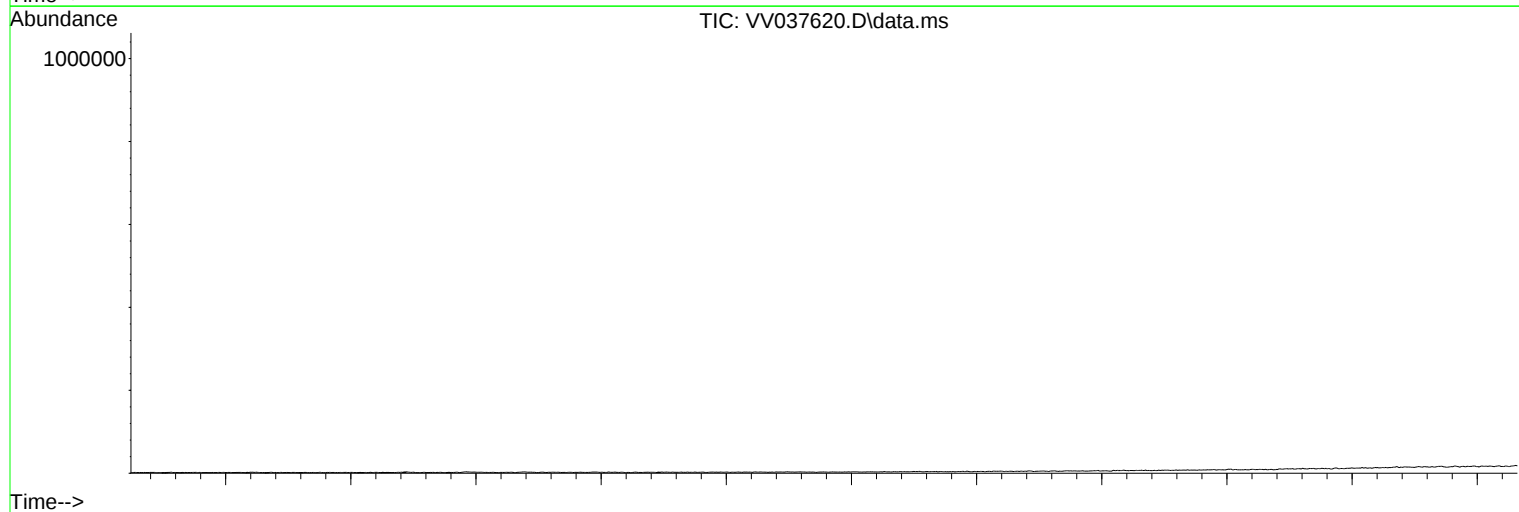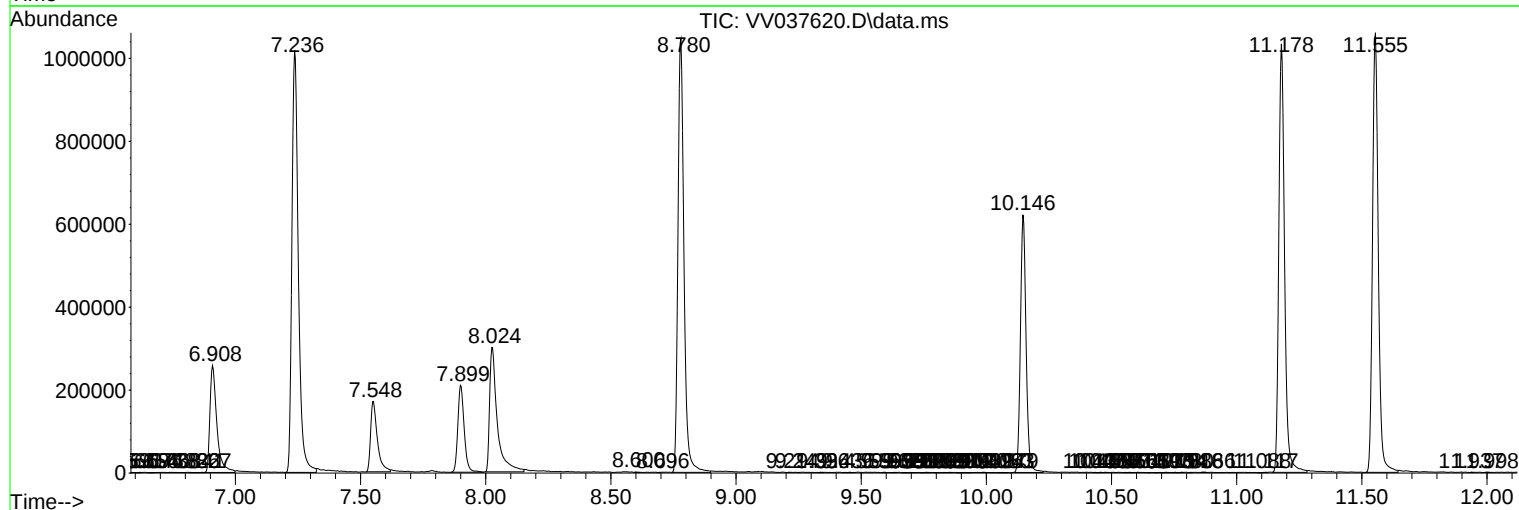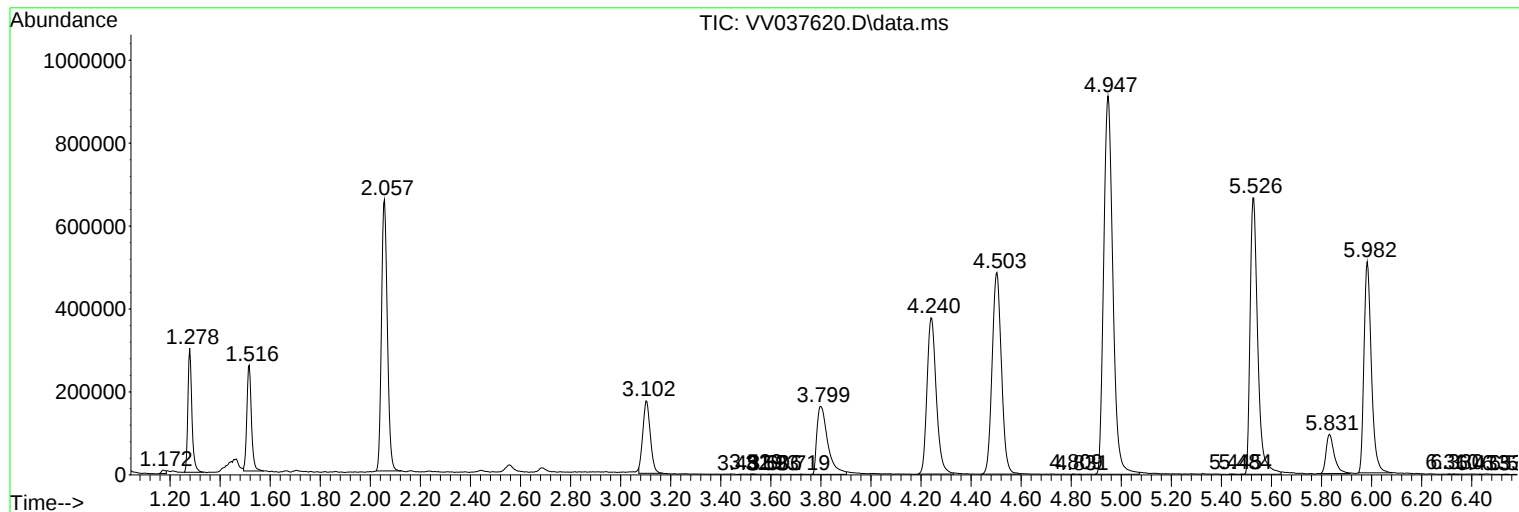

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037620.D
Acq On : 27 Sep 2024 20:39
Operator : SY/MD
Sample : P4184-20DL 5X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY046DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037620.D
Acq On : 27 Sep 2024 20:39
Operator : SY/MD
Sample : P4184-20DL 5X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY046DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------