

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037625.D
 Acq On : 27 Sep 2024 22:27
 Operator : SY/MD
 Sample : P4185-02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY067

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037625.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	37	42	52	rBV2	12934	22134	0.95%	0.127%
2	1.278	68	74	89	rVB	304447	326518	14.04%	1.881%
3	1.532	146	153	168	rVB	268693	311076	13.37%	1.792%
4	2.059	308	317	342	rVB	557377	819288	35.22%	4.719%
5	3.458	750	752	754	rBV2	513	256	0.01%	0.001%
6	3.529	772	774	779	rVB5	824	433	0.02%	0.002%
7	3.580	789	790	791	rBV	347	88	0.00%	0.001%
8	3.629	804	805	806	rBV	507	147	0.01%	0.001%
9	3.735	835	838	842	rBV3	528	328	0.01%	0.002%
10	3.754	842	844	847	rBV2	387	203	0.01%	0.001%
11	3.796	848	857	883	rBV	100270	287748	12.37%	1.657%
12	4.243	981	996	1027	rBV	376431	959973	41.27%	5.530%
13	4.506	1058	1078	1098	rBV	227022	584797	25.14%	3.369%
14	4.844	1181	1183	1184	rBV	480	229	0.01%	0.001%
15	4.879	1190	1194	1196	rBV2	670	440	0.02%	0.003%
16	4.950	1200	1216	1249	rBV2	920633	2326121	100.00%	13.399%
17	5.265	1312	1314	1316	rBV2	739	478	0.02%	0.003%
18	5.529	1385	1396	1429	rBV	666561	1397535	60.08%	8.050%
19	5.985	1525	1538	1571	rBV	522478	1083120	46.56%	6.239%
20	6.275	1625	1628	1631	rBV4	764	660	0.03%	0.004%
21	6.352	1649	1652	1654	rVB4	1153	584	0.03%	0.003%
22	6.368	1654	1657	1658	rBV2	584	290	0.01%	0.002%
23	6.503	1696	1699	1705	rBV3	559	527	0.02%	0.003%
24	6.603	1727	1730	1732	rBV3	684	510	0.02%	0.003%
25	6.667	1748	1750	1752	rBV3	434	224	0.01%	0.001%
26	6.747	1774	1775	1779	rBV4	639	474	0.02%	0.003%
27	6.776	1782	1784	1790	rVB2	908	640	0.03%	0.004%
28	6.812	1790	1795	1797	rBV4	601	478	0.02%	0.003%
29	6.834	1800	1802	1807	rBV5	826	838	0.04%	0.005%
30	6.873	1812	1814	1815	rBV	541	208	0.01%	0.001%
31	6.908	1815	1825	1854	rBV	251996	489707	21.05%	2.821%
32	7.239	1916	1928	1953	rBV	1013653	1822384	78.34%	10.497%
33	7.551	2016	2025	2053	rBV	166148	315003	13.54%	1.814%
34	7.908	2126	2136	2152	rVB3	29174	52658	2.26%	0.303%
35	7.992	2158	2162	2164	rBV4	1074	891	0.04%	0.005%
36	8.027	2164	2173	2207	rBV2	274312	613042	26.35%	3.531%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037625.D
 Acq On : 27 Sep 2024 22:27
 Operator : SY/MD
 Sample : P4185-02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY067

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	8.779	2396	2407	2434	rBV	1058693	1745590	75.04%	10.055%
38	9.181	2530	2532	2535	rBV3	708	397	0.02%	0.002%
39	9.197	2535	2537	2539	rBV3	1013	518	0.02%	0.003%
40	9.339	2579	2581	2582	rVB	359	111	0.00%	0.001%
41	9.349	2582	2584	2587	rBV4	706	471	0.02%	0.003%
42	9.365	2587	2589	2592	rVB	658	321	0.01%	0.002%
43	9.387	2592	2596	2597	rBV3	884	476	0.02%	0.003%
44	9.432	2608	2610	2611	rBV	571	268	0.01%	0.002%
45	9.535	2639	2642	2644	rBV2	970	569	0.02%	0.003%
46	9.635	2670	2673	2679	rVB3	643	598	0.03%	0.003%
47	9.660	2679	2681	2683	rBV2	596	326	0.01%	0.002%
48	9.754	2708	2710	2713	rVB3	659	295	0.01%	0.002%
49	9.773	2713	2716	2718	rBV2	816	507	0.02%	0.003%
50	9.786	2718	2720	2723	rVB3	324	119	0.01%	0.001%
51	9.818	2729	2730	2734	rBV3	439	284	0.01%	0.002%
52	9.834	2734	2735	2738	rBV	491	210	0.01%	0.001%
53	9.873	2743	2747	2753	rVB4	1758	1799	0.08%	0.010%
54	9.937	2765	2767	2769	rBV	561	228	0.01%	0.001%
55	9.976	2776	2779	2782	rVB3	1235	706	0.03%	0.004%
56	9.992	2782	2784	2785	rBV2	370	154	0.01%	0.001%
57	10.008	2787	2789	2792	rVB3	564	276	0.01%	0.002%
58	10.050	2799	2802	2809	rBV3	959	1225	0.05%	0.007%
59	10.078	2809	2811	2814	rBV3	617	368	0.02%	0.002%
60	10.146	2820	2832	2852	rBV	590488	946026	40.67%	5.449%
61	10.413	2913	2915	2917	rVB3	1023	326	0.01%	0.002%
62	10.471	2927	2933	2941	rBV4	1032	1377	0.06%	0.008%
63	10.622	2979	2980	2981	rVB4	482	93	0.00%	0.001%
64	10.693	2997	3002	3004	rBV2	489	386	0.02%	0.002%
65	10.763	3021	3024	3025	rBV	626	253	0.01%	0.001%
66	10.783	3028	3030	3032	rVV	732	318	0.01%	0.002%
67	10.940	3078	3079	3081	rBV	310	143	0.01%	0.001%
68	10.953	3081	3083	3086	rVV3	747	346	0.01%	0.002%
69	10.966	3086	3087	3090	rVB	603	300	0.01%	0.002%
70	11.014	3099	3102	3106	rVB3	544	384	0.02%	0.002%
71	11.178	3143	3153	3185	rBV	995181	1583786	68.09%	9.123%
72	11.554	3258	3270	3305	rBV	1024366	1645854	70.76%	9.480%
73	11.940	3387	3390	3392	rVB4	984	519	0.02%	0.003%
74	11.966	3392	3398	3401	rBV4	1019	940	0.04%	0.005%
75	11.985	3401	3404	3405	rBV2	916	443	0.02%	0.003%
76	12.429	3540	3542	3544	rBV2	677	254	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037625.D
Acq On : 27 Sep 2024 22:27
Operator : SY/MD
Sample : P4185-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY067

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis

77	12.950	3702	3704	3709	rVB4	727	449	0.02%	0.003%
78	13.043	3731	3733	3736	rBV	577	382	0.02%	0.002%
79	13.062	3737	3739	3741	rVB2	841	356	0.02%	0.002%
80	13.078	3741	3744	3747	rVB4	917	527	0.02%	0.003%
81	13.094	3747	3749	3752	rBV2	691	421	0.02%	0.002%
82	13.673	3925	3929	3931	rBV5	939	885	0.04%	0.005%




Sum of corrected areas: 17360614

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037625.D
Acq On : 27 Sep 2024 22:27
Operator : SY/MD
Sample : P4185-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY067

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

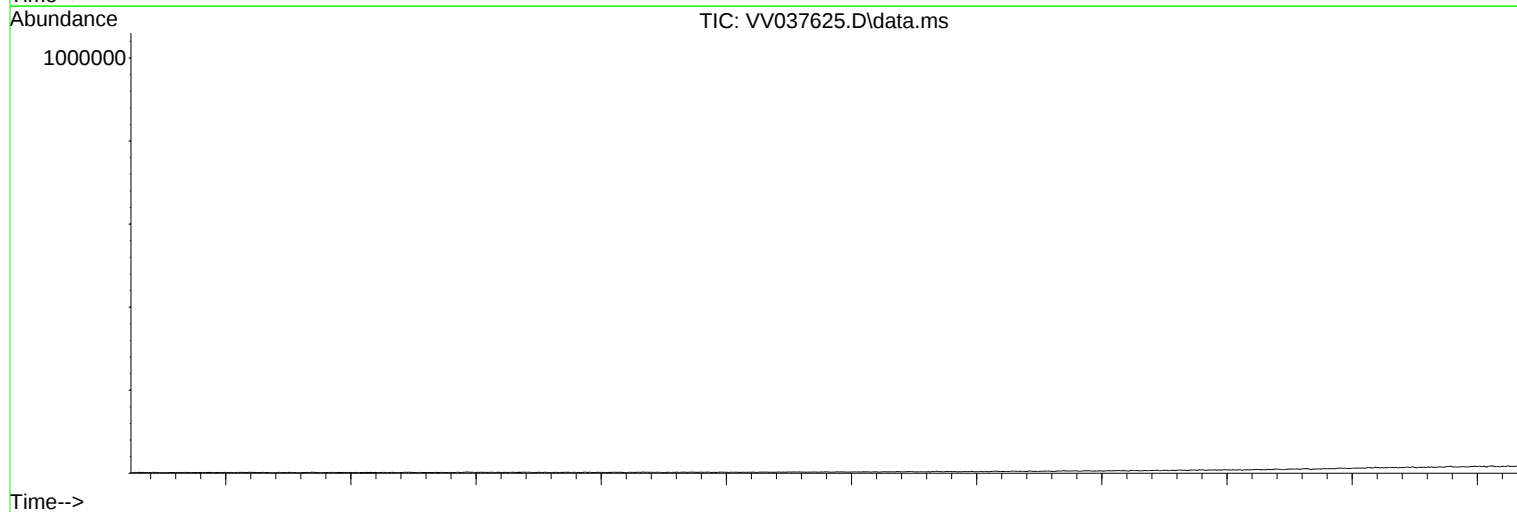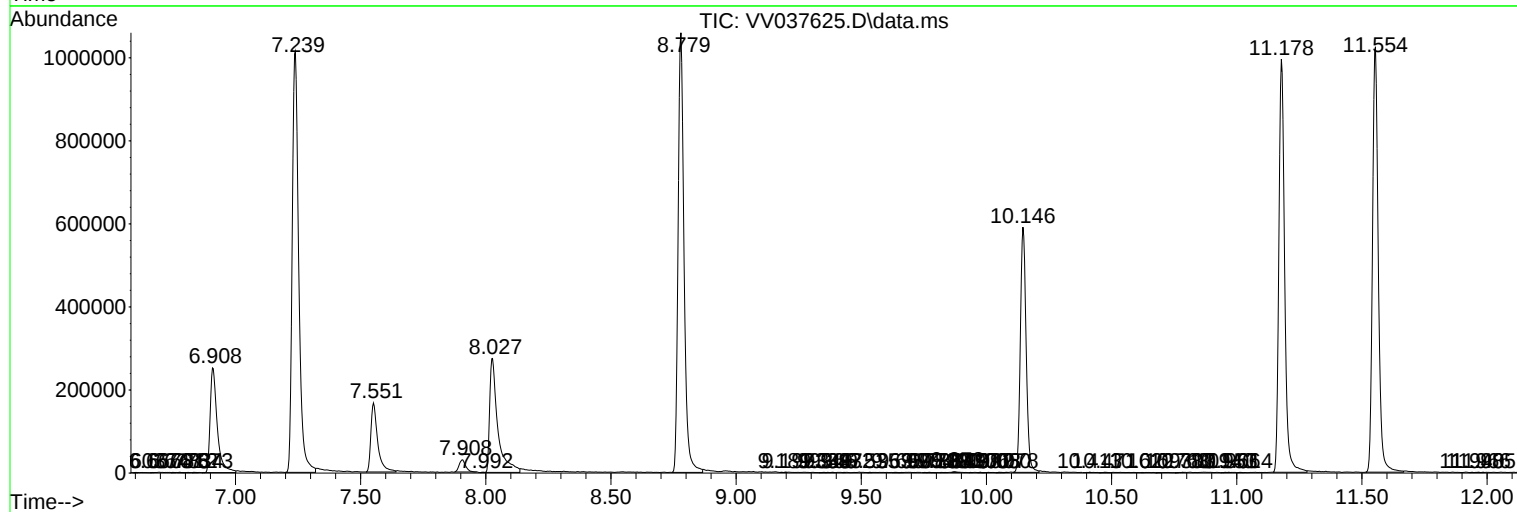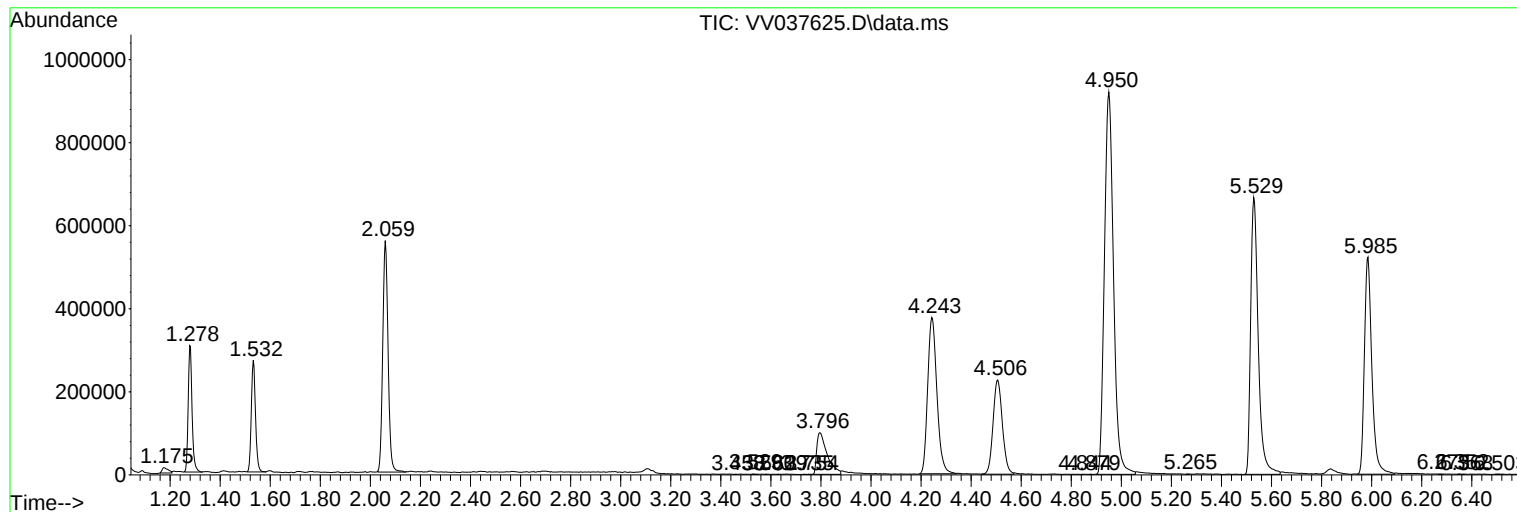

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037625.D
Acq On : 27 Sep 2024 22:27
Operator : SY/MD
Sample : P4185-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY067

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037625.D
Acq On : 27 Sep 2024 22:27
Operator : SY/MD
Sample : P4185-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY067

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
