

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037626.D
 Acq On : 27 Sep 2024 22:48
 Operator : SY/MD
 Sample : P4185-03DL 50X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY077DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037626.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	35	42	52	rBV	10106	19960	0.87%	0.111%
2	1.278	67	74	92	rVB	300563	324356	14.16%	1.803%
3	1.532	145	153	166	rVB	262146	308813	13.48%	1.716%
4	2.060	307	317	336	rVB	533370	780928	34.09%	4.340%
5	3.105	632	642	663	rVB2	83221	179289	7.83%	0.996%
6	3.336	710	714	716	rBV4	873	599	0.03%	0.003%
7	3.516	764	770	775	rVB5	799	977	0.04%	0.005%
8	3.609	797	799	803	rVB4	837	515	0.02%	0.003%
9	3.693	823	825	828	rBV2	705	531	0.02%	0.003%
10	3.722	831	834	839	rVB3	756	734	0.03%	0.004%
11	3.806	844	860	891	rBV2	428867	1181333	51.56%	6.565%
12	4.056	936	938	942	rVB3	1249	718	0.03%	0.004%
13	4.124	957	959	962	rBV2	798	614	0.03%	0.003%
14	4.243	980	996	1029	rVV	376691	959268	41.87%	5.331%
15	4.368	1032	1035	1039	rVV4	846	695	0.03%	0.004%
16	4.507	1062	1078	1099	rBV2	91894	237788	10.38%	1.322%
17	4.950	1200	1216	1251	rBV2	893943	2291003	100.00%	12.732%
18	5.394	1350	1354	1356	rBV2	579	499	0.02%	0.003%
19	5.481	1377	1381	1383	rBV3	950	641	0.03%	0.004%
20	5.529	1385	1396	1423	rBV	635414	1315690	57.43%	7.312%
21	5.831	1482	1490	1505	rVB	9287	20820	0.91%	0.116%
22	5.982	1522	1537	1567	rBV	509788	1075029	46.92%	5.975%
23	6.336	1643	1647	1649	rBV3	753	667	0.03%	0.004%
24	6.384	1661	1662	1668	rVB4	1240	839	0.04%	0.005%
25	6.506	1695	1700	1706	rVB5	718	675	0.03%	0.004%
26	6.548	1710	1713	1719	rVB4	458	473	0.02%	0.003%
27	6.728	1764	1769	1771	rVB3	750	517	0.02%	0.003%
28	6.770	1778	1782	1786	rVB3	766	690	0.03%	0.004%
29	6.908	1814	1825	1852	rBV	246966	481224	21.00%	2.674%
30	7.143	1895	1898	1903	rVB6	981	783	0.03%	0.004%
31	7.236	1916	1927	1969	rBV	988026	1781771	77.77%	9.902%
32	7.551	2016	2025	2055	rBV	166203	317675	13.87%	1.766%
33	7.760	2086	2090	2092	rBV4	930	846	0.04%	0.005%
34	7.889	2127	2130	2131	rBV3	1064	520	0.02%	0.003%
35	7.912	2131	2137	2143	rBV8	2377	2694	0.12%	0.015%
36	8.024	2163	2172	2214	rBV2	275328	624752	27.27%	3.472%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037626.D
 Acq On : 27 Sep 2024 22:48
 Operator : SY/MD
 Sample : P4185-03DL 50X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY077DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	8.545	2329	2334	2335	rBV5	1233	885	0.04%	0.005%
38	8.590	2345	2348	2353	rBV6	871	835	0.04%	0.005%
39	8.725	2387	2390	2395	rVB3	736	553	0.02%	0.003%
40	8.780	2395	2407	2450	rBV	960031	1642186	71.68%	9.127%
41	8.953	2455	2461	2477	rVB2	10078	20709	0.90%	0.115%
42	9.014	2478	2480	2484	rBV4	811	493	0.02%	0.003%
43	9.079	2494	2500	2514	rVB2	15606	28012	1.22%	0.156%
44	9.223	2543	2545	2549	rVB6	1038	589	0.03%	0.003%
45	9.252	2551	2554	2557	rVV5	714	622	0.03%	0.003%
46	9.272	2557	2560	2564	rVB3	885	699	0.03%	0.004%
47	9.294	2564	2567	2570	rVB5	765	508	0.02%	0.003%
48	9.481	2617	2625	2642	rVV	17559	31591	1.38%	0.176%
49	9.635	2670	2673	2675	rBV2	995	675	0.03%	0.004%
50	9.815	2727	2729	2732	rVB2	1066	544	0.02%	0.003%
51	9.879	2738	2749	2755	rBV6	2406	4026	0.18%	0.022%
52	9.998	2782	2786	2788	rBV3	992	673	0.03%	0.004%
53	10.146	2818	2832	2856	rBV	600701	952865	41.59%	5.296%
54	10.294	2871	2878	2886	rBV3	5894	9437	0.41%	0.052%
55	10.384	2896	2906	2915	rBV2	24684	44915	1.96%	0.250%
56	10.474	2928	2934	2949	rVB2	13797	22731	0.99%	0.126%
57	10.571	2962	2964	2968	rVB2	704	538	0.02%	0.003%
58	10.606	2970	2975	2977	rBV3	679	546	0.02%	0.003%
59	10.674	2988	2996	3010	rVV2	14897	24649	1.08%	0.137%
60	10.792	3027	3033	3037	rBV6	1253	1398	0.06%	0.008%
61	10.850	3041	3051	3075	rBV2	60888	101816	4.44%	0.566%
62	10.944	3078	3080	3085	rVB3	1006	473	0.02%	0.003%
63	11.018	3099	3103	3109	rBV5	989	1045	0.05%	0.006%
64	11.130	3129	3138	3143	rBV7	2864	4583	0.20%	0.025%
65	11.178	3143	3153	3174	rVV	940591	1478696	64.54%	8.218%
66	11.272	3176	3182	3195	rVB2	28191	47890	2.09%	0.266%
67	11.461	3233	3241	3253	rBV6	8598	16904	0.74%	0.094%
68	11.554	3259	3270	3298	rVB	998686	1596152	69.67%	8.871%
69	11.854	3355	3363	3367	rBV7	5335	6811	0.30%	0.038%
70	11.963	3387	3397	3404	rBV7	2792	5603	0.24%	0.031%
71	12.043	3417	3422	3423	rBV3	680	582	0.03%	0.003%
72	12.056	3423	3426	3429	rVV4	1034	806	0.04%	0.004%
73	12.407	3528	3535	3542	rBV5	2031	2862	0.12%	0.016%
74	12.474	3552	3556	3557	rBV2	1125	596	0.03%	0.003%
75	12.599	3592	3595	3599	rVB5	703	658	0.03%	0.004%
76	12.628	3599	3604	3606	rVB4	834	567	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037626.D
 Acq On : 27 Sep 2024 22:48
 Operator : SY/MD
 Sample : P4185-03DL 50X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY077DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.821	3657	3664	3669	rBV9	3175	3595	0.16%	0.020%
78	12.879	3679	3682	3685	rBV3	922	662	0.03%	0.004%
79	12.989	3713	3716	3718	rBV3	989	653	0.03%	0.004%
80	13.140	3758	3763	3768	rBV4	721	670	0.03%	0.004%
81	13.185	3773	3777	3781	rVB5	688	552	0.02%	0.003%
82	13.214	3781	3786	3790	rBV4	1205	1273	0.06%	0.007%
83	13.300	3809	3813	3814	rBV4	714	540	0.02%	0.003%
84	13.403	3841	3845	3848	rBV3	690	623	0.03%	0.003%
85	13.455	3852	3861	3862	rBV6	3189	2991	0.13%	0.017%
86	13.799	3965	3968	3970	rBV2	732	511	0.02%	0.003%
87	13.844	3977	3982	3984	rVV4	1020	771	0.03%	0.004%
88	13.860	3984	3987	3991	rVB3	1184	679	0.03%	0.004%
89	13.898	3996	3999	4002	rVV3	722	514	0.02%	0.003%
90	14.162	4078	4081	4084	rBV5	1147	864	0.04%	0.005%
91	14.307	4124	4126	4133	rVB5	796	483	0.02%	0.003%
92	14.361	4140	4143	4148	rBV3	991	679	0.03%	0.004%
93	14.439	4163	4167	4169	rBV3	703	554	0.02%	0.003%
94	14.718	4252	4254	4260	rVB7	1082	914	0.04%	0.005%
95	14.767	4265	4269	4272	rBV4	890	598	0.03%	0.003%
96	14.902	4309	4311	4313	rBV3	733	493	0.02%	0.003%
97	15.078	4363	4366	4368	rBV4	1022	619	0.03%	0.003%
98	15.146	4384	4387	4390	rBV4	887	728	0.03%	0.004%
99	15.165	4390	4393	4396	rBV4	990	881	0.04%	0.005%
100	15.297	4431	4434	4437	rBV4	1236	904	0.04%	0.005%

Sum of corrected areas: 17993400




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037626.D
Acq On : 27 Sep 2024 22:48
Operator : SY/MD
Sample : P4185-03DL 50X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY077DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

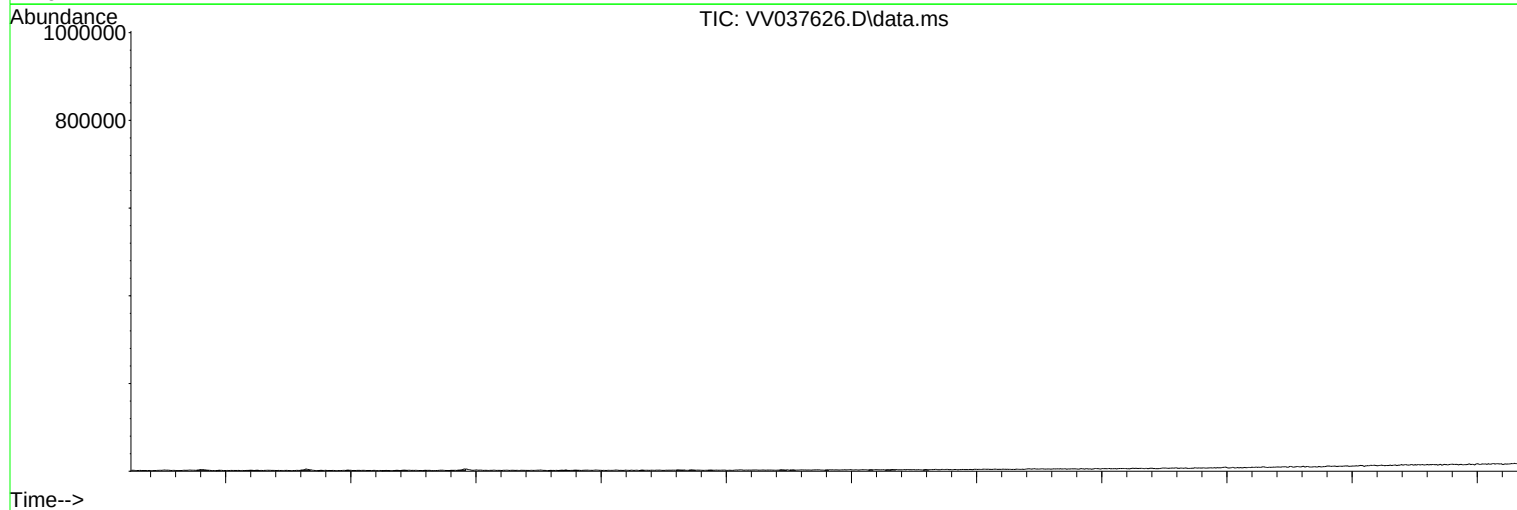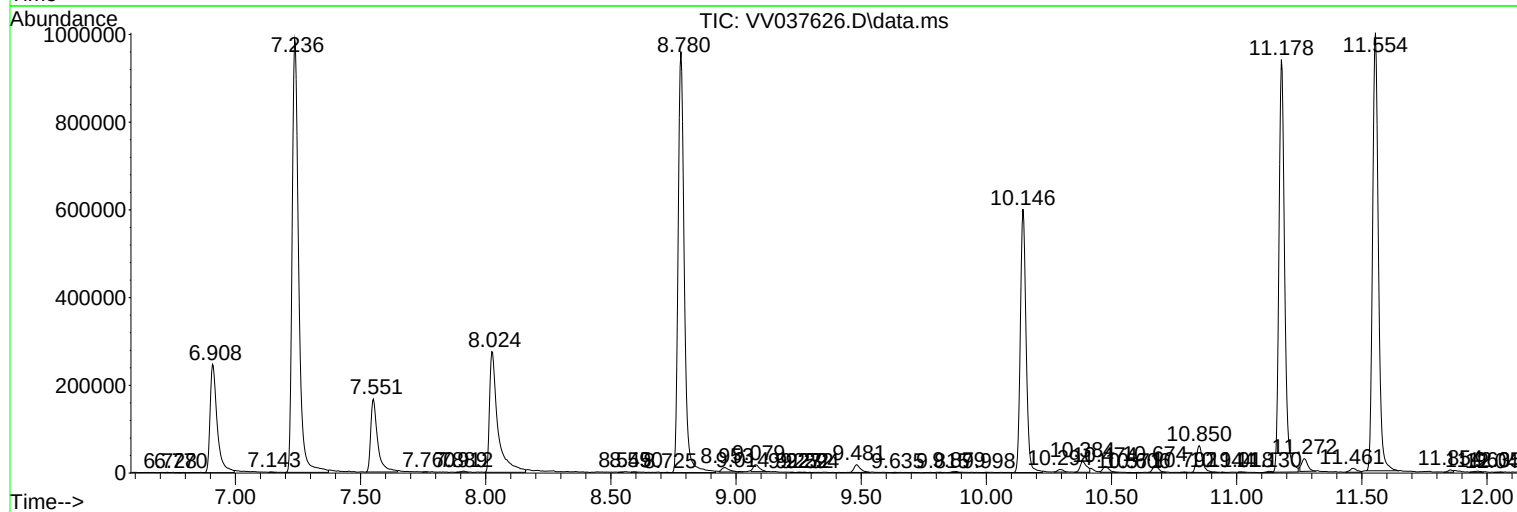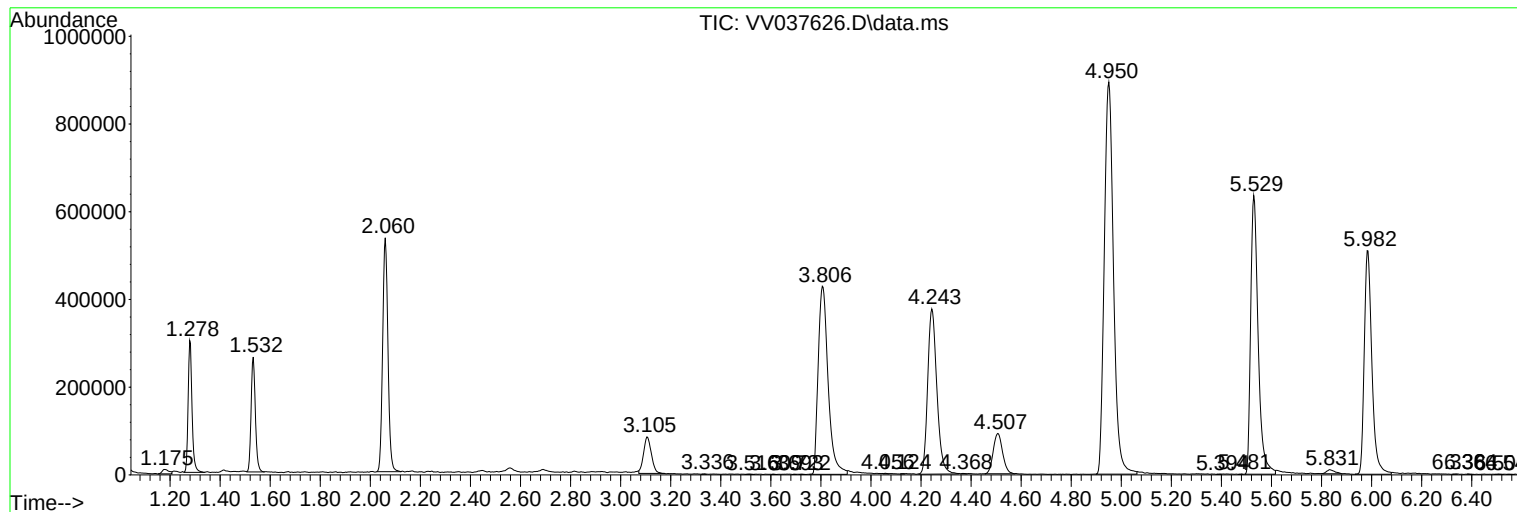

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037626.D
Acq On : 27 Sep 2024 22:48
Operator : SY/MD
Sample : P4185-03DL 50X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY077DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037626.D
Acq On : 27 Sep 2024 22:48
Operator : SY/MD
Sample : P4185-03DL 50X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY077DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc