

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037632.D
 Acq On : 28 Sep 2024 00:57
 Operator : SY/MD
 Sample : P4185-13DL 20X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY061DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037632.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	51	rBV	16819	27447	1.34%	0.188%
2	1.281	68	75	91	rVB2	301992	339530	16.60%	2.326%
3	1.532	145	153	155	rBV	246795	258883	12.66%	1.774%
4	2.060	308	317	332	rVB	445158	627714	30.69%	4.300%
5	3.487	759	761	763	rVB2	655	324	0.02%	0.002%
6	3.506	763	767	769	rBV3	691	479	0.02%	0.003%
7	3.539	774	777	781	rBV3	791	640	0.03%	0.004%
8	3.568	784	786	787	rBV	496	214	0.01%	0.001%
9	3.654	811	813	819	rVB3	740	475	0.02%	0.003%
10	3.754	842	844	846	rVB3	366	194	0.01%	0.001%
11	3.796	848	857	889	rBV	98781	307156	15.02%	2.104%
12	4.243	978	996	1028	rBV	342668	875605	42.81%	5.999%
13	4.584	1100	1102	1105	rBV2	432	225	0.01%	0.002%
14	4.600	1105	1107	1110	rVB2	759	380	0.02%	0.003%
15	4.619	1110	1113	1115	rBV3	637	441	0.02%	0.003%
16	4.725	1140	1146	1148	rBV3	916	638	0.03%	0.004%
17	4.789	1163	1166	1168	rBV2	414	256	0.01%	0.002%
18	4.809	1168	1172	1174	rVV3	829	541	0.03%	0.004%
19	4.822	1174	1176	1180	rVB2	669	362	0.02%	0.002%
20	4.879	1191	1194	1195	rBV2	870	454	0.02%	0.003%
21	4.950	1200	1216	1250	rBV2	794475	2045094	100.00%	14.010%
22	5.449	1369	1371	1372	rBV	451	197	0.01%	0.001%
23	5.468	1372	1377	1378	rBV2	384	291	0.01%	0.002%
24	5.529	1385	1396	1434	rBV	596753	1253561	61.30%	8.588%
25	5.985	1523	1538	1568	rBV	460097	966815	47.27%	6.623%
26	6.420	1671	1673	1676	rVB4	896	371	0.02%	0.003%
27	6.455	1683	1684	1687	rBV3	511	279	0.01%	0.002%
28	6.510	1694	1701	1704	rBV5	1243	1463	0.07%	0.010%
29	6.551	1711	1714	1716	rBV2	800	539	0.03%	0.004%
30	6.612	1731	1733	1734	rBV	459	199	0.01%	0.001%
31	6.632	1737	1739	1742	rVB4	751	396	0.02%	0.003%
32	6.651	1742	1745	1746	rBV2	965	576	0.03%	0.004%
33	6.680	1752	1754	1756	rVB3	611	156	0.01%	0.001%
34	6.715	1761	1765	1769	rBV4	935	704	0.03%	0.005%
35	6.776	1780	1784	1787	rBV2	473	456	0.02%	0.003%
36	6.847	1804	1806	1809	rBV2	645	286	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037632.D
 Acq On : 28 Sep 2024 00:57
 Operator : SY/MD
 Sample : P4185-13DL 20X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY061DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.911	1816	1826	1851	rBV	222095	427932	20.92%	2.932%
38	7.239	1917	1928	1968	rBV	825935	1488998	72.81%	10.201%
39	7.551	2016	2025	2048	rBV	147332	277279	13.56%	1.900%
40	7.831	2110	2112	2115	rVB4	1045	529	0.03%	0.004%
41	8.024	2163	2172	2210	rBV2	257715	576002	28.17%	3.946%
42	8.551	2329	2336	2338	rBV6	1747	1969	0.10%	0.013%
43	8.664	2368	2371	2373	rBV	868	633	0.03%	0.004%
44	8.699	2379	2382	2383	rBV3	510	249	0.01%	0.002%
45	8.741	2393	2395	2396	rBV	974	464	0.02%	0.003%
46	8.780	2396	2407	2434	rVV	914325	1510751	73.87%	10.350%
47	9.156	2521	2524	2525	rBV2	846	429	0.02%	0.003%
48	9.304	2568	2570	2571	rBV2	744	262	0.01%	0.002%
49	9.413	2600	2604	2608	rBV2	504	398	0.02%	0.003%
50	9.442	2611	2613	2614	rBV	962	332	0.02%	0.002%
51	9.477	2622	2624	2627	rBV3	646	354	0.02%	0.002%
52	9.529	2638	2640	2642	rBV2	526	251	0.01%	0.002%
53	9.628	2669	2671	2674	rBV3	637	314	0.02%	0.002%
54	9.651	2675	2678	2680	rVB3	776	441	0.02%	0.003%
55	9.667	2680	2683	2684	rBV	547	330	0.02%	0.002%
56	9.690	2688	2690	2691	rBV	498	199	0.01%	0.001%
57	9.728	2700	2702	2706	rVB3	750	300	0.01%	0.002%
58	9.747	2706	2708	2712	rBV3	638	519	0.03%	0.004%
59	9.915	2757	2760	2762	rBV4	906	453	0.02%	0.003%
60	9.963	2773	2775	2777	rBV3	340	185	0.01%	0.001%
61	10.021	2790	2793	2794	rBV2	367	175	0.01%	0.001%
62	10.034	2794	2797	2801	rVV3	687	515	0.03%	0.004%
63	10.056	2801	2804	2809	rVV5	608	505	0.02%	0.003%
64	10.146	2820	2832	2858	rBV	543199	868548	42.47%	5.950%
65	10.365	2898	2900	2903	rVB4	896	462	0.02%	0.003%
66	10.390	2904	2908	2909	rBV3	738	444	0.02%	0.003%
67	10.455	2926	2928	2933	rBV3	889	464	0.02%	0.003%
68	10.493	2938	2940	2943	rBV2	645	347	0.02%	0.002%
69	10.542	2953	2955	2959	rBV2	571	343	0.02%	0.002%
70	10.561	2959	2961	2964	rVB3	681	305	0.01%	0.002%
71	10.603	2971	2974	2977	rBV3	793	520	0.03%	0.004%
72	10.641	2983	2986	2989	rBV3	506	489	0.02%	0.003%
73	10.683	2989	2999	3005	rBV5	4708	8457	0.41%	0.058%
74	10.767	3021	3025	3026	rBV3	423	286	0.01%	0.002%
75	10.837	3044	3047	3048	rBV3	799	442	0.02%	0.003%
76	10.863	3049	3055	3064	rVV7	2887	4574	0.22%	0.031%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037632.D
 Acq On : 28 Sep 2024 00:57
 Operator : SY/MD
 Sample : P4185-13DL 20X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY061DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.902	3064	3067	3074	rVB5	1267	1272	0.06%	0.009%
78	10.937	3074	3078	3079	rBV2	846	710	0.03%	0.005%
79	10.963	3084	3086	3090	rVB2	565	300	0.01%	0.002%
80	10.995	3093	3096	3099	rBV2	786	555	0.03%	0.004%
81	11.037	3108	3109	3113	rVB2	433	210	0.01%	0.001%
82	11.069	3113	3119	3122	rVB2	886	911	0.04%	0.006%
83	11.088	3122	3125	3127	rBV2	839	547	0.03%	0.004%
84	11.178	3143	3153	3195	rBV	827634	1318351	64.46%	9.032%
85	11.554	3253	3270	3298	rBV	851189	1376103	67.29%	9.427%
86	11.982	3400	3403	3408	rVB5	1170	1023	0.05%	0.007%
87	12.050	3422	3424	3428	rBV4	599	440	0.02%	0.003%
88	12.146	3450	3454	3457	rVB3	910	598	0.03%	0.004%
89	12.242	3482	3484	3488	rBV3	689	507	0.02%	0.003%
90	12.342	3514	3515	3518	rBV2	655	385	0.02%	0.003%
91	12.419	3537	3539	3541	rBV3	590	240	0.01%	0.002%
92	12.445	3545	3547	3550	rBV4	652	322	0.02%	0.002%
93	12.718	3629	3632	3637	rVB3	654	434	0.02%	0.003%
94	12.882	3680	3683	3687	rBV2	995	736	0.04%	0.005%
95	13.037	3727	3731	3737	rBV5	956	1016	0.05%	0.007%
96	13.085	3744	3746	3747	rBV2	417	168	0.01%	0.001%
97	13.194	3778	3780	3783	rBV3	667	424	0.02%	0.003%
98	13.339	3823	3825	3830	rVB4	639	521	0.03%	0.004%
99	13.802	3967	3969	3970	rBV	579	232	0.01%	0.002%
100	13.969	4015	4021	4023	rBV5	1382	1264	0.06%	0.009%

Sum of corrected areas: 14597059




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037632.D
Acq On : 28 Sep 2024 00:57
Operator : SY/MD
Sample : P4185-13DL 20X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY061DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

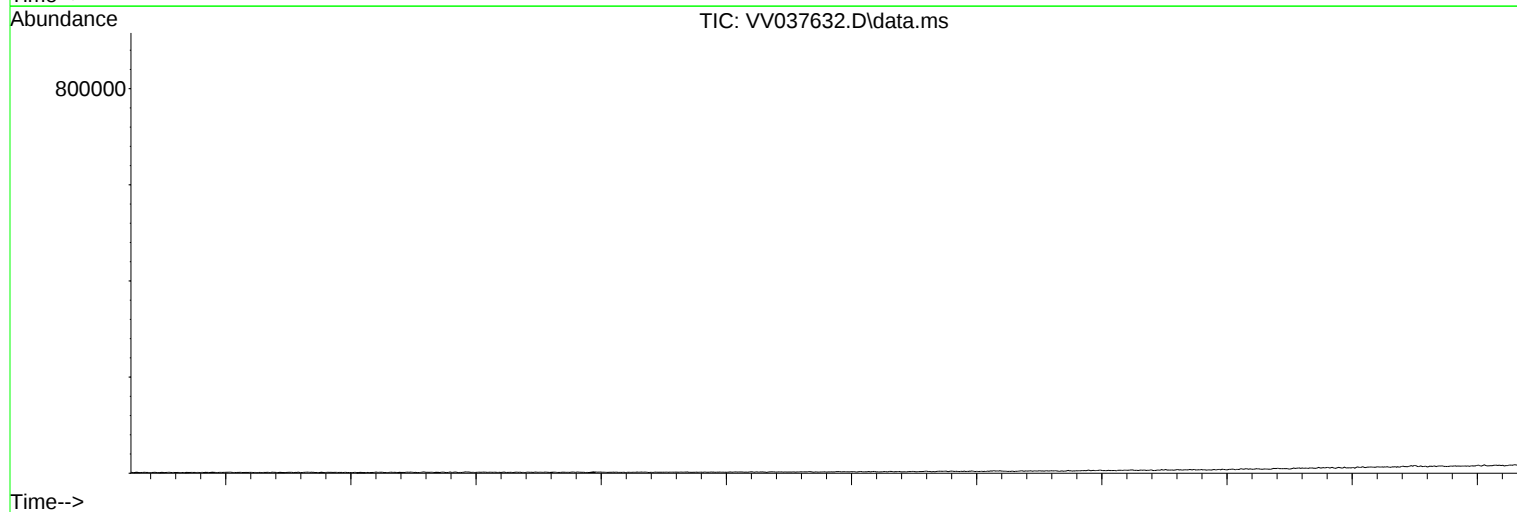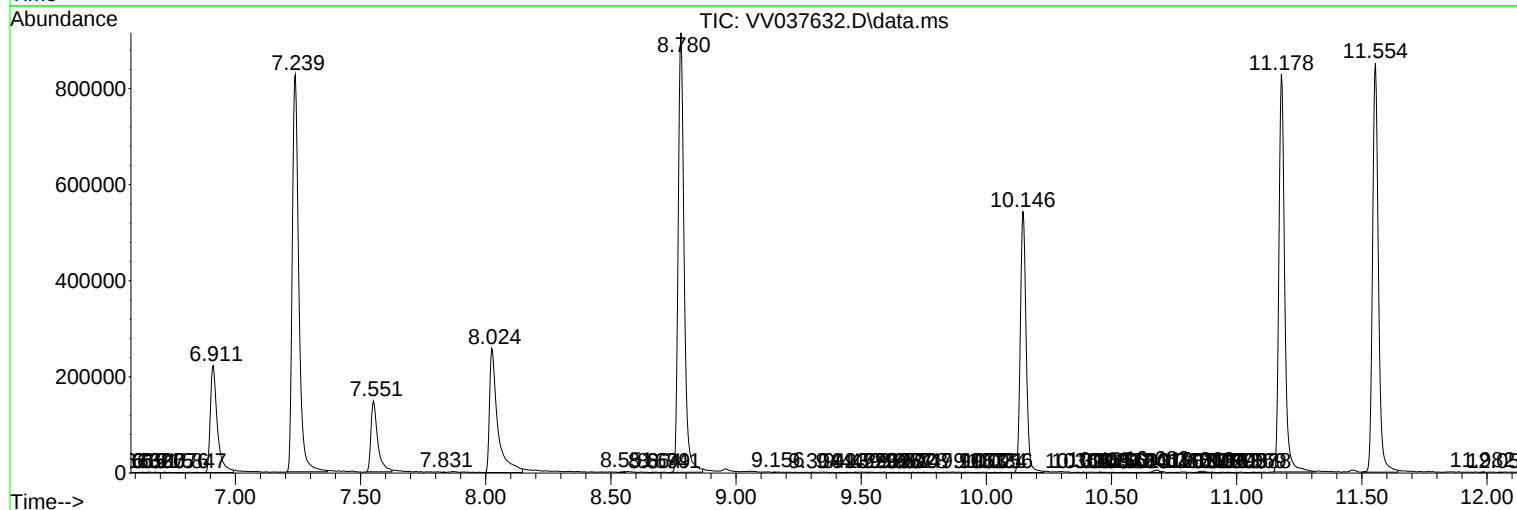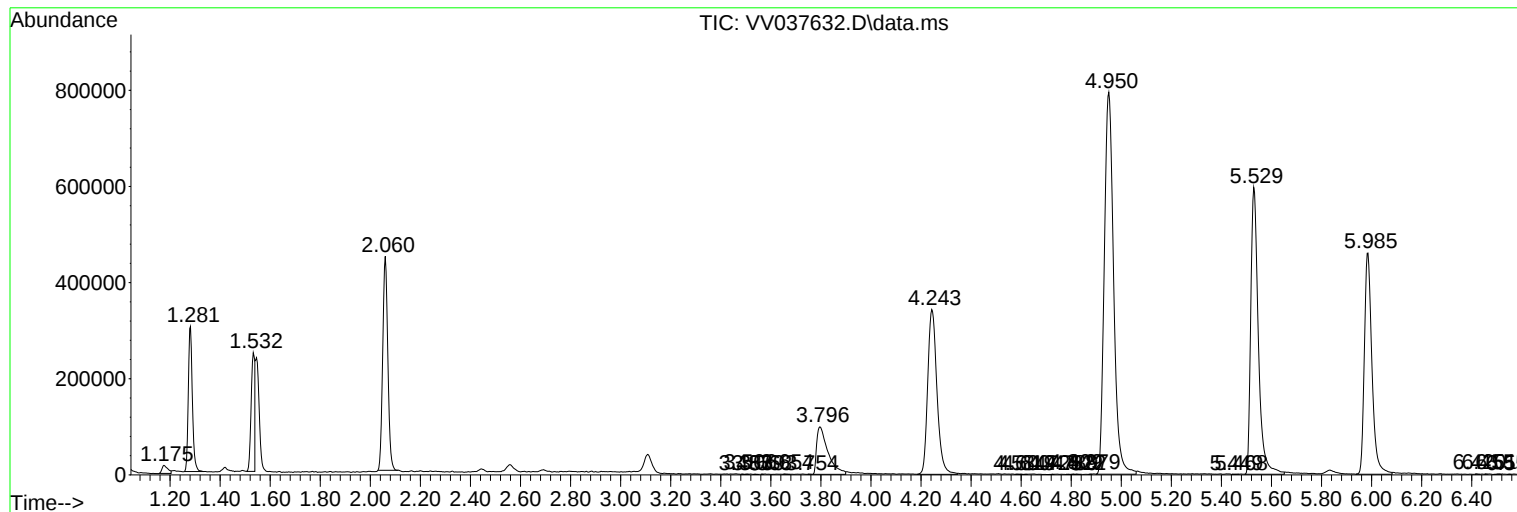

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037632.D
Acq On : 28 Sep 2024 00:57
Operator : SY/MD
Sample : P4185-13DL 20X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY061DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037632.D
Acq On : 28 Sep 2024 00:57
Operator : SY/MD
Sample : P4185-13DL 20X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY061DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc