

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037633.D
 Acq On : 28 Sep 2024 01:18
 Operator : SY/MD
 Sample : P4185-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY062

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037633.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	51	rBV	19202	30451	1.39%	0.174%
2	1.278	68	74	88	rVB	267136	287197	13.13%	1.643%
3	1.532	146	153	167	rVB	247824	289093	13.22%	1.654%
4	2.060	308	317	332	rBV	505825	726953	33.24%	4.159%
5	3.108	632	643	665	rVB2	214481	452521	20.69%	2.589%
6	3.625	802	804	807	rBV2	527	348	0.02%	0.002%
7	3.805	847	860	889	rBV2	214229	612859	28.02%	3.506%
8	4.137	960	963	966	rVB3	924	533	0.02%	0.003%
9	4.243	981	996	1024	rBV	354993	903157	41.30%	5.167%
10	4.506	1062	1078	1101	rBV2	268489	680662	31.13%	3.894%
11	4.703	1136	1139	1140	rBV3	507	241	0.01%	0.001%
12	4.744	1150	1152	1154	rBV3	596	217	0.01%	0.001%
13	4.844	1179	1183	1186	rBV3	700	587	0.03%	0.003%
14	4.870	1188	1191	1196	rVB3	535	428	0.02%	0.002%
15	4.950	1196	1216	1257	rBV2	851190	2186856	100.00%	12.511%
16	5.201	1293	1294	1299	rVB4	901	515	0.02%	0.003%
17	5.259	1308	1312	1313	rBV	1081	745	0.03%	0.004%
18	5.371	1345	1347	1350	rBV3	733	479	0.02%	0.003%
19	5.439	1366	1368	1373	rVB4	614	454	0.02%	0.003%
20	5.458	1373	1374	1376	rBV2	522	213	0.01%	0.001%
21	5.529	1385	1396	1432	rBV	657592	1365418	62.44%	7.812%
22	5.838	1483	1492	1510	rVB5	33955	76000	3.48%	0.435%
23	5.985	1525	1538	1563	rBV	480613	1003478	45.89%	5.741%
24	6.275	1622	1628	1632	rBV5	1269	1629	0.07%	0.009%
25	6.323	1636	1643	1644	rBV4	856	994	0.05%	0.006%
26	6.368	1654	1657	1658	rBV2	717	409	0.02%	0.002%
27	6.416	1666	1672	1675	rBV5	955	968	0.04%	0.006%
28	6.452	1681	1683	1685	rBV3	448	172	0.01%	0.001%
29	6.477	1688	1691	1693	rBV2	473	340	0.02%	0.002%
30	6.519	1702	1704	1706	rVB2	965	286	0.01%	0.002%
31	6.555	1713	1715	1719	rBV3	970	755	0.03%	0.004%
32	6.587	1721	1725	1728	rBV4	823	697	0.03%	0.004%
33	6.632	1735	1739	1741	rVB2	679	312	0.01%	0.002%
34	6.648	1741	1744	1745	rBV2	549	318	0.01%	0.002%
35	6.686	1752	1756	1760	rVB5	921	674	0.03%	0.004%
36	6.715	1761	1765	1769	rBV3	659	468	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037633.D
 Acq On : 28 Sep 2024 01:18
 Operator : SY/MD
 Sample : P4185-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY062

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.738	1769	1772	1773	rBV	477	222	0.01%	0.001%
38	6.773	1777	1783	1786	rBV4	1146	1216	0.06%	0.007%
39	6.911	1815	1826	1854	rBV	228279	449548	20.56%	2.572%
40	7.165	1903	1905	1909	rVB2	623	422	0.02%	0.002%
41	7.239	1917	1928	1969	rBV	947975	1719399	78.62%	9.837%
42	7.551	2016	2025	2050	rBV	155647	292762	13.39%	1.675%
43	7.754	2083	2088	2089	rBV3	1002	753	0.03%	0.004%
44	7.905	2123	2135	2150	rBV2	62547	115247	5.27%	0.659%
45	7.976	2155	2157	2162	rVB5	1103	588	0.03%	0.003%
46	8.024	2164	2172	2208	rBV2	247078	557214	25.48%	3.188%
47	8.673	2372	2374	2377	rVB2	883	392	0.02%	0.002%
48	8.738	2392	2394	2396	rBV2	521	321	0.01%	0.002%
49	8.780	2396	2407	2439	rBV	1015120	1708777	78.14%	9.776%
50	9.156	2522	2524	2528	rBV4	695	452	0.02%	0.003%
51	9.175	2528	2530	2533	rVV2	596	238	0.01%	0.001%
52	9.223	2539	2545	2547	rBV5	1034	918	0.04%	0.005%
53	9.281	2561	2563	2568	rBV5	930	597	0.03%	0.003%
54	9.387	2592	2596	2597	rBV	558	372	0.02%	0.002%
55	9.432	2601	2610	2611	rBV4	739	997	0.05%	0.006%
56	9.558	2644	2649	2651	rBV4	905	627	0.03%	0.004%
57	9.577	2653	2655	2657	rVV	351	231	0.01%	0.001%
58	9.590	2657	2659	2663	rVV2	755	500	0.02%	0.003%
59	9.638	2671	2674	2675	rBV2	461	236	0.01%	0.001%
60	9.664	2678	2682	2683	rBV2	516	368	0.02%	0.002%
61	9.686	2686	2689	2692	rVB3	405	234	0.01%	0.001%
62	9.725	2695	2701	2702	rBV2	500	338	0.02%	0.002%
63	9.738	2702	2705	2706	rBV2	630	289	0.01%	0.002%
64	9.776	2713	2717	2718	rBV	666	362	0.02%	0.002%
65	9.821	2725	2731	2733	rBV3	660	527	0.02%	0.003%
66	9.834	2733	2735	2737	rBV	474	286	0.01%	0.002%
67	9.876	2742	2748	2754	rVB7	1552	1898	0.09%	0.011%
68	9.972	2776	2778	2781	rVB	350	169	0.01%	0.001%
69	10.024	2790	2794	2796	rVV	838	597	0.03%	0.003%
70	10.085	2810	2813	2814	rBV2	432	216	0.01%	0.001%
71	10.095	2814	2816	2819	rBV2	601	334	0.02%	0.002%
72	10.146	2821	2832	2854	rBV	559745	888242	40.62%	5.082%
73	10.320	2884	2886	2889	rVB3	811	342	0.02%	0.002%
74	10.378	2901	2904	2906	rBV2	713	407	0.02%	0.002%
75	10.406	2910	2913	2915	rBV	528	268	0.01%	0.002%
76	10.474	2933	2934	2938	rVB3	839	430	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037633.D
 Acq On : 28 Sep 2024 01:18
 Operator : SY/MD
 Sample : P4185-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY062

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.500	2940	2942	2945	rVB2	789	412	0.02%	0.002%
78	10.516	2945	2947	2948	rBV	434	206	0.01%	0.001%
79	10.619	2977	2979	2981	rBV	494	230	0.01%	0.001%
80	10.747	3014	3019	3020	rBV	677	566	0.03%	0.003%
81	10.773	3023	3027	3028	rBV	364	232	0.01%	0.001%
82	10.860	3048	3054	3056	rBV4	673	699	0.03%	0.004%
83	11.027	3104	3106	3109	rBV2	398	230	0.01%	0.001%
84	11.072	3118	3120	3123	rVB2	560	267	0.01%	0.002%
85	11.095	3123	3127	3129	rBV3	533	367	0.02%	0.002%
86	11.120	3134	3135	3139	rBV	324	170	0.01%	0.001%
87	11.178	3142	3153	3182	rBV	952367	1534164	70.15%	8.777%
88	11.554	3258	3270	3294	rBV	956444	1562471	71.45%	8.939%
89	11.937	3387	3389	3391	rBV2	707	443	0.02%	0.003%
90	11.972	3398	3400	3401	rBV	563	237	0.01%	0.001%
91	12.008	3408	3411	3414	rBV	700	648	0.03%	0.004%
92	12.140	3449	3452	3454	rBV3	598	461	0.02%	0.003%
93	12.194	3467	3469	3470	rBV	804	377	0.02%	0.002%
94	12.204	3470	3472	3475	rVB3	897	454	0.02%	0.003%
95	12.371	3520	3524	3525	rBV2	576	412	0.02%	0.002%
96	12.381	3525	3527	3529	rBV	392	181	0.01%	0.001%
97	12.776	3647	3650	3652	rBV2	503	263	0.01%	0.002%
98	12.943	3700	3702	3703	rBV	550	196	0.01%	0.001%
99	13.821	3973	3975	3976	rBV	748	282	0.01%	0.002%
100	13.950	4013	4015	4020	rBV4	877	580	0.03%	0.003%




Sum of corrected areas: 17479311

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037633.D
Acq On : 28 Sep 2024 01:18
Operator : SY/MD
Sample : P4185-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY062

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

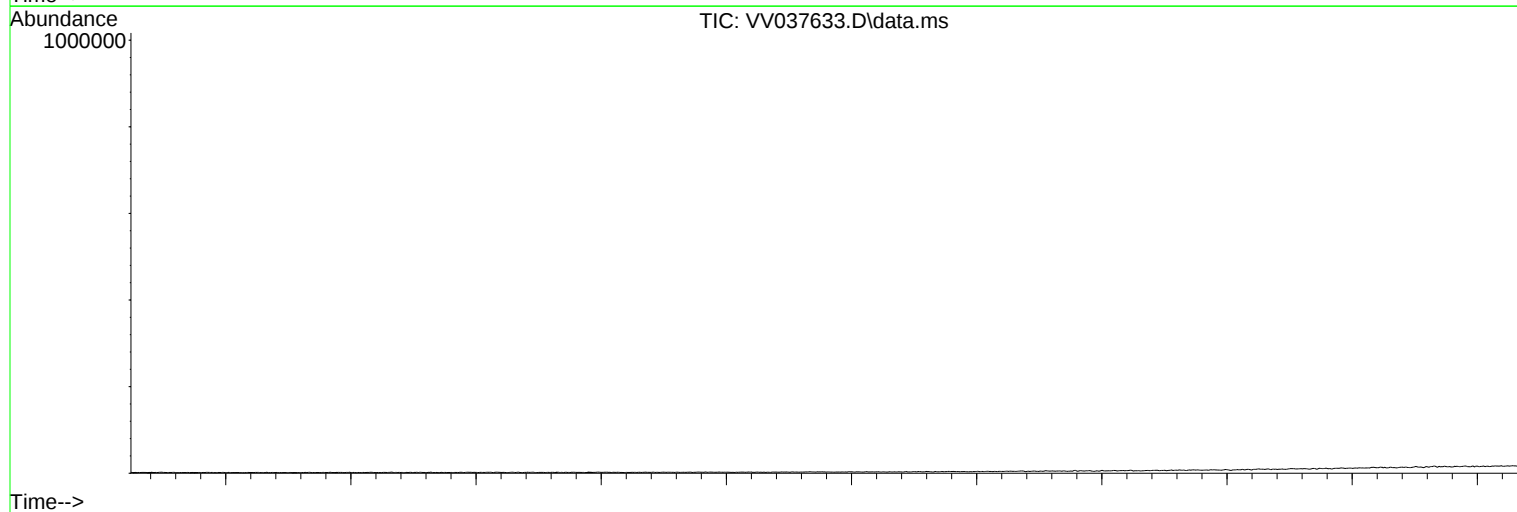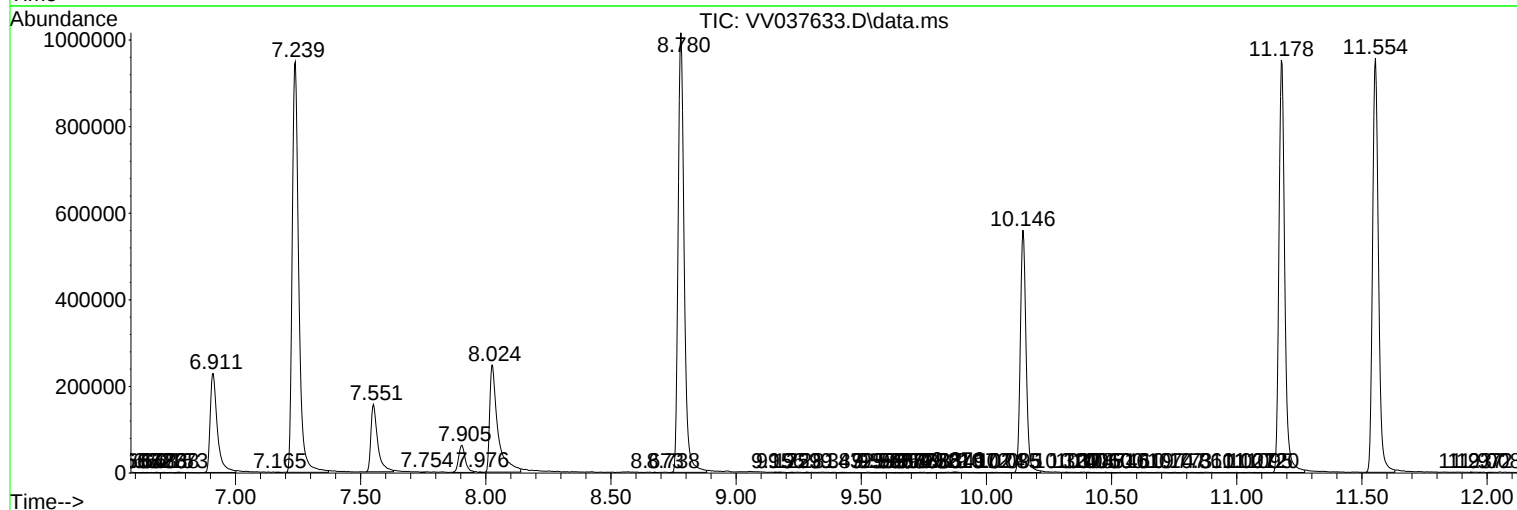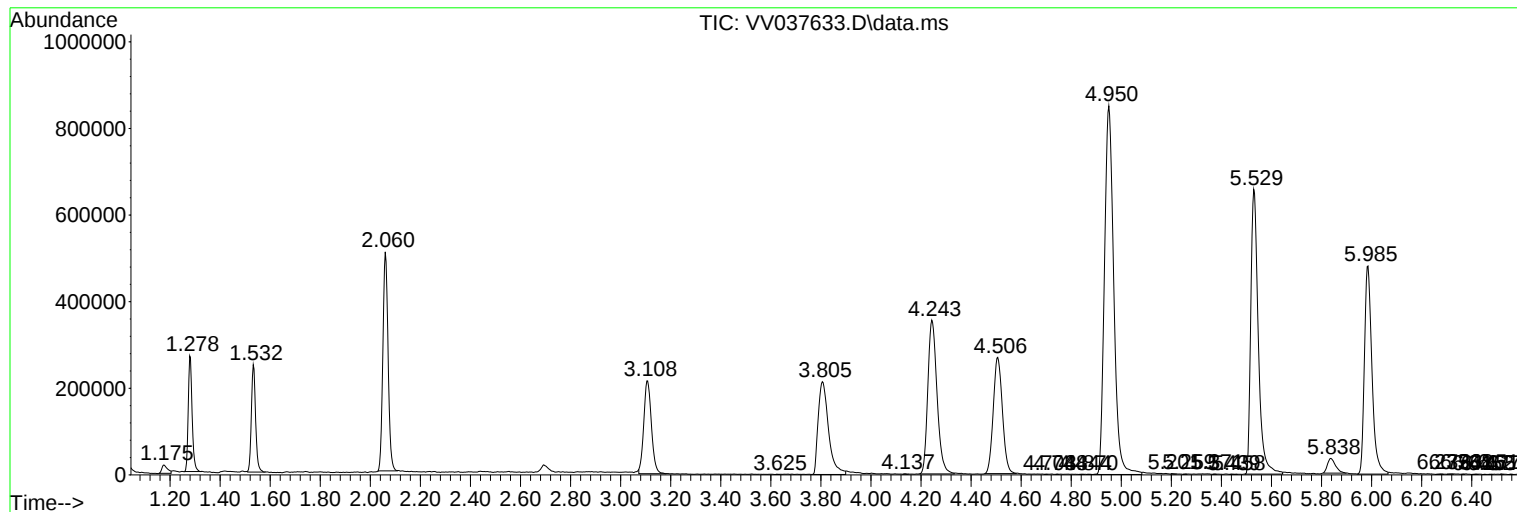

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037633.D
Acq On : 28 Sep 2024 01:18
Operator : SY/MD
Sample : P4185-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY062

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037633.D
Acq On : 28 Sep 2024 01:18
Operator : SY/MD
Sample : P4185-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY062

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc