

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037634.D
 Acq On : 28 Sep 2024 01:40
 Operator : SY/MD
 Sample : P4185-15
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY063

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037634.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	53	rBV	16896	29705	1.36%	0.168%
2	1.281	68	75	88	rVB	273558	292381	13.35%	1.655%
3	1.532	146	153	169	rVB	242224	287384	13.12%	1.627%
4	2.059	308	317	340	rVB	502320	738849	33.73%	4.183%
5	3.108	632	643	662	rVB	220851	456502	20.84%	2.585%
6	3.442	744	747	751	rBV4	558	368	0.02%	0.002%
7	3.567	783	786	790	rBV3	615	439	0.02%	0.002%
8	3.619	800	802	804	rBV	280	141	0.01%	0.001%
9	3.651	810	812	815	rBV2	484	301	0.01%	0.002%
10	3.664	815	816	820	rVB	373	120	0.01%	0.001%
11	3.728	832	836	837	rBV2	581	362	0.02%	0.002%
12	3.805	846	860	890	rBV2	217276	625094	28.54%	3.539%
13	4.172	970	974	976	rBV3	695	639	0.03%	0.004%
14	4.243	982	996	1025	rBV	360625	903826	41.26%	5.117%
15	4.506	1062	1078	1104	rBV2	275289	701083	32.01%	3.970%
16	4.741	1149	1151	1154	rVB3	572	304	0.01%	0.002%
17	4.764	1156	1158	1160	rVV3	572	221	0.01%	0.001%
18	4.828	1176	1178	1183	rVB2	603	382	0.02%	0.002%
19	4.857	1183	1187	1189	rBV2	639	417	0.02%	0.002%
20	4.886	1194	1196	1197	rBV2	471	207	0.01%	0.001%
21	4.950	1201	1216	1251	rBV2	852590	2190513	100.00%	12.403%
22	5.461	1372	1375	1378	rBV2	414	296	0.01%	0.002%
23	5.529	1385	1396	1425	rBV	673277	1384172	63.19%	7.837%
24	5.837	1481	1492	1508	rBV6	34890	82911	3.79%	0.469%
25	5.985	1526	1538	1569	rBV	478472	1002408	45.76%	5.676%
26	6.246	1616	1619	1622	rBV3	887	669	0.03%	0.004%
27	6.281	1628	1630	1634	rVB3	1245	673	0.03%	0.004%
28	6.300	1634	1636	1638	rBV3	1062	720	0.03%	0.004%
29	6.345	1646	1650	1652	rBV4	809	582	0.03%	0.003%
30	6.519	1702	1704	1705	rBV	468	194	0.01%	0.001%
31	6.558	1711	1716	1717	rBV4	597	509	0.02%	0.003%
32	6.583	1722	1724	1727	rBV3	556	356	0.02%	0.002%
33	6.673	1748	1752	1754	rBV2	653	479	0.02%	0.003%
34	6.702	1759	1761	1762	rBV	320	117	0.01%	0.001%
35	6.754	1775	1777	1782	rVB5	901	647	0.03%	0.004%
36	6.776	1782	1784	1785	rBV	550	169	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037634.D
 Acq On : 28 Sep 2024 01:40
 Operator : SY/MD
 Sample : P4185-15
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY063

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.792	1787	1789	1790	rBV	568	258	0.01%	0.001%
38	6.863	1804	1811	1815	rBV5	1139	1055	0.05%	0.006%
39	6.911	1815	1826	1858	rBV2	231025	457338	20.88%	2.589%
40	7.239	1916	1928	1954	rBV	961672	1715659	78.32%	9.714%
41	7.551	2016	2025	2050	rBV2	152774	291983	13.33%	1.653%
42	7.860	2116	2121	2124	rBV5	1200	1182	0.05%	0.007%
43	7.905	2124	2135	2151	rVV4	63457	115437	5.27%	0.654%
44	8.027	2164	2173	2212	rBV2	245618	564293	25.76%	3.195%
45	8.734	2390	2393	2396	rBV2	1005	837	0.04%	0.005%
46	8.779	2396	2407	2436	rBV	1057203	1738704	79.37%	9.845%
47	9.323	2574	2576	2578	rBV3	565	217	0.01%	0.001%
48	9.406	2598	2602	2607	rBV3	609	524	0.02%	0.003%
49	9.448	2613	2615	2617	rBV3	826	411	0.02%	0.002%
50	9.480	2622	2625	2630	rVV6	968	700	0.03%	0.004%
51	9.503	2630	2632	2635	rVB2	1013	455	0.02%	0.003%
52	9.606	2662	2664	2669	rBV3	742	622	0.03%	0.004%
53	9.657	2675	2680	2683	rBV3	864	894	0.04%	0.005%
54	9.738	2703	2705	2708	rBV2	303	162	0.01%	0.001%
55	9.750	2708	2709	2712	rVB2	985	382	0.02%	0.002%
56	9.773	2712	2716	2718	rBV3	581	374	0.02%	0.002%
57	9.796	2718	2723	2727	rBV3	714	675	0.03%	0.004%
58	9.834	2731	2735	2737	rVB3	500	317	0.01%	0.002%
59	9.847	2737	2739	2740	rBV	680	190	0.01%	0.001%
60	9.863	2740	2744	2745	rBV2	889	543	0.02%	0.003%
61	9.947	2767	2770	2773	rBV2	642	545	0.02%	0.003%
62	9.992	2781	2784	2785	rBV2	285	149	0.01%	0.001%
63	10.021	2791	2793	2794	rBV	397	158	0.01%	0.001%
64	10.043	2797	2800	2801	rBV3	309	165	0.01%	0.001%
65	10.101	2815	2818	2819	rBV2	903	464	0.02%	0.003%
66	10.146	2821	2832	2856	rVV	564027	886445	40.47%	5.019%
67	10.381	2903	2905	2907	rBV3	487	296	0.01%	0.002%
68	10.413	2913	2915	2917	rBV2	739	289	0.01%	0.002%
69	10.503	2941	2943	2945	rBV	329	176	0.01%	0.001%
70	10.586	2967	2969	2972	rVB3	474	224	0.01%	0.001%
71	10.603	2972	2974	2975	rBV	365	137	0.01%	0.001%
72	10.677	2995	2997	3000	rBV3	822	420	0.02%	0.002%
73	10.709	3005	3007	3010	rVB2	535	217	0.01%	0.001%
74	10.734	3013	3015	3016	rBV2	484	222	0.01%	0.001%
75	10.767	3022	3025	3028	rBV2	528	396	0.02%	0.002%
76	10.789	3028	3032	3034	rBV3	907	594	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037634.D
 Acq On : 28 Sep 2024 01:40
 Operator : SY/MD
 Sample : P4185-15
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY063

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.847	3049	3050	3052	rBV	444	161	0.01%	0.001%
78	10.869	3054	3057	3062	rBV3	1300	1094	0.05%	0.006%
79	10.924	3067	3074	3077	rBV3	762	764	0.03%	0.004%
80	10.998	3093	3097	3100	rBV5	658	621	0.03%	0.004%
81	11.014	3100	3102	3104	rVV	702	306	0.01%	0.002%
82	11.037	3107	3109	3112	rVB2	1017	458	0.02%	0.003%
83	11.053	3112	3114	3115	rBV2	369	175	0.01%	0.001%
84	11.085	3119	3124	3125	rBV3	711	661	0.03%	0.004%
85	11.178	3141	3153	3190	rBV	980636	1592078	72.68%	9.014%
86	11.554	3258	3270	3300	rBV	966770	1571072	71.72%	8.895%
87	12.197	3468	3470	3472	rBV2	681	202	0.01%	0.001%
88	12.229	3478	3480	3481	rBV	761	325	0.01%	0.002%
89	12.275	3489	3494	3495	rBV3	588	513	0.02%	0.003%
90	12.320	3506	3508	3511	rBV2	561	398	0.02%	0.002%
91	12.493	3560	3562	3564	rVB2	1018	404	0.02%	0.002%
92	12.590	3590	3592	3594	rBV3	869	459	0.02%	0.003%
93	12.644	3606	3609	3611	rBV2	760	438	0.02%	0.002%
94	12.779	3649	3651	3653	rBV2	498	253	0.01%	0.001%
95	12.873	3677	3680	3683	rBV3	768	623	0.03%	0.004%
96	13.123	3755	3758	3760	rBV2	295	186	0.01%	0.001%
97	13.432	3851	3854	3855	rBV	717	417	0.02%	0.002%
98	13.580	3898	3900	3906	rBV4	823	771	0.04%	0.004%
99	13.699	3935	3937	3939	rBV2	882	457	0.02%	0.003%
100	14.207	4094	4095	4099	rBV3	687	456	0.02%	0.003%

Sum of corrected areas: 17661541




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037634.D
Acq On : 28 Sep 2024 01:40
Operator : SY/MD
Sample : P4185-15
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY063

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

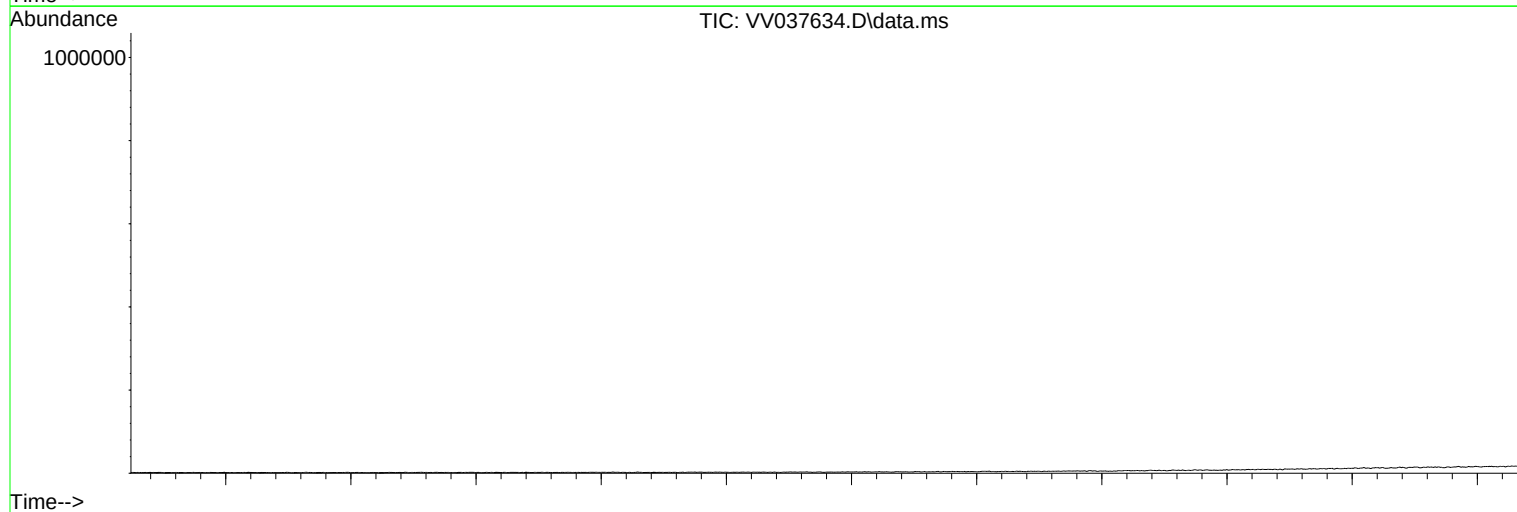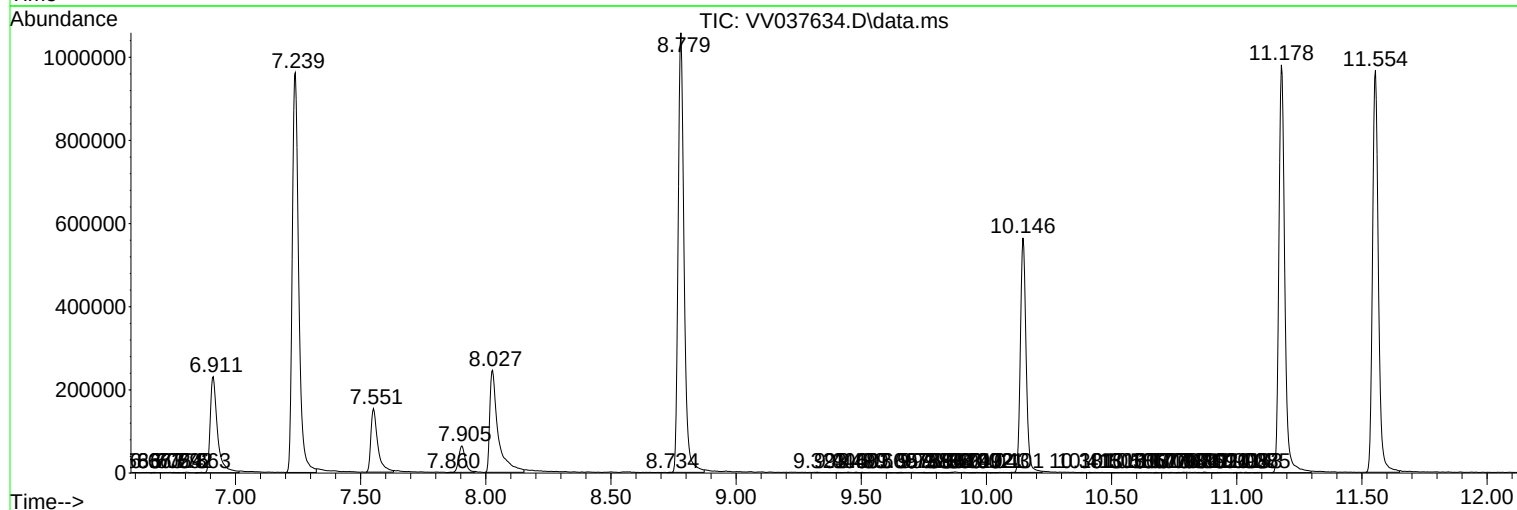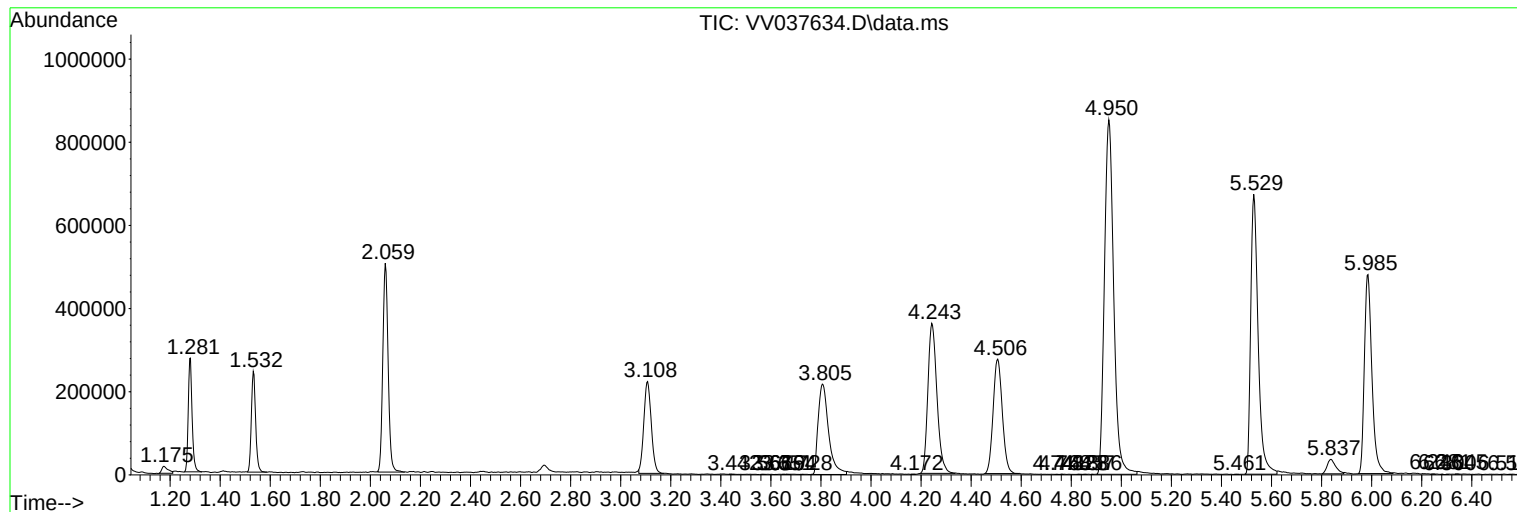

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037634.D
Acq On : 28 Sep 2024 01:40
Operator : SY/MD
Sample : P4185-15
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY063

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037634.D
Acq On : 28 Sep 2024 01:40
Operator : SY/MD
Sample : P4185-15
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY063

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------