

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037637.D
 Acq On : 28 Sep 2024 02:44
 Operator : SY/MD
 Sample : P4185-20
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY073

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037637.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	37	42	53	rBV	15173	25959	0.11%	0.044%
2	1.285	68	76	93	rBV2	1539410	1711721	7.05%	2.929%
3	1.548	146	158	180	rVB2	698558	1077088	4.44%	1.843%
4	2.063	308	318	342	rVB3	585696	937976	3.86%	1.605%
5	2.690	503	513	536	rVB	449958	769348	3.17%	1.317%
6	3.104	626	642	672	rVB	5679015	11545804	47.57%	19.759%
7	3.400	732	734	737	rBV3	870	327	0.00%	0.001%
8	3.503	763	766	768	rVB2	1122	597	0.00%	0.001%
9	3.526	768	773	780	rBV6	915	1069	0.00%	0.002%
10	3.558	780	783	785	rBV3	585	334	0.00%	0.001%
11	3.593	792	794	797	rBV2	527	237	0.00%	0.000%
12	3.709	826	830	832	rBV3	1360	1051	0.00%	0.002%
13	3.805	843	860	905	rBV	10497375	24270909	100.00%	41.537%
14	4.243	983	996	1025	rVB	361493	920612	3.79%	1.576%
15	4.506	1061	1078	1100	rBV2	329718	829475	3.42%	1.420%
16	4.793	1164	1167	1168	rBV3	536	293	0.00%	0.001%
17	4.950	1201	1216	1241	rBV2	886111	2369690	9.76%	4.055%
18	5.465	1372	1376	1380	rBV4	1163	1191	0.00%	0.002%
19	5.529	1385	1396	1435	rBV	682725	1416065	5.83%	2.423%
20	5.828	1477	1489	1521	rBV	818557	1642338	6.77%	2.811%
21	5.985	1527	1538	1571	rVB	496916	1022469	4.21%	1.750%
22	6.294	1632	1634	1635	rBV	618	234	0.00%	0.000%
23	6.484	1691	1693	1695	rBV2	815	252	0.00%	0.000%
24	6.580	1721	1723	1725	rVB2	593	231	0.00%	0.000%
25	6.609	1730	1732	1735	rBV3	365	248	0.00%	0.000%
26	6.645	1741	1743	1744	rBV	475	219	0.00%	0.000%
27	6.735	1769	1771	1774	rVB3	461	265	0.00%	0.000%
28	6.757	1774	1778	1779	rBV3	492	324	0.00%	0.001%
29	6.799	1789	1791	1793	rBV	455	277	0.00%	0.000%
30	6.841	1802	1804	1806	rBV	400	252	0.00%	0.000%
31	6.908	1813	1825	1854	rBV	239222	472204	1.95%	0.808%
32	7.239	1917	1928	1958	rBV	984011	1766520	7.28%	3.023%
33	7.551	2016	2025	2052	rBV	157467	301599	1.24%	0.516%
34	7.776	2088	2095	2109	rVB3	19056	34303	0.14%	0.059%
35	7.898	2121	2133	2153	rBV	475461	811949	3.35%	1.390%
36	8.027	2164	2173	2231	rVB2	250125	567992	2.34%	0.972%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037637.D
 Acq On : 28 Sep 2024 02:44
 Operator : SY/MD
 Sample : P4185-20
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY073

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	8.487	2313	2316	2319	rBV5	789	769	0.00%	0.001%
38	8.532	2328	2330	2333	rBV3	975	829	0.00%	0.001%
39	8.702	2380	2383	2385	rBV3	837	477	0.00%	0.001%
40	8.738	2391	2394	2395	rBV2	489	241	0.00%	0.000%
41	8.779	2395	2407	2429	rBV	1060140	1755954	7.23%	3.005%
42	9.185	2529	2533	2536	rBV3	957	973	0.00%	0.002%
43	9.226	2544	2546	2548	rBV2	572	323	0.00%	0.001%
44	9.259	2553	2556	2557	rBV2	535	246	0.00%	0.000%
45	9.339	2579	2581	2585	rVB4	548	323	0.00%	0.001%
46	9.361	2585	2588	2590	rBV3	664	452	0.00%	0.001%
47	9.397	2597	2599	2603	rVB5	735	546	0.00%	0.001%
48	9.487	2625	2627	2630	rBV3	789	439	0.00%	0.001%
49	9.551	2643	2647	2650	rBV4	602	531	0.00%	0.001%
50	9.728	2698	2702	2704	rBV4	575	408	0.00%	0.001%
51	9.773	2713	2716	2719	rBV3	607	453	0.00%	0.001%
52	9.821	2725	2731	2735	rVB4	726	782	0.00%	0.001%
53	9.869	2735	2746	2749	rBV6	1360	1890	0.01%	0.003%
54	9.969	2775	2777	2779	rVB2	577	242	0.00%	0.000%
55	9.985	2779	2782	2784	rBV3	365	270	0.00%	0.000%
56	10.014	2789	2791	2794	rBV2	498	335	0.00%	0.001%
57	10.088	2812	2814	2817	rBV3	402	313	0.00%	0.001%
58	10.146	2820	2832	2851	rBV	571862	915011	3.77%	1.566%
59	10.352	2894	2896	2900	rBV	519	319	0.00%	0.001%
60	10.374	2900	2903	2906	rBV3	1021	699	0.00%	0.001%
61	10.426	2916	2919	2924	rVB4	826	649	0.00%	0.001%
62	10.445	2924	2925	2927	rBV	562	289	0.00%	0.000%
63	10.464	2930	2931	2933	rVV	657	233	0.00%	0.000%
64	10.480	2933	2936	2939	rVV2	848	653	0.00%	0.001%
65	10.500	2939	2942	2946	rVB5	801	534	0.00%	0.001%
66	10.532	2948	2952	2955	rVB3	600	415	0.00%	0.001%
67	10.651	2986	2989	2994	rVB4	1149	883	0.00%	0.002%
68	10.680	2994	2998	2999	rBV2	685	457	0.00%	0.001%
69	10.779	3024	3029	3030	rBV2	926	568	0.00%	0.001%
70	10.808	3036	3038	3040	rBV2	548	249	0.00%	0.000%
71	10.824	3040	3043	3046	rBV2	599	467	0.00%	0.001%
72	10.931	3073	3076	3078	rBV3	449	257	0.00%	0.000%
73	10.982	3089	3092	3095	rBV	652	415	0.00%	0.001%
74	10.998	3095	3097	3100	rVV3	694	445	0.00%	0.001%
75	11.072	3116	3120	3122	rBV4	1049	725	0.00%	0.001%
76	11.127	3132	3137	3139	rBV3	622	519	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037637.D
 Acq On : 28 Sep 2024 02:44
 Operator : SY/MD
 Sample : P4185-20
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY073

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	11.178	3142	3153	3186	rBV	993343	1612960	6.65%	2.760%
78	11.554	3258	3270	3295	rBV	1007446	1617304	6.66%	2.768%
79	12.175	3460	3463	3466	rBV4	542	329	0.00%	0.001%
80	12.213	3472	3475	3479	rBV4	745	562	0.00%	0.001%
81	12.268	3488	3492	3494	rBV2	717	563	0.00%	0.001%
82	12.303	3500	3503	3505	rBV2	724	313	0.00%	0.001%
83	12.448	3545	3548	3550	rBV	502	353	0.00%	0.001%
84	12.538	3573	3576	3577	rBV2	438	218	0.00%	0.000%
85	12.631	3603	3605	3608	rVB2	900	456	0.00%	0.001%
86	12.686	3617	3622	3623	rBV4	833	512	0.00%	0.001%
87	12.702	3625	3627	3632	rVV4	651	537	0.00%	0.001%
88	12.757	3640	3644	3646	rBV2	776	694	0.00%	0.001%
89	12.789	3652	3654	3657	rVB2	702	397	0.00%	0.001%
90	12.853	3672	3674	3676	rBV2	704	321	0.00%	0.001%
91	13.078	3741	3744	3746	rBV2	514	295	0.00%	0.001%
92	13.149	3764	3766	3771	rBV3	907	710	0.00%	0.001%
93	13.217	3784	3787	3790	rBV3	1027	824	0.00%	0.001%
94	13.252	3796	3798	3801	rBV2	759	507	0.00%	0.001%
95	13.487	3868	3871	3874	rBV	614	458	0.00%	0.001%
96	13.516	3878	3880	3882	rBV2	1052	635	0.00%	0.001%
97	13.557	3891	3893	3895	rBV	917	446	0.00%	0.001%
98	13.654	3921	3923	3925	rBV2	588	397	0.00%	0.001%
99	13.692	3932	3935	3937	rBV4	965	601	0.00%	0.001%
100	13.914	4002	4004	4005	rBV	512	264	0.00%	0.000%




Sum of corrected areas: 58432661

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037637.D
Acq On : 28 Sep 2024 02:44
Operator : SY/MD
Sample : P4185-20
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY073

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

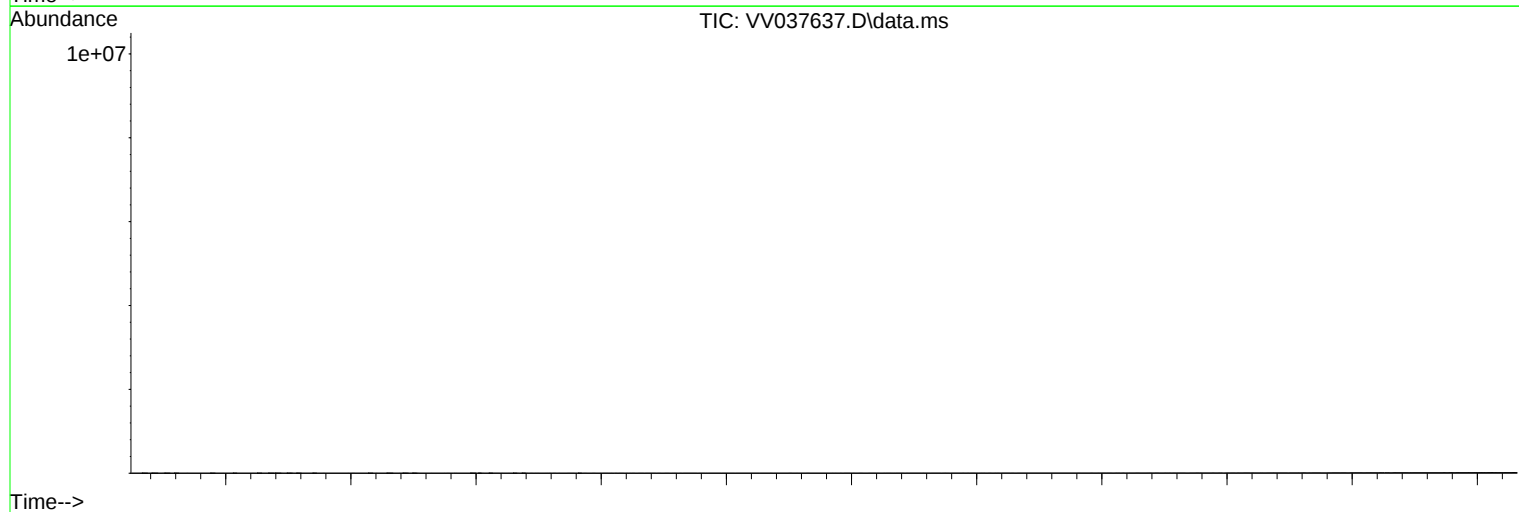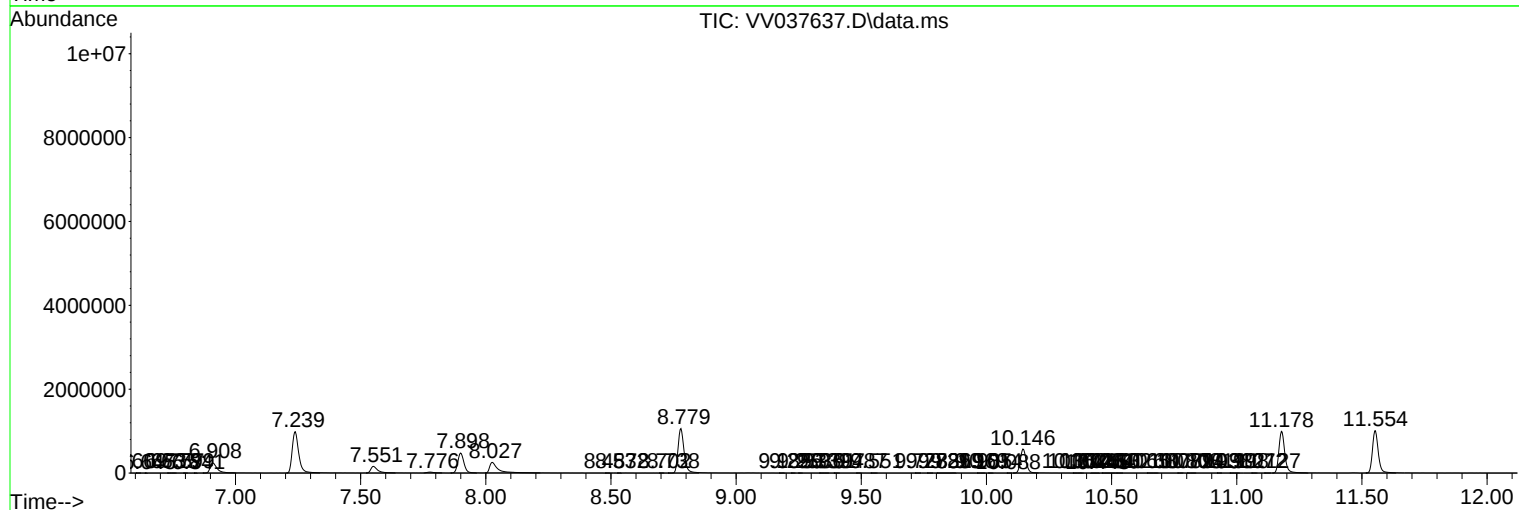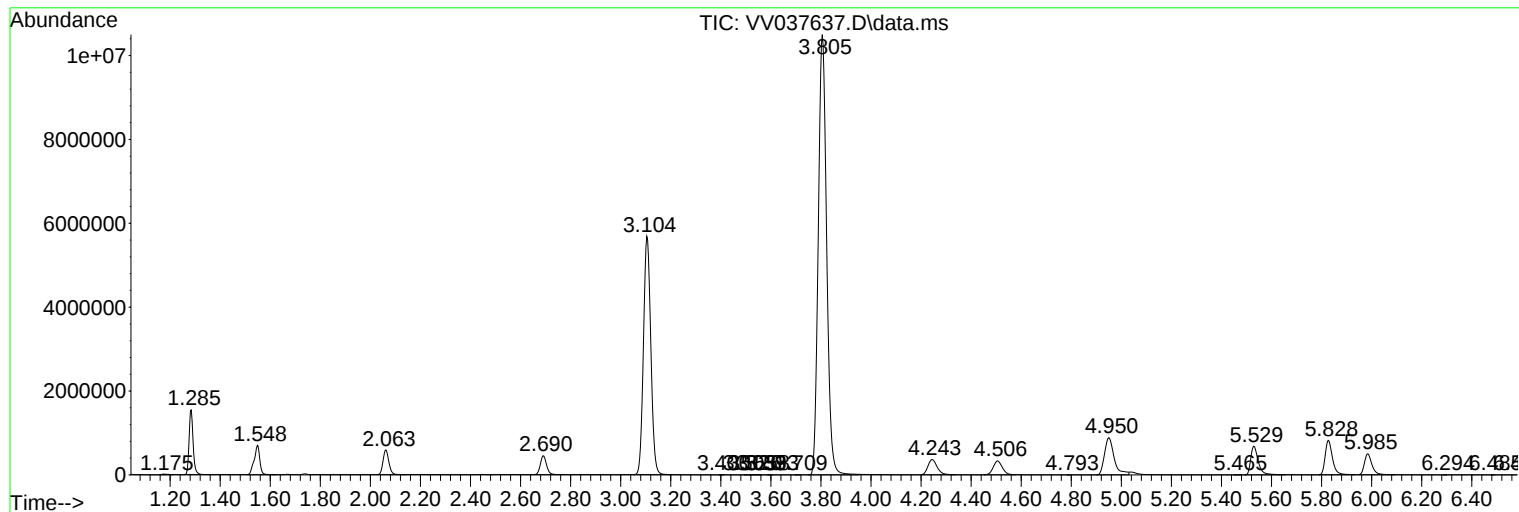

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037637.D
Acq On : 28 Sep 2024 02:44
Operator : SY/MD
Sample : P4185-20
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY073

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037637.D
Acq On : 28 Sep 2024 02:44
Operator : SY/MD
Sample : P4185-20
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY073

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
